



McKesson Radiology 12.2

# **DICOM CONFORMANCE STATEMENT**

**McKesson Technology Solutions**

**130 – 10711 Cambie Road, Richmond, BC, Canada V6X 3G5**

**Telephone: 604.279.5422 Toll-Free: 1-800-661-5885 Fax: 1.800.261.5432**

**<http://www.mckesson.com>**

DOCUMENT DESCRIPTION	
<b>Document Title</b>	McKesson Radiology™ 12.2 DICOM Conformance Statement
<b>Document Number and Revision Number</b>	2015-30991 Rev # 1.0
<b>Released</b>	This document is effective as of the last approval date

### Copyright notice

Copyright © 2015 McKesson Corporation and/or one of its subsidiaries. All Rights Reserved.

The document and the software are furnished under license and may not be reproduced in any form without the prior written consent of McKesson Corporation and/or one of its subsidiaries.

### Trademarks

McKesson Radiology™ and McKesson Radiology Station™ are trademarks of McKesson Corporation and/or one of its subsidiaries. All other brands and product names are registered trademarks or trademarks of their respective holders and are used only for reference, where specifically needed, without any intent to infringe.

All other product and company names may be trademarks or registered trademarks of their respective companies.

## Revision History

Document Version	Date	Description	Author
1.0	Oct 16, 2016	Changes listed in WPR. Final approval cycle	Wayne Tran

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 3

## 1. CONFORMANCE STATEMENT OVERVIEW

McKesson Radiology™ 12.2 is a self-contained, networked computer system used for receiving, archiving, and displaying diagnostic medical images. It is also capable of creating derived images using Multi-Planar Reconstruction (MPR). It can create DICOM Secondary Capture Image objects from documents scanned directly into McKesson Radiology. The MPR and Secondary Capture Image objects can both be exported via the Query/Retrieve or Storage Services. It can display DICOM Standard GSPS Text and graphic annotations and Presentation State information (i.e. Shutter, Display Area, VOILUT etc.) created by other DICOM compliant devices. It can also export internal (proprietary format) Text and graphic annotations and Presentation State information (i.e. Shutter, Display Area, VOILUT etc.) that are created by the McKesson Radiology System using standard DICOM GSPS SOP Instances (See 7.1.9).

For Shared Image Management (SIM) customers who want to DICOM archive their non-DICOM Cardiology files to a separate DICOM archive, McKesson Radiology™ 12.2 can create DICOM SOP instances for these non-DICOM files so they can be DICOM archive. DICOM Raw Data instances will be used to wrap file types<sup>20</sup> that are non pdf format. Encapsulated PDF instances will be used to wrap .pdf data file type. This allows these files to be sent and query/retrieved back from a separate DICOM archive.

McKesson Radiology™ 12.2 supports displaying information about CAD findings encoded in R2 and iCAD DICOM Mammography SR objects (See 7.1.12)

McKesson Radiology™ 12.2 includes the ability to import, send, query and retrieve, perform media import/export, and display Digital Breast Tomosynthesis (DBT) images and synthesized 2D MG images. Display of DBT images is only for 64-bit McKesson Radiology Station. A few of the functions include: scroll, power scroll, window/level, zoom, pan, annotate, creation of display protocols that support hanging of both 2D and DBT images and view DBT image data at different slice thicknesses to visualize anatomical regions of interest and calcifications in greater detail (slab DBT images - Single Plane Reconstruction (SPR) presentation of DBT volumes). Please consult with a McKesson Representative for a complete list of features that McKesson Radiology™ 12.2 supports for DBT images.

McKesson Radiology™ 12.2 needs to handle imaging data where the patient and study identifiers can be from multiple assigning authorities. With the addition of the IHE MIMA Multiple Identity Resolution option feature, McKesson Radiology™ 12.2 will be capable of exchanging the patient and study identifiers associated with the assigning authorities in a standard manner.

McKesson Radiology™ 12.2 supports Query based on ID for DICOM Objects by Representational State Transfer Services (QIDO-RS) to allow web based queries for studies, series and instances.

McKesson Radiology™ 12.2 supports Web Access to DICOM Persistent Objects by RESTful Services (WADO-RS) to allow web based retrieve for studies, series and instances.

The system conforms to the DICOM 3.0 standard<sup>1</sup> to allow the sharing of medical information with other digital imaging systems.

Table 1 provides an overview of the network services supported by McKesson Radiology™ 12.2.

**Table 1: Network Services**

DICOM SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	Yes
<b>Transfer</b>			
12-lead ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	Yes

<sup>1</sup> NEMA PS 3.1 - 3.20 (2014)

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 4

DICOM SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Ambulatory ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	Yes
Basic Voice Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	Yes
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	Yes
General Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.2	Yes	Yes
Arterial Pulse Waveform	1.2.840.10008.5.1.4.1.1.9.5.1	Yes	Yes
Respiratory Waveform	1.2.840.10008.5.1.4.1.1.9.6.1	Yes	Yes
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11	Yes	Yes
Comprehensive Structured Report	1.2.840.10008.5.1.4.1.1.88.33	Yes	Yes
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	Yes	Yes
Mammography CAD Structured Report	1.2.840.10008.5.1.4.1.1.88.50	Yes	Yes
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Yes	Yes
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Yes	Yes
Colon CAD SR Document	1.2.840.10008.5.1.4.1.1.88.69	Yes	Yes
Implantation Plan SR Document	1.2.840.10008.5.1.4.1.1.88.70	Yes	Yes
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes
Encapsulated CDA IOD	1.2.840.10008.5.1.4.1.1.104.2	Yes	Yes
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Yes	Yes
CT Image	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
Digital X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes
Digital X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes
Digital Mammography Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes
Digital Mammography Image (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes
Breast Tomosynthesis Image	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	Yes
Digital Intra-oral X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	Yes	Yes
Digital Intra-oral X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	Yes
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	Yes
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes
Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.2	Yes	Yes
Pseudo-Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.3	Yes	Yes
Blending Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.4	Yes	Yes
XA/XRF Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.5	Yes	Yes
Hardcopy Color Image	1.2.840.10008.5.1.1.30	Yes	Yes
Hardcopy Grayscale Image	1.2.840.10008.5.1.1.29	Yes	Yes
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	Yes
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	Yes	Yes
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes
MR Image	1.2.840.10008.5.1.4.1.1.4	Yes	Yes
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	Yes
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	Yes	Yes
Nuclear Medicine Image (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	Yes
Positron Emission Tomography Image	1.2.840.10008.5.1.4.1.1.128	Yes	Yes
Raw Data	1.2.840.10008.5.1.4.1.1.66	Yes	Yes
Spatial Registration	1.2.840.10008.5.1.4.1.1.66.1	Yes	Yes
Spatial Fiducials	1.2.840.10008.5.1.4.1.1.66.2	Yes	Yes
Deformable Spatial Registration	1.2.840.10008.5.1.4.1.1.66.3	Yes	Yes
Segmentation	1.2.840.10008.5.1.4.1.1.66.4	Yes	Yes

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 5

DICOM SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Surface Segmentation	1.2.840.10008.5.1.4.1.1.66.5	Yes	Yes
Real World Value Mapping	1.2.840.10008.5.1.4.1.1.67	Yes	Yes
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Yes	Yes
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Yes	Yes
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Yes	Yes
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Yes	Yes
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Yes	Yes
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Yes	Yes
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	Yes
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	Yes
RT Beams Delivery Instruction	1.2.840.10008.5.1.4.34.7	Yes	Yes
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Stand-alone Curve	1.2.840.10008.5.1.4.1.1.9	Yes	Yes
Stand-alone Modality LUT	1.2.840.10008.5.1.4.1.1.10	Yes	Yes
Stand-alone Overlay	1.2.840.10008.5.1.4.1.1.8	Yes	Yes
Stand-alone VOI LUT	1.2.840.10008.5.1.4.1.1.11	Yes	Yes
Standalone PET Curve	1.2.840.10008.5.1.4.1.1.129	Yes	Yes
Stored Print	1.2.840.10008.5.1.1.27	Yes	Yes
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes
Ultrasound Image (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	Yes
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes
Ultrasound Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	Yes
VL Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	Yes
VL Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	Yes
VL Slide-Coordinates Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	Yes
VL Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	Yes
VL Image (Retired)	1.2.840.10008.5.1.4.1.1.77.1	Yes	Yes
VL Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.77.2	Yes	Yes
Video Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1.1	Yes	Yes
Video Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2.1	Yes	Yes
Video Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4.1	Yes	Yes
Ophthalmic Photography 8 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.1	Yes	Yes
Ophthalmic Photography 16 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.2	Yes	Yes
Stereometric Relationship	1.2.840.10008.5.1.4.1.1.77.1.5.3	Yes	Yes
X-Ray Angiographic Bi-Plane Image (retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	Yes
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes
X-Ray Radiation Dose Structured Report	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes
Lensometry Measurements	1.2.840.10008.5.1.4.1.1.78.1	Yes	Yes
Autorefraction Measurements	1.2.840.10008.5.1.4.1.1.78.2	Yes	Yes
Keratometry Measurements	1.2.840.10008.5.1.4.1.1.78.3	Yes	Yes
Subjective Refraction Measurements	1.2.840.10008.5.1.4.1.1.78.4	Yes	Yes
Visual Acuity Measurements	1.2.840.10008.5.1.4.1.1.78.5	Yes	Yes
Spectacle Prescription Report	1.2.840.10008.5.1.4.1.1.78.6	Yes	Yes
Ophthalmic Axial Measurements	1.2.840.10008.5.1.4.1.1.78.7	Yes	Yes
Intraocular Lens Calculations	1.2.840.10008.5.1.4.1.1.78.8	Yes	Yes
Macular Grid Thickness and Volume Report	1.2.840.10008.5.1.4.1.1.79.1	Yes	Yes
Ophthalmic Visual Field Static Perimetry Measurements	1.2.840.10008.5.1.4.1.1.80.1	Yes	Yes

DICOM SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Basic Structured Display IOD	1.2.840.10008.5.1.4.1.1.131	Yes	Yes
Generic Implant Template	1.2.840.10008.5.1.4.43.1	Yes	Yes
Implant Assembly Template	1.2.840.10008.5.1.4.44.1	Yes	Yes
Implant Template Group	1.2.840.10008.5.1.4.45.1	Yes	Yes
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	Yes	Yes
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	Yes	Yes
Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	Yes	Yes
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Yes	Yes
Radiopharmaceutical Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.68	Yes	Yes
<b>Query/Retrieve</b>			
Patient Root Q/R – FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	Yes
Patient Root Q/R – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes
Study Root Q/R – FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Study Root Q/R – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Patient Study Only – FIND	1.2.840.10008.5.1.4.1.2.3.1	Yes	Yes
Patient Study Only – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Yes	Yes
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	Yes
Modality Worklist	1.2.840.10008.5.1.4.31	Yes	Yes
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Yes	Yes
<b>Print Management</b>			
Basic Grayscale Print Management	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management	1.2.840.10008.5.1.1.18	Yes	No

NOTE1: Relational Queries are not supported either as an SCU or SCP.

Table 2 provides an overview of the Media Storage Application Profiles supported by McKesson Radiology™ 12.2.

**Table 2: Media Storage Application Profiles**

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
<b>Compact Disk – Recordable</b>		
General Purpose CD-R	Yes	Yes
Ultrasound Image Display Single Frame	Yes	Yes
Ultrasound Spatial Calibration Single Frame	Yes	Yes
Ultrasound Combined Calibration Single Frame	Yes	Yes
Ultrasound Image Display Single and Multi-Frame	Yes	Yes
Ultrasound Spatial Calibration Single and Multi-Frame	Yes	Yes
Ultrasound Combined Calibration Single and Multi-Frame	Yes	Yes

NOTE1: For the system to act as an FSC or FSU of the STD-GEN-CD Application Profile it must be equipped with the necessary hardware option for writing to CD media. This is not a standard feature of all McKesson Radiology™ systems. McKesson Radiology™ systems can also support these Ultrasound Application Profiles for MOD media if equipped with the necessary hardware.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 7

**Table 3: QIDO-RS and WADO-RS NETWORK SERVICES**

Network Service	User of Service (Client)	Provider of Service (Server)
<b>Query by ID for DICOM Objects (QIDO)</b>		
QIDO-RS – Search for Studies	No	Yes
QIDO-RS – Search for Series	No	Yes
QIDO-RS – Search for Instances	No	Yes
<b>Web Access to DICOM Objects (WADO)</b>		
WADO – RS – Retrieve Study	No	Yes
WADO – RS – Retrieve Series	No	Yes
WADO – RS – Retrieve Instance	No	Yes
WADO – RS – Retrieve Frames	No	Yes
WADO – RS – Retrieve BulkData	No	Yes
WADO – RS – Retrieve Metadata	No	Yes

## 1.1 DICOM SOP Classes supported for Display

McKesson Radiology Station™ 12.2 as a multi-modality diagnostic medical workstation shall support the display of DICOM SOP Classes that are conforming to the DICOM 3.0 standard. However, McKesson Radiology Station™ 12.2 cannot actually support the display of all of the Composite SOP Classes listed in Table 1. Please refer to Table 181: “Supported Composite Image SOP Classes for Display” and Table 182: “Unsupported Composite SOP Classes for Display” for the SOP Classes in the two sets.



## CONTENTS

<b>1. CONFORMANCE STATEMENT OVERVIEW .....</b>	<b>3</b>
<b>1.1 DICOM SOP Classes supported for Display .....</b>	<b>7</b>
<b>2. INTRODUCTION.....</b>	<b>16</b>
<b>2.1 AUDIENCE .....</b>	<b>16</b>
<b>2.2 REMARKS .....</b>	<b>16</b>
<b>2.3 DEFINITIONS, TERMS AND ABBREVIATIONS.....</b>	<b>16</b>
<b>3. NETWORKING .....</b>	<b>16</b>
<b>3.1 Implementation Model.....</b>	<b>16</b>
<b>3.1.1 Application Data Flow Diagram .....</b>	<b>16</b>
<b>3.1.2 Functional Definitions of Application Entities.....</b>	<b>21</b>
<b>3.1.2.1 Sender AE .....</b>	<b>21</b>
<b>3.1.2.2 Importer AE .....</b>	<b>21</b>
<b>3.1.2.3 Query/Retrieve Server AE .....</b>	<b>21</b>
<b>3.1.2.4 Query/Retrieve Client AE .....</b>	<b>21</b>
<b>3.1.2.5 Modality Worklist Client AE .....</b>	<b>22</b>
<b>3.1.2.6 Print Management AE.....</b>	<b>22</b>
<b>3.1.2.7 External Notifier AE .....</b>	<b>22</b>
<b>3.1.2.8 Event Handler AE.....</b>	<b>22</b>
<b>3.1.2.9 Storage Commitment Client AE .....</b>	<b>22</b>
<b>3.1.2.10 QIDO-RS Service Provider .....</b>	<b>22</b>
<b>3.1.2.11 WADO-RS Service Provider .....</b>	<b>22</b>
<b>3.1.3 Sequencing of Real-World Activities.....</b>	<b>22</b>
<b>3.2 AE Specifications .....</b>	<b>24</b>
<b>3.2.1 Sender AE Specification .....</b>	<b>24</b>
<b>3.2.1.1 SOP Classes .....</b>	<b>24</b>
<b>3.2.1.2 Association Establishment Policies.....</b>	<b>26</b>
<b>3.2.1.2.1 General.....</b>	<b>26</b>
<b>3.2.1.2.2 Number of Associations .....</b>	<b>27</b>
<b>3.2.1.2.3 Asynchronous Nature .....</b>	<b>27</b>
<b>3.2.1.2.4 Implementation Identifying Information .....</b>	<b>27</b>
<b>3.2.1.3 Association Initiation Policy.....</b>	<b>27</b>
<b>3.2.1.3.1 Activity – User Requests Transmission of Images .....</b>	<b>27</b>
<b>3.2.1.3.1.1 Description and Sequencing of Activity.....</b>	<b>27</b>
<b>3.2.1.3.1.2 Proposed Presentation Contexts.....</b>	<b>27</b>
<b>3.2.1.3.1.3 SOP Specific Conformance as an Association Requestor .....</b>	<b>28</b>
<b>3.2.1.3.1.3.1 SOP Specific Conformance – Storage .....</b>	<b>28</b>
<b>3.2.1.3.1.3.2 Association Requestor Communication Failure Behavior .....</b>	<b>29</b>
<b>3.2.1.4 Association Acceptance Policy .....</b>	<b>30</b>
<b>3.2.2 Importer AE Specification .....</b>	<b>30</b>

<b>3.2.2.1</b>	<b>SOP Classes .....</b>	<b>30</b>
<b>3.2.2.2</b>	<b>Association Establishment Policies.....</b>	<b>33</b>
3.2.2.2.1	General.....	33
3.2.2.2.2	Number of Associations .....	33
3.2.2.2.3	Asynchronous Nature .....	33
3.2.2.2.4	Implementation Identifying Information .....	33
<b>3.2.2.3</b>	<b>Association Initiation Policies .....</b>	<b>33</b>
3.2.2.3.1	Activity – Require New Association for Storage Commitment .....	33
3.2.2.3.1.1	Description and Sequencing of Activity.....	34
3.2.2.3.1.2	Proposed Presentation Contexts.....	35
3.2.2.3.1.3	SOP Specific Conformance as an Association Requestor .....	35
3.2.2.3.1.3.1	SOP Specific Conformance - Storage Commitment .....	35
3.2.2.3.1.3.2	Association Requestor Communication Failure Behavior .....	36
3.2.2.3.4	Association Acceptance Policy .....	36
3.2.2.3.4.1	Activity – Receive Images and Storage Commitment Requests .....	36
3.2.2.3.4.1.1	Description and Sequencing of Activity.....	36
3.2.2.3.4.1.2	Accepted Presentation Contexts .....	38
3.2.2.3.4.1.3	SOP Specific Conformance as an Association Acceptor.....	38
3.2.2.3.4.1.3.1	SOP Specific Conformance – Verification .....	38
3.2.2.3.4.1.3.2	SOP Specific Conformance – Storage .....	38
3.2.2.3.4.1.3.3	SOP Specific Conformance – Storage Commitment .....	40
3.2.2.3.4.1.3.4	Association Acceptor Communication Failure Behavior .....	41
3.2.2.3.4.1.3.5	Presentation Context Acceptance Criterion .....	42
3.2.2.3.4.1.3.6	Transfer Syntax Selection Policies .....	42
<b>3.2.3</b>	<b>Query/Retrieve Server AE Specification .....</b>	<b>43</b>
3.2.3.1	SOP Classes .....	43
3.2.3.2	Association Establishment Policies.....	45
3.2.3.2.1	General.....	45
3.2.3.2.2	Number of Associations .....	46
3.2.3.2.3	Asynchronous Nature .....	46
3.2.3.2.4	Implementation Identifying Information .....	46
3.2.3.3	Association Initiation Policy .....	46
3.2.3.3.1	Activity – Remote AE requests the retrieval of images .....	46
3.2.3.3.1.1	Description and Sequencing of Activity.....	46
3.2.3.3.1.2	Proposed Presentation Contexts.....	47
3.2.3.3.1.3	SOP Specific Conformance as an Association Requestor .....	47
3.2.3.3.1.3.1	SOP Specific Conformance - Storage.....	47
3.2.3.3.1.3.2	Association Requestor Communication Failure Behavior .....	49
3.2.3.4	Association Acceptance Policy .....	49
3.2.3.4.1	Activity – External system queries McKesson Radiology™.....	49
3.2.3.4.1.1	Description and Sequencing of Activity.....	49
3.2.3.4.1.2	Accepted Presentation Contexts .....	51
3.2.3.4.1.3	SOP Specific Conformance as an Association Acceptor.....	52
3.2.3.4.1.3.1	SOP Specific Conformance – Verification .....	52
3.2.3.4.1.3.2	SOP Specific Conformance – Query (C-FIND).....	52
3.2.3.4.1.3.3	SOP Specific Conformance – Retrieve (C-MOVE).....	60

3.2.3.4.1.3.4	SOP Specific Conformance – Modality Worklist.....	62
3.2.3.4.1.3.5	Association Acceptor Communication Failure Behavior .....	65
3.2.3.4.1.3.6	Presentation Context Acceptance Criteria .....	65
3.2.3.4.1.3.7	Transfer Syntax Selection Policies .....	65
3.2.4	Query/Retrieve Client AE Specification.....	65
3.2.4.1	SOP Classes .....	65
3.2.4.2	Association Establishment Policies.....	66
3.2.4.2.1	General.....	66
3.2.4.2.2	Number of Associations .....	66
3.2.4.2.3	Asynchronous Nature .....	67
3.2.4.2.4	Implementation Identifying Information .....	67
3.2.4.3	Association Initiation Policy .....	67
3.2.4.3.1	Activity – Users Send Query Request to Remote AE.....	67
3.2.4.3.1.1	Description and Sequencing of Activity.....	67
3.2.4.3.1.2	Proposed Presentation Contexts.....	68
3.2.4.3.1.3	SOP Specific Conformance as an Association Requestor .....	69
3.2.4.3.1.3.1	SOP Specific Conformance – Query (C-FIND).....	69
3.2.4.3.1.3.2	SOP Specific Conformance - Retrieval (C-MOVE) .....	73
3.2.4.3.1.3.3	Association Requestor Communication Failure Behavior .....	75
3.2.4.4	Association Acceptance Policy .....	76
3.2.5	Modality Worklist Client AE Specification .....	76
3.2.5.1	SOP Classes .....	76
3.2.5.2	Association Establishment Policies.....	76
3.2.5.2.1	General.....	76
3.2.5.2.2	Number of Associations .....	76
3.2.5.2.3	Asynchronous Nature .....	77
3.2.5.2.4	Implementation Identifying Information .....	77
3.2.5.3	Association Initiation Policy .....	77
3.2.5.3.1	Activity – Update Modality Worklist .....	77
3.2.5.3.1.1	Description and Sequencing of Activity.....	77
3.2.5.3.1.2	Proposed Presentation Contexts.....	77
3.2.5.3.1.3	SOP Specific Conformance as an Association Requestor .....	78
3.2.5.3.1.3.1	SOP Specific Conformance - Modality Worklist.....	78
3.2.5.3.1.3.2	Association Requestor Communication Failure Behavior .....	79
3.2.5.4	Association Acceptance Policy .....	80
3.2.6	Print Management AE Specification.....	80
3.2.6.1	Association Establishment Policies.....	81
3.2.6.1.1	General.....	81
3.2.6.1.2	Number of Associations .....	81
3.2.6.1.3	Asynchronous Nature .....	81
3.2.6.1.4	Implementation Identifying Information .....	81
3.2.6.2	Association Initiation Policy .....	82
3.2.6.2.1	Activity – Images Sent to Printer.....	82
3.2.6.2.1.1	Description and Sequencing of Activity.....	82
3.2.6.2.1.2	Proposed Presentation Contexts.....	82
3.2.6.2.1.3	SOP Specific Conformance as an Association Requestor .....	83

3.2.6.2.1.3.1	SOP Specific Conformance - Printer SOP Class.....	83
3.2.6.2.1.3.2	SOP Specific Conformance - Film Session SOP Class .....	84
3.2.6.2.1.3.3	SOP Specific Conformance - Film Box SOP Class .....	85
3.2.6.2.1.3.4	SOP Specific Conformance - Basic Annotation SOP Class .....	88
3.2.6.2.1.3.5	SOP Specific Conformance - Image Box SOP Classes .....	91
3.2.6.2.1.3.6	Association Requestor Communication Failure Behavior .....	93
3.2.6.3	Association Acceptance Policy .....	93
3.2.7	External Notifier AE Specifications .....	93
3.2.7.1	Association Establishment Policies.....	94
3.2.7.1.1	General.....	94
3.2.7.1.2	Number of Associations .....	94
3.2.7.1.3	Asynchronous Nature .....	94
3.2.7.1.4	Implementation Identifying Information .....	94
3.2.7.2	Association Initiation Policy.....	94
3.2.7.2.1	Activity – Event Occurs that Requires Notification of a Remote AE ....	94
3.2.7.2.1.1	Description and Sequencing of Activity.....	94
3.2.7.2.1.2	Proposed Presentation Contexts.....	94
3.2.7.2.1.3	SOP Specific Conformance as an Association Requestor .....	95
3.2.7.2.1.3.1	SOP Specific Conformance - Modality Performed Procedure Step	95
3.2.7.2.1.3.2	Association Requestor Communication Failure Behavior .....	96
3.2.7.3	Association Acceptance Policy .....	97
3.2.8	Event Handler AE.....	97
3.2.8.1	Association Establishment Policies.....	97
3.2.8.1.1	General.....	97
3.2.8.1.2	Number of Associations .....	97
3.2.8.1.3	Asynchronous Nature .....	97
3.2.8.1.4	Implementation Identifying Information .....	97
3.2.8.2	Association Initiation Policies .....	98
3.2.8.3	Association Acceptance Policies .....	98
3.2.8.3.1	Activity – External system sends notification of an event .....	98
3.2.8.3.1.1	Description and Sequencing of Activity.....	98
3.2.8.3.1.2	Accepted Presentation Contexts .....	98
3.2.8.3.1.3	SOP Specific Conformance as an Association Acceptor.....	99
3.2.8.3.1.3.1	SOP Specific Conformance – Modality Performed Procedure	99
3.2.8.3.1.3.2	Association Acceptor Communication Failure Behavior .....	100
3.2.8.3.1.3.3	Presentation Context Acceptance Criterion .....	100
3.2.8.3.1.3.4	Transfer Syntax Selection Policies .....	100
3.2.9	Storage Commitment Client AE Specification.....	101
3.2.9.1	SOP Classes .....	101
3.2.9.2	Association Establishment Policies.....	101
3.2.9.2.1	General.....	101
3.2.9.2.2	Number of Associations .....	101
3.2.9.2.3	Asynchronous Nature .....	102
3.2.9.2.4	Implementation Identifying Information .....	102

<b>3.2.9.3 Association Initiation Policies .....</b>	<b>102</b>
<b>3.2.9.3.1 Activity – Send Storage Commitment Request .....</b>	<b>102</b>
<b>3.2.9.3.1.1 Description and Sequencing of Activity .....</b>	<b>102</b>
<b>3.2.9.3.2 General .....</b>	<b>102</b>
<b>3.2.9.3.2.1 Proposed Presentation Contexts .....</b>	<b>103</b>
<b>3.2.9.3.2.2 SOP Specific Conformance as an Association Requestor .....</b>	<b>103</b>
<b>3.2.9.3.2.2.1 SOP Specific Conformance - Storage Commitment .....</b>	<b>103</b>
<b>3.2.9.3.2.2.2 Association Requestor Communication Failure Behavior .....</b>	<b>105</b>
<b>3.2.9.4 Association Acceptance Policy .....</b>	<b>106</b>
<b>3.2.9.4.1 Activity – Receive Storage Commitment Response .....</b>	<b>106</b>
<b>3.2.9.4.1.1 Description and Sequencing of Activity .....</b>	<b>106</b>
<b>3.2.9.4.1.2 Accepted Presentation Contexts .....</b>	<b>107</b>
<b>3.2.9.4.1.3 SOP Specific Conformance as an Association Acceptor .....</b>	<b>107</b>
<b>3.2.9.4.1.3.1 SOP Specific Conformance – Verification .....</b>	<b>107</b>
<b>3.2.9.4.1.3.2 SOP Specific Conformance – Storage Commitment .....</b>	<b>108</b>
<b>3.2.9.4.1.3.3 Association Acceptor Communication Failure Behavior .....</b>	<b>108</b>
<b>3.2.10 QIDO-RS Service Provider Specification .....</b>	<b>109</b>
<b>3.2.10.1 QIDO-RS Search For Studies .....</b>	<b>109</b>
<b>3.2.10.1.1 Command .....</b>	<b>109</b>
<b>3.2.10.2 QIDO-RS Search For Series .....</b>	<b>111</b>
<b>3.2.10.2.1 Command .....</b>	<b>111</b>
<b>3.2.10.3 QIDO-RS Search For Instances .....</b>	<b>113</b>
<b>3.2.10.3.1 Command .....</b>	<b>113</b>
<b>3.2.10.4 QIDO RS Multi-Context Support .....</b>	<b>114</b>
<b>3.2.10.5 QIDO RS Limitations .....</b>	<b>115</b>
<b>3.2.10.6 Preference Order for Multiple Accept Headers .....</b>	<b>115</b>
<b>3.2.10.7 QIDO-RS Status Codes .....</b>	<b>115</b>
<b>3.2.10.8 Connection Policies .....</b>	<b>116</b>
<b>3.2.10.8.1 General .....</b>	<b>116</b>
<b>3.2.10.8.2 Security .....</b>	<b>116</b>
<b>3.2.11 WADO-RS Service Provider Specification .....</b>	<b>116</b>
<b>3.2.11.1 Supported Transfer Syntaxes/Media Types .....</b>	<b>116</b>
<b>3.2.11.1.1 WADO-RS DICOM Object Transfer Syntaxes Support .....</b>	<b>116</b>
<b>3.2.11.1.2 WADO-RS Image Transfer Syntaxes Support .....</b>	<b>117</b>
<b>3.2.11.1.3 DICOM Little Endian Media-Type / Transfer Syntax Support .....</b>	<b>118</b>
<b>3.2.11.1.4 Retrieve Metadata Media Type Support .....</b>	<b>118</b>
<b>3.2.11.2 HTTP Status Codes .....</b>	<b>118</b>
<b>3.2.11.3 WADO-RS Retrieve Study .....</b>	<b>119</b>
<b>3.2.11.3.1 Command .....</b>	<b>119</b>
<b>3.2.11.3.2 URL Parameters .....</b>	<b>119</b>
<b>3.2.11.3.3 WADO-RS Retrieve Study Options .....</b>	<b>119</b>
<b>3.2.11.3.4 WADO-RS Retrieve Study Response .....</b>	<b>120</b>
<b>3.2.11.3.4.1 Response Headers .....</b>	<b>120</b>
<b>3.2.11.3.4.2 Response Content .....</b>	<b>121</b>
<b>3.2.11.3.5 Retrieve Study Example .....</b>	<b>121</b>
<b>3.2.11.4 WADO-RS Retrieve Series .....</b>	<b>122</b>

3.2.11.4.1	Command.....	122
3.2.11.4.2	URL Parameters.....	122
3.2.11.4.3	WADO-RS Retrieve Series Options .....	122
3.2.11.4.4	WADO-RS Retrieve Series Response.....	122
3.2.11.4.4.1	Response Headers.....	122
3.2.11.4.4.2	Response Content .....	123
3.2.11.4.5	Retrieve Series Example .....	123
3.2.11.5	WADO-RS Retrieve Instance.....	124
3.2.11.5.1	Command.....	124
3.2.11.5.2	URL Parameters.....	124
3.2.11.5.3	WADO-RS Retrieve Instance Options .....	124
3.2.11.5.4	WADO-RS Retrieve Instance Response .....	125
3.2.11.5.4.1	Response Headers.....	125
3.2.11.5.4.2	Response Content .....	126
3.2.11.5.5	Retrieve Instance Example .....	126
3.2.11.6	WADO-RS Retrieve Frames.....	126
3.2.11.6.1	Command.....	126
3.2.11.6.2	URL Parameters.....	126
3.2.11.6.3	WADO-RS Retrieve Frames Options .....	127
3.2.11.6.4	WADO-RS Retrieve Frames Response.....	127
3.2.11.6.4.1	Response Headers.....	127
3.2.11.6.4.2	Response Content .....	127
3.2.11.6.5	Retrieve Frames Example .....	128
3.2.11.7	WADO-RS Retrieve BulkData.....	128
3.2.11.7.1	Command.....	128
3.2.11.7.2	WADO-RS Retrieve BulkData Options.....	128
3.2.11.7.3	WADO-RS Retrieve BulkData Response .....	129
3.2.11.7.3.1	Response Headers.....	129
3.2.11.7.3.2	Retrieve BulkData response.....	129
3.2.11.7.3.3	Response Content .....	130
3.2.11.7.4	Retrieve BulkData Example .....	130
3.2.11.8	WADO-RS Retrieve Metadata .....	130
3.2.11.8.1	Command.....	130
3.2.11.8.2	URL Parameters.....	130
3.2.11.8.3	WADO-RS Retrieve Metadata Options.....	130
3.2.11.8.4	WADO-RS Retrieve Metadata Response .....	131
3.2.11.8.4.1	Response Headers.....	131
3.2.11.8.4.2	Retrieve Metadata response.....	131
3.2.11.8.4.3	Response Content .....	131
3.2.11.8.5	Retrieve Metadata Example .....	132
3.2.11.9	WADO RS Multi-Context Support .....	132
3.2.11.10	Preference Order For Multiple Accept Headers .....	132
3.2.11.11	WADO RS Limitations .....	132
3.2.11.12	Connection Policies.....	133
3.2.11.12.1	General.....	133
3.2.11.12.2	Security .....	133

<b>3.3</b>	<b>Network Interfaces .....</b>	<b>133</b>
3.3.1	Physical Network Interface .....	133
3.3.2	Additional Protocols.....	133
3.3.2.1	DHCP .....	133
3.3.2.2	DNS.....	134
<b>3.4</b>	<b>Configuration.....</b>	<b>134</b>
3.4.1	AE Title/Presentation Address Mapping .....	134
3.4.1.1	Local AE Titles .....	134
3.4.1.2	Remote AE Title/Presentation Address Mapping .....	135
3.4.1.2.1	Sender AE .....	135
3.4.1.2.2	Importer AE.....	135
3.4.1.2.3	Query/Retrieve Server AE .....	135
3.4.1.2.4	Query/Retrieve Client AE .....	135
3.4.1.2.5	Modality Worklist Client AE .....	135
3.4.1.2.6	Print Management AE .....	135
3.4.1.2.7	External Notifier AE.....	135
3.4.1.2.8	Event Handler AE .....	135
3.4.1.2.9	Storage Commitment Client AE.....	136
3.4.2	Configurable Parameters .....	136
<b>4.</b>	<b>MEDIA INTERCHANGE.....</b>	<b>141</b>
4.1	Implementation Model.....	141
4.1.1	Application Data Flow .....	141
4.1.2	Functional Definitions of AEs.....	141
4.1.2.1	Removable Media AE .....	141
4.1.3	Sequencing of Real-World Activities.....	141
4.1.4	File Meta Information Options .....	141
4.2	AE Specifications .....	142
4.2.1	Removable Media AE Specification.....	142
4.2.1.1	File Meta Information for the Application Entity.....	145
4.2.1.2	Real-World Activities.....	145
4.2.1.2.1	Activity – User Imports Files from Removable Media.....	145
4.2.1.2.2	Activity – User Exports Files to Removable Media .....	145
4.2.1.3	Options.....	146
4.3	Augmented and Private Application Profiles.....	146
4.4	Media Configuration.....	146
<b>5.</b>	<b>SUPPORT FOR EXTENDED CHARACTER SETS.....</b>	<b>147</b>
<b>6.</b>	<b>SECURITY.....</b>	<b>148</b>
<b>7.</b>	<b>ANNEXES.....</b>	<b>149</b>
7.1	IOD Contents.....	149
7.1.1	Importer AE Standard Element Use.....	149

7.1.1.1	Supported Composite SOP Classes for Display .....	149
7.1.1.2	Unsupported Composite SOP Classes for Display .....	150
7.1.2	Significant Elements in Received Images.....	152
7.1.3	Significant Elements in Received GSPS Instances.....	155
7.1.4	McKesson Radiology™ Added Private Elements .....	172
7.1.5	Sender AE and Query/Retrieve Server AE Element Modification .....	172
7.1.6	Sender AE MIMA Element Support .....	173
7.1.7	Derived MPR Image Creation.....	174
7.1.7.1	Derived MPR Image IODs.....	175
7.1.7.2	Derived MPR Image Module Attributes .....	176
7.1.7.2.1	Derived MPR Image Common Module Attributes.....	176
7.1.7.2.2	Derived MPR CT Image Specific Module Attributes.....	181
7.1.7.2.3	Derived MPR MR Image Specific Module Attributes .....	181
7.1.8	Secondary Capture Image Creation for Scanned Document .....	182
7.1.8.1	Secondary Capture Image IODs for Scanned Document .....	182
7.1.8.2	Secondary Capture Image Module Attributes for Scan Document .....	183
7.1.9	Grayscale SoftCopy Presentation State Object Creation.....	186
7.1.9.1	Grayscale SoftCopy Presentation State IODs Modules .....	186
7.1.9.2	Grayscale SoftCopy Presentation State Module Attributes .....	187
7.1.10	Raw Data Instance Creation for MC Study Data Files .....	216
7.1.10.1	Raw Data IOD for MC Study Data Files .....	216
7.1.10.2	RAW Data Object Module Attributes for MC Data files.....	216
7.1.11	Encapsulated PDF Instance Creation for MC Study PDF Files.....	220
7.1.11.1	EPDF IOD for MC Study PDF Files .....	220
7.1.11.2	EPDF Object Module Attributes for MC PDF files .....	220
7.1.12	Significant Elements in Received Mammography CAD SR .....	225
8.	REVIEWERS .....	237
9.	APPROVERS.....	238



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 16

## 2. INTRODUCTION

### 2.1 AUDIENCE

This document is the DICOM 3.0 Conformance Statement for McKesson Radiology™ 12.2. It is intended for hospital staff, health system integrators, and software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

### 2.2 REMARKS

McKesson Radiology™ is a self-contained, networked computer system used for receiving, archiving, and displaying diagnostic medical images. The system conforms to the DICOM 3.0 standard to allow the sharing of medical information with other digital imaging systems.

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information.

The scope of this Conformance Statement is to facilitate communication between McKesson Radiology 12.2 and other DICOM systems. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different Conformance Statements is the first step towards assessing interconnectivity between McKesson Radiology 12.2 and other DICOM conformant equipment.
- Test procedures should be defined to validate the desired level of connectivity.

### 2.3 DEFINITIONS, TERMS AND ABBREVIATIONS

VR Value Representation - The value type of the DICOM attribute  
SIM Shared Image Management - With SIM, customers will have one PACS system to learn and maintain instead of having a separate PACS system for both Radiology and Cardiology Studies.

## 3. NETWORKING

### 3.1 Implementation Model

#### 3.1.1 Application Data Flow Diagram

**Figure 1: McKesson Radiology™ DICOM Network Data Flow Diagram**

Figure 1-1 Send Instances to External System

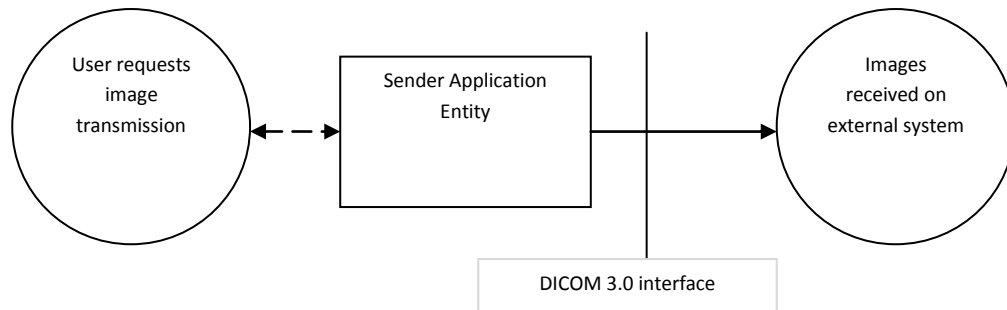


Figure 1-2 Receive Instances from External System

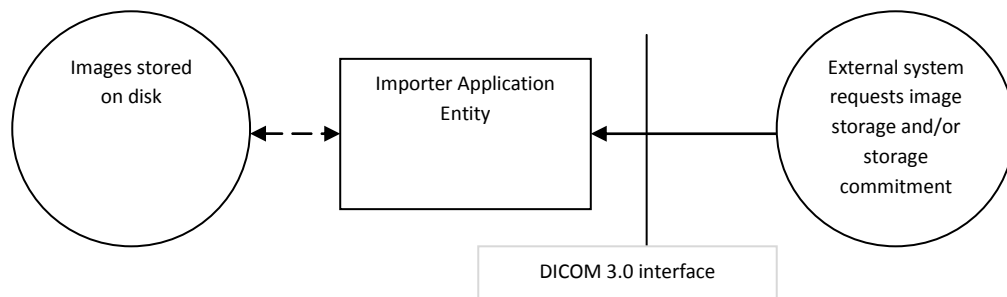


Figure 1-3 Issue Query/Retrieve Request

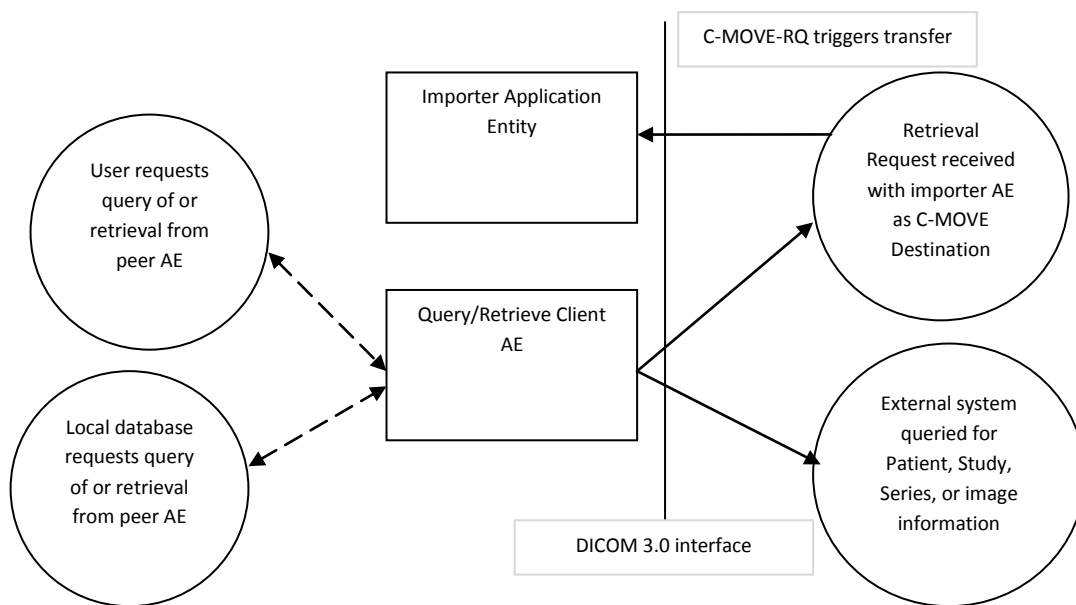


Figure 1-4 Issue Modality Worklist Request

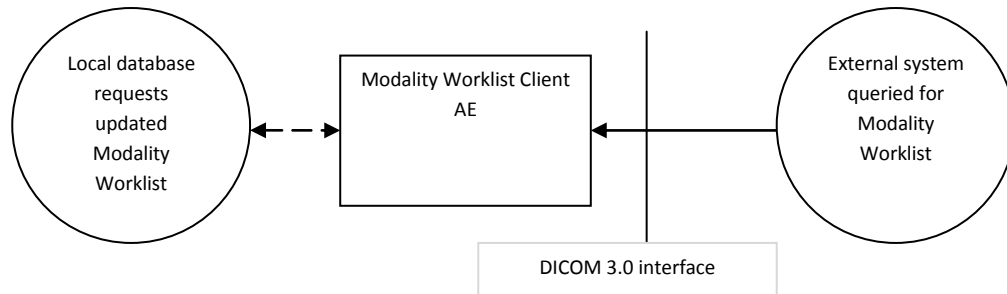


Figure 1-5 Receive Query/Retrieve and MWL requests

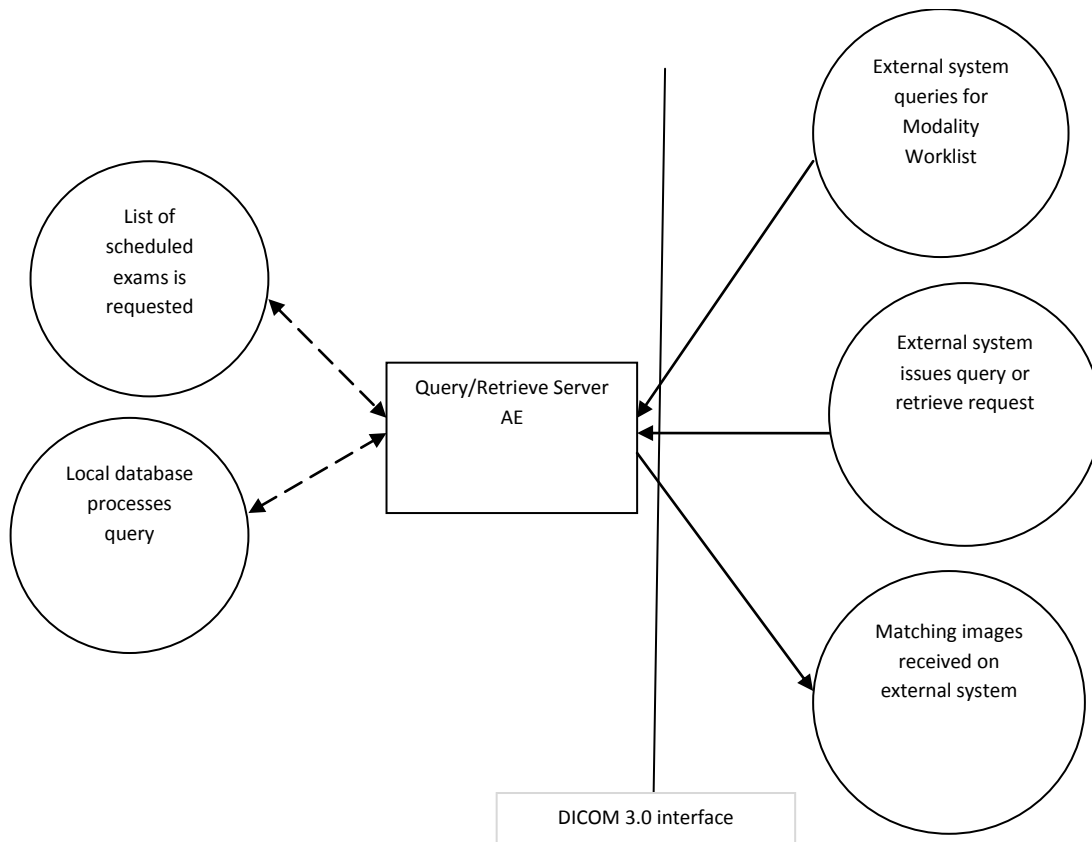


Figure 1-6 Send Notification Message

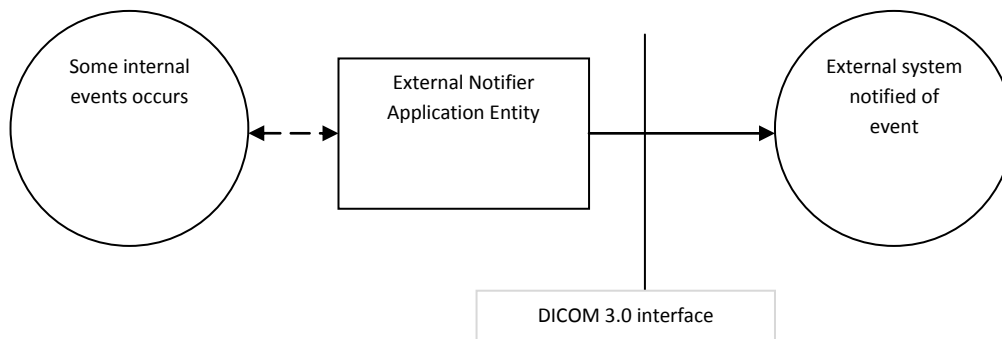


Figure 1-7 Issue Storage Commitment request and Receive Event

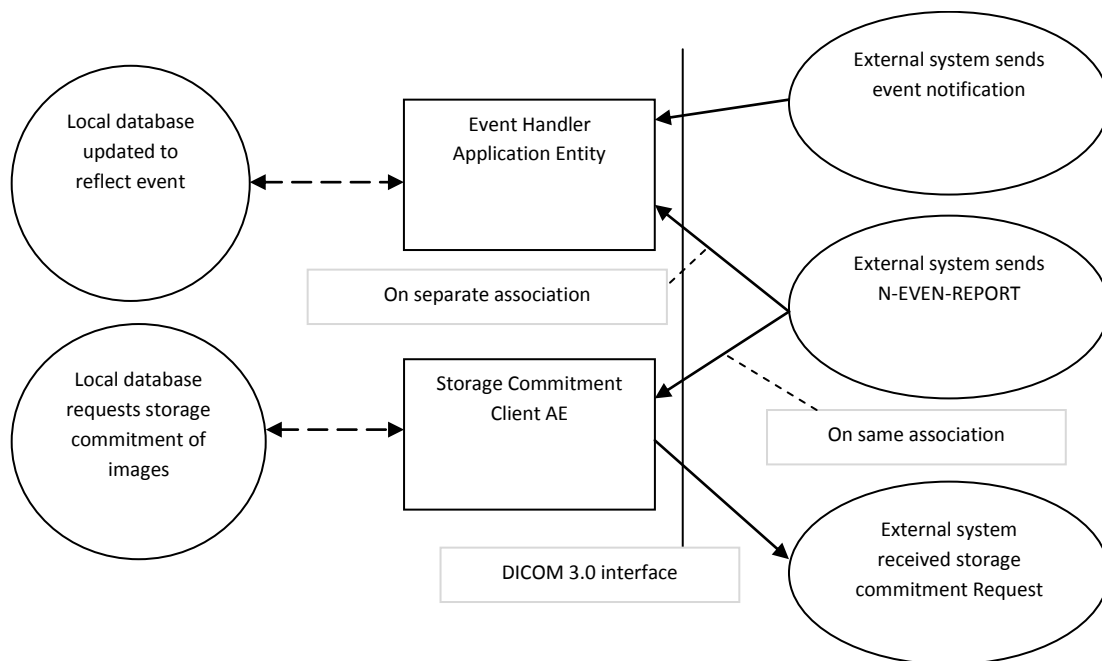


Figure 1-8 Issue Printing Request

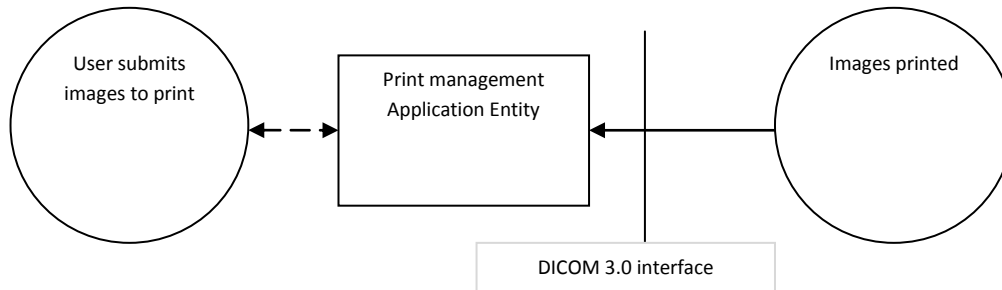


Figure 1-9 Receive QIDO-RS Request


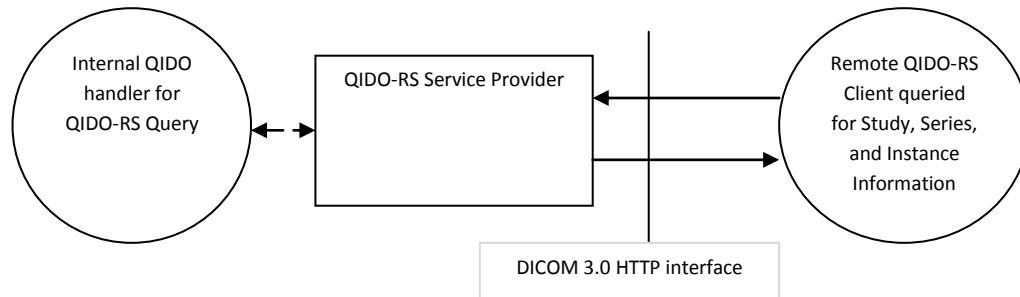


Figure 1-10 Receive WADO-RS Request

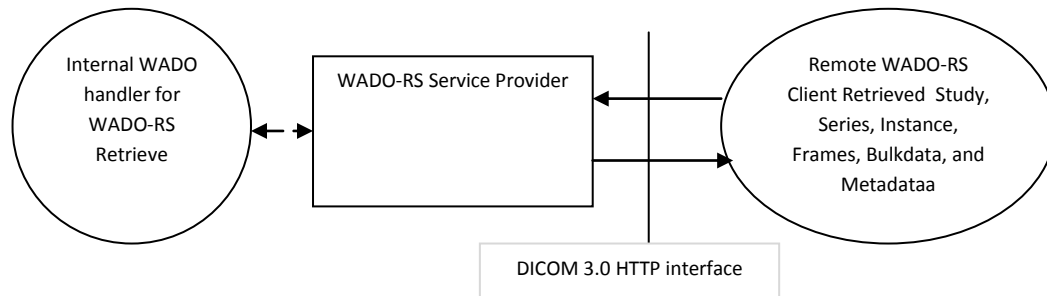

The Sender AE can send Storage Image objects as a C-STORE SCU. It receives requests from a McKesson Radiology™ user to transmit a list of images to a specific DICOM destination.

The Importer AE can receive Storage Image objects as a C-STORE SCP. As an SCP it can respond to external Storage Requests which are either unsolicited or a result of DICOM C-MOVE requests. It can also receive Storage Commitment Push Model N-ACTION Requests from the SCU. The Importer can send all N-EVENT Reports over this same Association or open a new Association to the SCU and send the N-EVENT report over the new Association.

The Query/Retrieve Server AE allows external systems to query McKesson Radiology™ for Modality Worklist, patient, study and series demographic queries as a C-FIND SCP. Also, image retrievals will be processed by this AE as a C-MOVE SCP.

The Query/Retrieve Client AE acts as an Association Requestor for sending queries or retrieval requests to a remote AE acting as an SCP for the C-FIND query or C-MOVE retrieval SOP Classes. The Query/Retrieve Client AE can either be triggered directly through the user interface, or when the McKesson Radiology™ system is aware that it must retrieve SOP Instances from a remote AE (i.e. The McKesson Radiology™ database indicates that the data was sent to the remote AE earlier, such as when the remote AE is serving as the primary archive).

The Modality Worklist Client AE acts as an Association Requestor for sending queries to a remote AE acting as an SCP for the Modality Worklist SOP Class. If the Modality Worklist Client AE is enabled then it will automatically query a remote AE repeatedly for the latest Modality Worklist. The time period between queries is configurable.

The Print Management AE enables users to initiate an Association with a DICOM-compliant printer to print a list of selected images.

The External Notifier AE will forward any Modality Performed Procedure Step request received by the Event Handler AE.

The Event Handler AE receives notifications of events from external systems. This AE can receive Modality Performed Procedure Step requests.

The Storage Commitment Client AE implements the Storage Commitment Service Class as an SCU. When acting as an SCU, it issues a Storage Commitment Push Model N-ACTION Request to a Remote Storage Commitment SCP AE to explicitly request the remote Storage Commitment SCP AE to make the commitment for the safekeeping of the SOP Instances archived by the Sender AE.

The Removable Media AE can be used to create and read DICOM removable media. The user can choose to access the image files for individual studies on DICOM removable media. They can also choose to export individual studies that exist in the system's database to removable media.

The QIDO-RS Service Provider receives QIDO requests from a remote QIDO-RS Client. These requests are HTTP/1.1 GET requests. It uses the request to select matching Studies, Series or Instances. It then returns a set of matching Studies, Series or Instances or a response code indicating warning or failure back to the requesting QIDO-RS Client.

The WADO-RS Service Provider receives WADO-RS requests from a remote WADO-RS Client. These requests are HTTP/1.1 GET requests. It converts these requests into internal lookup functions to find the matching SOP Instances. It then obtains these matching SOP Instances and composes a response back to the requesting WADO-RS Client.

### **3.1.2 Functional Definitions of Application Entities**

McKesson Radiology™ contains, conceptually, eleven local Application Entities (AE's) and Service Providers: Sender, Importer, Query/Retrieve Server, Query/Retrieve Client, Modality Worklist Client, Print Management, External Notifier, Event Handler, Storage Commitment Client, QIDO-RS Service Provider, and WADO-RS Service Provider. The Application Entities and Service Providers run as background Windows tasks or Restful Web Services.

#### **3.1.2.1 Sender AE**

The Sender AE acts as an SCU and implements the Storage Service Class operation. It can transmit images that have been received from prior external DICOM transmissions.

#### **3.1.2.2 Importer AE**

The Importer AE acts as an SCP and implements the Storage Service Class operation. It can receive unsolicited image storage requests from external DICOM storage SCUs. It also acts as an SCP for the Storage Commitment Push Model SOP Class.

#### **3.1.2.3 Query/Retrieve Server AE**

The Query/Retrieve Server AE implements the Query/Retrieve Service Class as an SCP. The Query/Retrieve Server AE can handle requests from external devices to query the database for worklists, patient, study and series demographics, and image level information. It can also handle C-MOVE Requests from remote AEs for the retrieval of Composite SOP Instances. The Query/Retrieve Server AE can act as an SCU of the Storage Service to transfer the requested Composite SOP Instances.

#### **3.1.2.4 Query/Retrieve Client AE**

The Query/Retrieve Client AE implements the Query/Retrieve Service Class as an SCU. It can act as an SCU to query remote AEs for patient, study and series information. It can also request the retrieval of Composite SOP Instances from remote AEs using C-MOVE Requests. When doing so, it always specifies the Importer AE running on the same McKesson Radiology™ system as the C-MOVE Destination AE.

### **3.1.2.5 Modality Worklist Client AE**

The Modality Worklist Client AE implements the Modality Worklist SOP Class as an SCU. It cannot be triggered through the user interface. Instead it will repeatedly query for the latest Modality Worklist, with a configurable delay period between each query.

### **3.1.2.6 Print Management AE**

The Print Management AE implements the Print Management Service Class as an SCU. It supports both the Basic Grayscale Print Management and Basic Color Print Management Classes.

### **3.1.2.7 External Notifier AE**

The External Notifier AE implements the Modality Performed Procedure Step Service Class. It can send Modality Performed Procedure Step messages whenever a configurable set of system events occurs.

### **3.1.2.8 Event Handler AE**

The Event Handler AE implements full support of the Modality Performed Procedure Step Service Class..

### **3.1.2.9 Storage Commitment Client AE**

The Storage Commitment Client AE implements the Storage Commitment Service Class as an SCU. When acting as an SCU, it issues a Storage Commitment Push Model N-ACTION Request to a Remote Storage Commitment SCP AE to explicitly request the remote Storage Commitment SCP AE to make the commitment for the safekeeping of the SOP Instances archived by the Sender AE. Depending on the configuration value, the Storage Commitment Client AE can receive Storage Commitment Confirmation for Composite SOP Instances from the Storage Commitment SCP AE on the same association or on a separate association. The Event Handler AE will handle Storage Commitment Confirmation if sent on a different association.

### **3.1.2.10 QIDO-RS Service Provider**


The QIDO-RS Service Provider implements the Query based on ID for DICOM Objects (QIDO) by Representational State Transfer (REST) Services. Upon receiving a QIDO-RS HTTP/1.1 GET request for DICOM studies, series, or instances, from a Remote QIDO-RS Client, the QIDO-RS Service Provider performs the search based on the URL of the request. The search is similar to the DICOM C-FIND for the "Study Root" hierarchical Information Model for Query and Retrieve. The Study is the highest, or root level, containing study information such as patient ID and Accession Number. Below that is Series, followed by the Instance level (Study→Series→Instance). The response returned to the Remote QIDO-RS Client is a status code indicating the success, warning, or failure of the search along with any matching results stored in the McKesson Radiology™ system.

### **3.1.2.11 WADO-RS Service Provider**

The WADO-RS Service Provider implements the Web Access to DICOM Persistent Objects by RESTful Services for access to DICOM SOP Instances that are stored in the McKesson Radiology™ system. The DICOM WADO-RS Services defines several action types (RetrieveStudy, RetrieveSeries, RetrieveInstance, RetrieveFrames, RetrieveBulkdata, and RetrieveMetadata) that the Remote WADO-RS Client can use for accessing the SOP Instances. Upon receiving a WADO-RS HTTP/1.1 GET request for one of the action types from a Remote WADO-RS Client, the WADO-RS Service Provider retrieves the indicated SOP Instance(s) based on the URL of the request. The response returned to the Remote WADO-RS Client is a status code indicating the success, warning, or failure of the request along with resulting data retrieved.

## **3.1.3 Sequencing of Real-World Activities**

The only sequencing constraint that exists across all the McKesson Radiology™ Application Entities is the fact that a Composite SOP Instance must be received by the Importer AE before Storage Commitment Push Model or Query-Retrieve Requests related to this SOP Instance can be successfully handled:

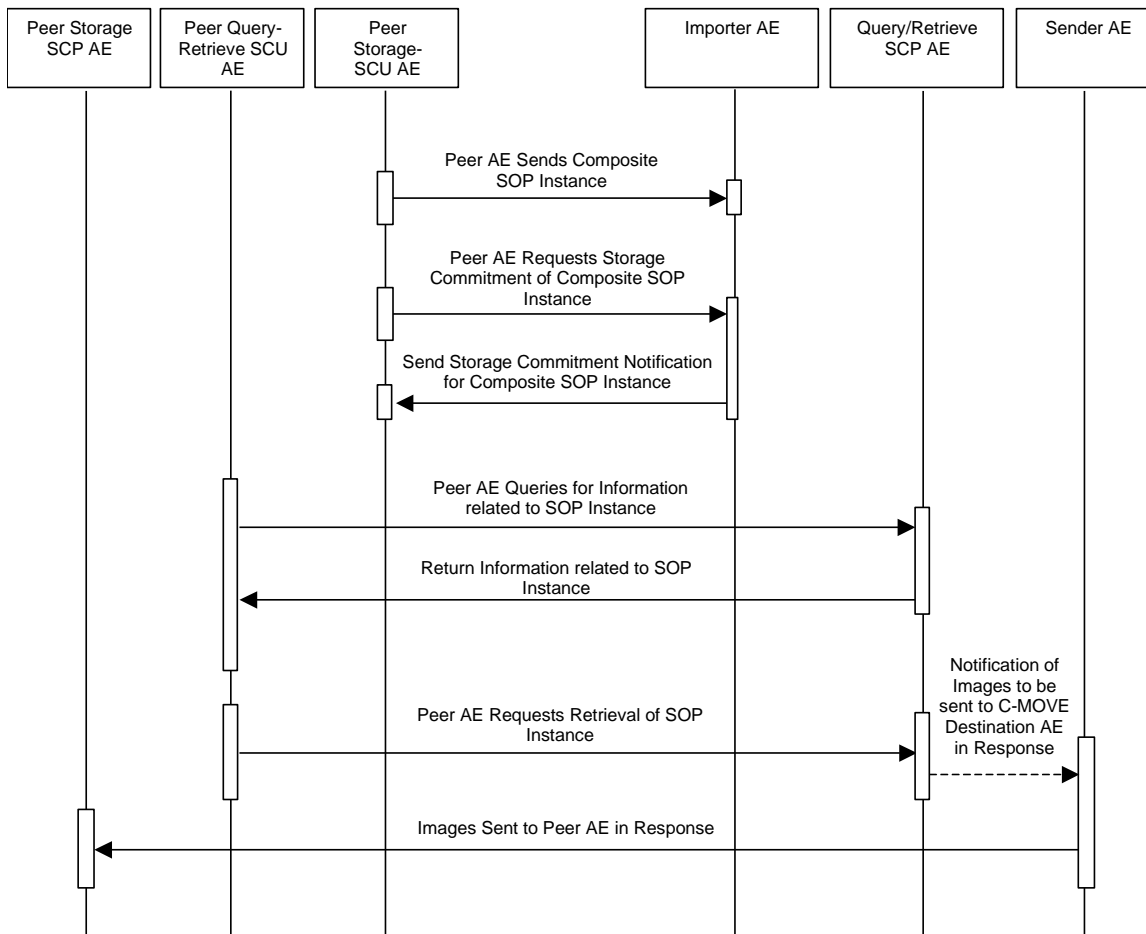**Figure 2: McKesson Radiology™ Sequencing Constraints**

Note that the only constraint is for the Composite SOP Instance to be received prior to the other events. For example, it is not necessary for the Storage Commitment Push Model Request to be received prior to receiving Query or Retrieval Requests related to the SOP Instance.



## 3.2 AE Specifications

### 3.2.1 Sender AE Specification

#### 3.2.1.1 SOP Classes

The Sender AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 4: SOP Class Conformance of Sender AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	No
<b>Transfer</b>			
12-lead ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	No
Ambulatory ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	No
Basic Voice Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	No
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	No
General Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.2	Yes	No
Arterial Pulse Waveform	1.2.840.10008.5.1.4.1.1.9.5.1	Yes	No
Respiratory Waveform	1.2.840.10008.5.1.4.1.1.9.6.1	Yes	No
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11	Yes	No
Comprehensive Structured Report	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	Yes	No
Mammography CAD Structured Report	1.2.840.10008.5.1.4.1.1.88.50	Yes	No
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Yes	No
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Yes	No
Colon CAD SR Document	1.2.840.10008.5.1.4.1.1.88.69	Yes	No
Implantation Plan SR Document	1.2.840.10008.5.1.4.1.1.88.70	Yes	No
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Yes	No
Encapsulated CDA IOD	1.2.840.10008.5.1.4.1.1.104.2	Yes	No
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Yes	No
CT Image	1.2.840.10008.5.1.4.1.1.2	Yes	No
Digital X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	Yes	No
Digital X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	No
Digital Mammography Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.2	Yes	No
Digital Mammography Image (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	No
Breast Tomosynthesis Image	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	No
Digital Intra-oral X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	Yes	No
Digital Intra-oral X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	No
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	No
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1	Yes	No
Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.2	Yes	No
Pseudo-Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.3	Yes	No
Blending Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.4	Yes	No
XA/XRF Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.5	Yes	No
Hardcopy Color Image	1.2.840.10008.5.1.1.30	Yes	No
Hardcopy Grayscale Image	1.2.840.10008.5.1.1.29	Yes	No
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	No
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	Yes	No
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	Yes	No

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 25

DICOM SOP Class Name	SOP Class UID	SCU	SCP
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	Yes	No
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Yes	No
MR Image	1.2.840.10008.5.1.4.1.1.4	Yes	No
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	No
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	Yes	No
Nuclear Medicine Image (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	No
Positron Emission Tomography Image	1.2.840.10008.5.1.4.1.1.128	Yes	No
Raw Data	1.2.840.10008.5.1.4.1.1.66	Yes	No
Spatial Registration	1.2.840.10008.5.1.4.1.1.66.1	Yes	No
Spatial Fiducials	1.2.840.10008.5.1.4.1.1.66.2	Yes	No
Deformable Spatial Registration	1.2.840.10008.5.1.4.1.1.66.3	Yes	No
Segmentation	1.2.840.10008.5.1.4.1.1.66.4	Yes	No
Surface Segmentation	1.2.840.10008.5.1.4.1.1.66.5	Yes	No
Real World Value Mapping	1.2.840.10008.5.1.4.1.1.67	Yes	No
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Yes	No
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Yes	No
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Yes	No
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	No
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Yes	No
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Yes	No
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Yes	No
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	No
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	No
RT Beams Delivery Instruction	1.2.840.10008.5.1.4.34.7	Yes	No
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Yes	No
Stand-alone Curve	1.2.840.10008.5.1.4.1.1.9	Yes	No
Stand-alone Modality LUT	1.2.840.10008.5.1.4.1.1.10	Yes	No
Stand-alone Overlay	1.2.840.10008.5.1.4.1.1.8	Yes	No
Stand-alone VOI LUT	1.2.840.10008.5.1.4.1.1.11	Yes	No
Standalone PET Curve	1.2.840.10008.5.1.4.1.1.129	Yes	No
Stored Print	1.2.840.10008.5.1.1.27	Yes	No
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Yes	No
Ultrasound Image (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	No
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Yes	No
Ultrasound Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	No
VL Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	No
VL Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	No
VL Slide-Coordinates Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	No
VL Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	No
VL Image (Retired)	1.2.840.10008.5.1.4.1.1.77.1	Yes	No
VL Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.77.2	Yes	No
Video Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1.1	Yes	No
Video Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2.1	Yes	No
Video Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4.1	Yes	No
Ophthalmic Photography 8 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.1	Yes	No
Ophthalmic Photography 16 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.2	Yes	No
Stereometric Relationship	1.2.840.10008.5.1.4.1.1.77.1.5.3	Yes	No
X-Ray Angiographic Bi-Plane Image (retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	No
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Yes	No
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Yes	No

DICOM SOP Class Name	SOP Class UID	SCU	SCP
X-Ray Radiation Dose Structured Report	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes
Lensometry Measurements	1.2.840.10008.5.1.4.1.1.78.1	Yes	No
Autorefractometry Measurements	1.2.840.10008.5.1.4.1.1.78.2	Yes	No
Keratometry Measurements	1.2.840.10008.5.1.4.1.1.78.3	Yes	No
Subjective Refraction Measurements	1.2.840.10008.5.1.4.1.1.78.4	Yes	No
Visual Acuity Measurements	1.2.840.10008.5.1.4.1.1.78.5	Yes	No
Spectacle Prescription Report	1.2.840.10008.5.1.4.1.1.78.6	Yes	No
Ophthalmic Axial Measurements	1.2.840.10008.5.1.4.1.1.78.7	Yes	No
Intraocular Lens Calculations	1.2.840.10008.5.1.4.1.1.78.8	Yes	No
Macular Grid Thickness and Volume Report	1.2.840.10008.5.1.4.1.1.79.1	Yes	No
Ophthalmic Visual Field Static Perimetry Measurements	1.2.840.10008.5.1.4.1.1.80.1	Yes	No
Basic Structured Display IOD	1.2.840.10008.5.1.4.1.1.131	Yes	No
Generic Implant Template	1.2.840.10008.5.1.4.43.1	Yes	No
Implant Assembly Template	1.2.840.10008.5.1.4.44.1	Yes	No
Implant Template Group	1.2.840.10008.5.1.4.45.1	Yes	No
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	Yes	No
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	Yes	No
Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	Yes	No
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Yes	No
Radiopharmaceutical Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.68	Yes	No

The Sender AE will attempt to send stored DICOM images in the abstract syntax in which they were received. If a negotiated Association to a remote C-STORE SCP does not support the required abstract syntax, the Sender AE will attempt to transform the image object into an abstract syntax that is supported on that Association. The transformations that the Sender AE will attempt depend on the initial abstract syntax of the image.

To send images objects in either the single or multi-frame retired Ultrasound SOP classes across Associations not supporting these classes, the Sender AE first attempts to send the images by transforming them into the matching (single or multi-frame) Ultrasound new SOP classes. Likewise, for Associations not supporting the new Ultrasound classes, the Sender AE will transform the images into the corresponding retired class.

The Sender AE will attempt to send stored DICOM images in the Transfer Syntax in which they were received. If, however, that Transfer Syntax is not supported on an Association, the Sender AE will transform the Transfer Syntax of the image to the default DICOM Implicit VR Little Endian and send it in that syntax.

The Sender AE represents a single task on a Windows machine, with multiple instances of the Sender AE possible on a single host. Each Sender AE is configured to send to a single remote DICOM C-STORE SCP destination. Multiple C-STORE SCP destinations can be implemented by configuring more than one Sender AE. In this case each separate Sender AE acts independently of any others (are implemented as separate processes). In addition, multiple instances of the Sender AE can be configured to send to a single Remote AE.

### 3.2.1.2 Association Establishment Policies

#### 3.2.1.2.1 General

The Sender AE will initiate a new Association when the user requests the transmission of a set of images (either a complete study or series, or part thereof). Also, McKesson Radiology™ can be configured to automatically send (i.e. forward) any images that are sent to it (received via the Import AE). An attempt will be made to transmit all the images in the study in a single Association. The Association will be released when all the images have been sent. If the Association is broken or some other Association related error is detected, the Association will be aborted and an attempt will be made to transmit the unsent images in a new Association.

The DICOM Standard Application Context Name is always proposed:

**Table 5: DICOM Application Context for Sender AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

The maximum PDU size that will be offered is configurable, and by default is 16,384 bytes.

### 3.2.1.2.2 Number of Associations

Each Sender AE process will only attempt to open one Association at a time to the destination it is configured to send to. By default, each instance of the Sender AE application will send to a different Remote AE, although it is possible to configure multiple Sender AE instances to send to the same Remote AE. However, as multiple destinations can be configured, each with their own Sender AE process, multiple Sender AE connections can be open at one time. Thus, there is no limit on the number of simultaneous Associations that Sender AE can attempt.

**Table 6: Number of Simultaneous Associations as an SCU for Sender AE**

Maximum number of simultaneous Associations	Unlimited
---	-----------

### 3.2.1.2.3 Asynchronous Nature

The Sender AE does not provide asynchronous communication (multiple outstanding transactions over a single Association). All Association requests must be completed and acknowledged before a new operation can be initiated.

**Table 7: Asynchronous Nature as an SCU for Sender AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

### 3.2.1.2.4 Implementation Identifying Information

**Table 8: DICOM Implementation Class and Version for Sender AE**

Implementation Class UID	1.2.840.113711.1
Implementation Version Name	V1.0

### 3.2.1.3 Association Initiation Policy

#### 3.2.1.3.1 Activity – User Requests Transmission of Images

##### 3.2.1.3.1.1 Description and Sequencing of Activity

The Sender AE attempts to open a new Association for each set of images within a single study it attempts to transfer (i.e. images belonging to separate studies will not be sent over the same Association). This occurs when a user of McKesson Radiology™ requests the transmission of Images. There is no sequencing of this activity.

##### 3.2.1.3.1.2 Proposed Presentation Contexts

The Sender AE may propose any one or more of the following Transfer Syntaxes for each of the abstract syntaxes listed in Table 4. Each proposed **Presentation Context** contains a single Transfer Syntax. Multiple Transfer Syntaxes per abstract syntax would be proposed with multiple Presentation Contexts.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 28

**Table 9: Sender AE Proposed Transfer Syntaxes**

Transfer Syntax		Role	Extended Negotiation
Name	UID		
DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
DICOM JPEG Baseline Process 1	1.2.840.10008.1.2.4.50	SCU	None
DICOM JPEG Extended Process 2 & 4	1.2.840.10008.1.2.4.51	SCU	None
DICOM JPEG Lossless Proc 14	1.2.840.10008.1.2.4.57	SCU	None
DICOM JPEG Lossless First Order Prediction	1.2.840.10008.1.2.4.70	SCU	None
DICOM JPEG 2000 (Lossless Only)	1.2.840.10008.1.2.4.90	SCU	None
DICOM JPEG 2000	1.2.840.10008.1.2.4.91	SCU	None
DICOM RLE	1.2.840.10008.1.2.5	SCU	None
ALI Wavelet (Private)	1.2.840.113711.1.2.100.1	SCU	None

NOTE1: The Transfer Syntaxes and supported SOP Classes the Sender AE proposes, as listed above, represent the default behavior. The Sender AE can be configured to propose a subset of these.

NOTE2: The ALI Wavelet private Transfer Syntax is implemented using the Pegasus Imaging Corporation's medical image toolkit.

### **3.2.1.3.1.3 SOP Specific Conformance as an Association Requestor**

#### **3.2.1.3.1.3.1 SOP Specific Conformance – Storage**

In the case of a successful C-STORE response from the SCP, the Sender AE will continue to send any unsent images belonging to the same study. The Association will be properly released after all relevant images have been sent.

When an image is sent to the McKesson Radiology™ Importer AE, the entire set of tags received with the image will be saved in McKesson Radiology™. When the object is selected for transmission from McKesson Radiology™, the content of these objects will be as they were originally received unless patient demographic information and/or study-related information are altered. In such cases the latest values in the database will replace the original information in the DICOM image. Thus, the set of optional tags contained in DICOM objects going out from McKesson Radiology™ depends on the information that was received. For the list of patient, study, and series attributes that can be updated by the Sender AE when a SOP Instance is exported please refer to 7.1.5: Sender AE and Query/Retrieve Server AE Element Modification

McKesson Radiology™ can support the display of overlays included in the original DICOM image (either embedded or separate). It can also be configured to automatically create overlays of its own by specifying that certain DICOM header values should be displayed as strings at certain locations on the displayed image. Additional annotations can be added to images using the 'Mark and Measure' tool of McKesson Radiology Station™. The Sender AE can be configured to convert such annotations to a single bit per pixel overlay that is added as a DICOM Overlay to the exported images. The overlay bitmap is added as an Overlay Data (60xx,3000) Element with the overlay characteristics added to the required Group (60xx) Elements (see DICOM Part 3, Table C.9-2).

The Sender AE can be configured to automatically try resending the SOP Instances if some failure occurs. In addition, the Sender AE can be configured to demote the priority of an export task if export fails a certain number of times. Refer to 3.4.2: Configurable Parameters, for the default values for these settings.

The Sender AE creates files called Service Logs that can be used to monitor its status and diagnose any problems that may arise. If any error occurs during DICOM communication then appropriate messages are always output to these Service Logs. In addition, error messages may be output as alerts to the User Interface in certain cases.

The Sender AE will exhibit the following Behavior according to the Status Code value returned in a C-STORE Response from a destination C-STORE SCP:

**Table 10: Sender AE C-STORE Response Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has successfully stored the exported SOP Instance. Success indication message is output to the Service Logs. A success indication is posted to the User Interface.
Refused	Out of Resources	A700 – A7FF	This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Error	Data Set does not match SOP Class	A900 – A9FF	This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Error	Cannot Understand	C000 – CFFF	This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Warning	Coercion of Data Elements	B000	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. A success indication is also posted to the User Interface.
Warning	Element Discarded	B006	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. A success indication is also posted to the User Interface.
Warning	Data Set does not match SOP Class	B007	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. A success indication is also posted to the User Interface.
Warning	Attribute List Error	0107	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. A success indication is also posted to the User Interface.
Warning	Attribute Value Out of Range	0116	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. A success indication is also posted to the User Interface.
*	*	Any other status code	This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.

### 3.2.1.3.1.3.2

### Association Requestor Communication Failure Behavior

The Behavior of the Sender AE during communication failure is summarized in the following table:

<sup>2</sup> Sender AE can be configured to treat all failures as either permanent or transient. The default behavior is to consider all failures to be transient and to attempt to resend the SOP Instances up to 20 times.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 30

**Table 11: Sender AE Communication Failure Behavior**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure <sup>2</sup> . An error indication is output to the Service Logs. An error indication is also posted to the User Interface.

### 3.2.1.4 Association Acceptance Policy

The Sender AE does not accept Associations.

## 3.2.2 Importer AE Specification

### 3.2.2.1 SOP Classes

The Importer AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 12: SOP Class Conformance of Importer AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	No	Yes
<b>Transfer</b>			
12-lead ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	No	Yes
Ambulatory ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.3	No	Yes
Basic Voice Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.1	No	Yes
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1	No	Yes
General Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.2	No	Yes
Arterial Pulse Waveform	1.2.840.10008.5.1.4.1.1.9.5.1	No	Yes
Respiratory Waveform	1.2.840.10008.5.1.4.1.1.9.6.1	No	Yes
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11	No	Yes
Comprehensive Structured Report	1.2.840.10008.5.1.4.1.1.88.33	No	Yes
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	No	Yes
Mammography CAD Structured Report	1.2.840.10008.5.1.4.1.1.88.50	No	Yes
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	No	Yes
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	No	Yes
Colon CAD SR Document	1.2.840.10008.5.1.4.1.1.88.69	No	Yes
Implantation Plan SR Document	1.2.840.10008.5.1.4.1.1.88.70	No	Yes
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	No	Yes
Encapsulated CDA IOD	1.2.840.10008.5.1.4.1.1.104.2	No	Yes
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	No	Yes
CT Image	1.2.840.10008.5.1.4.1.1.2	No	Yes
Digital X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	No	Yes
Digital X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1	No	Yes
Digital Mammography Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.2	No	Yes

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 31

DICOM SOP Class Name	SOP Class UID	SCU	SCP
Digital Mammography Image (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1	No	Yes
Breast Tomosynthesis Image	1.2.840.10008.5.1.4.1.1.13.1.3	No	Yes
Digital Intra-oral X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	No	Yes
Digital Intra-oral X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1	No	Yes
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2	No	Yes
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1	No	Yes
Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.2	No	Yes
Pseudo-Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.3	No	Yes
Blending Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.4	No	Yes
XA/XRF Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.5	No	Yes
Hardcopy Color Image	1.2.840.10008.5.1.1.30	No	Yes
Hardcopy Grayscale Image	1.2.840.10008.5.1.1.29	No	Yes
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	No	Yes
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	No	Yes
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	No	Yes
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	No	Yes
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	No	Yes
MR Image	1.2.840.10008.5.1.4.1.1.4	No	Yes
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	No	Yes
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	No	Yes
Nuclear Medicine Image (Retired)	1.2.840.10008.5.1.4.1.1.5	No	Yes
Positron Emission Tomography Image	1.2.840.10008.5.1.4.1.1.128	No	Yes
Raw Data	1.2.840.10008.5.1.4.1.1.66	No	Yes
Spatial Registration	1.2.840.10008.5.1.4.1.1.66.1	No	Yes
Spatial Fiducials	1.2.840.10008.5.1.4.1.1.66.2	No	Yes
Deformable Spatial Registration	1.2.840.10008.5.1.4.1.1.66.3	No	Yes
Segmentation	1.2.840.10008.5.1.4.1.1.66.4	No	Yes
Surface Segmentation	1.2.840.10008.5.1.4.1.1.66.5	No	Yes
Real World Value Mapping	1.2.840.10008.5.1.4.1.1.67	No	Yes
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	No	Yes
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	No	Yes
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	No	Yes
RT Image	1.2.840.10008.5.1.4.1.1.481.1	No	Yes
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	No	Yes
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	No	Yes
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	No	Yes
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	No	Yes
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	No	Yes
RT Beams Delivery Instruction	1.2.840.10008.5.1.4.34.7	No	Yes
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	No	Yes
Stand-alone Curve	1.2.840.10008.5.1.4.1.1.9	No	Yes
Stand-alone Modality LUT	1.2.840.10008.5.1.4.1.1.10	No	Yes
Stand-alone Overlay	1.2.840.10008.5.1.4.1.1.8	No	Yes
Stand-alone VOI LUT	1.2.840.10008.5.1.4.1.1.11	No	Yes
Standalone PET Curve	1.2.840.10008.5.1.4.1.1.129	No	Yes
Stored Print	1.2.840.10008.5.1.1.27	No	Yes
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	No	Yes
Ultrasound Image (Retired)	1.2.840.10008.5.1.4.1.1.6	No	Yes
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	No	Yes
Ultrasound Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.3	No	Yes



DICOM SOP Class Name	SOP Class UID	SCU	SCP
VL Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1	No	Yes
VL Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2	No	Yes
VL Slide-Coordinates Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.3	No	Yes
VL Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4	No	Yes
VL Image (Retired)	1.2.840.10008.5.1.4.1.1.77.1	No	Yes
VL Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.77.2	No	Yes
Video Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1.1	No	Yes
Video Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2.1	No	Yes
Video Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4.1	No	Yes
Ophthalmic Photography 8 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.1	No	Yes
Ophthalmic Photography 16 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.2	No	Yes
Stereometric Relationship	1.2.840.10008.5.1.4.1.1.77.1.5.3	No	Yes
X-Ray Angiographic Bi-Plane Image (retired)	1.2.840.10008.5.1.4.1.1.12.3	No	Yes
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	No	Yes
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	No	Yes
X-Ray Radiation Dose Structured Report	1.2.840.10008.5.1.4.1.1.88.67	No	Yes
Lensometry Measurements	1.2.840.10008.5.1.4.1.1.78.1	No	Yes
Autorefraction Measurements	1.2.840.10008.5.1.4.1.1.78.2	No	Yes
Keratometry Measurements	1.2.840.10008.5.1.4.1.1.78.3	No	Yes
Subjective Refraction Measurements	1.2.840.10008.5.1.4.1.1.78.4	No	Yes
Visual Acuity Measurements	1.2.840.10008.5.1.4.1.1.78.5	No	Yes
Spectacle Prescription Report	1.2.840.10008.5.1.4.1.1.78.6	No	Yes
Ophthalmic Axial Measurements	1.2.840.10008.5.1.4.1.1.78.7	No	Yes
Intraocular Lens Calculations	1.2.840.10008.5.1.4.1.1.78.8	No	Yes
Macular Grid Thickness and Volume Report	1.2.840.10008.5.1.4.1.1.79.1	No	Yes
Ophthalmic Visual Field Static Perimetry Measurements	1.2.840.10008.5.1.4.1.1.80.1	No	Yes
Basic Structured Display IOD	1.2.840.10008.5.1.4.1.1.131	No	Yes
Generic Implant Template	1.2.840.10008.5.1.4.43.1	No	Yes
Implant Assembly Template	1.2.840.10008.5.1.4.44.1	No	Yes
Implant Template Group	1.2.840.10008.5.1.4.45.1	No	Yes
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	No	Yes
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	No	Yes
Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	No	Yes
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	No	Yes
Radiopharmaceutical Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.68	No	Yes
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	No	Yes

These are the default SOP Classes supported. By altering the configuration it is possible to support fewer or more SOP Classes.

The Importer AE will store the DICOM Composite SOP Instances as DICOM Part 10 compliant files using the Transfer Syntax with which they were received.

The Importer AE will fork a child process to handle each Association requested by a remote AE for the Storage of Composite SOP Instances and/or to send a Storage Commitment Push Model N-ACTION Request.

McKesson Radiology Station™ is capable of creating new Derived images by performing Multi-Planar Reconstruction on CT and MR image sets received by the Importer. For the characteristics of these MPR images, refer to 7.1.7: Derived MPR Image Creation.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 33

### 3.2.2.2 Association Establishment Policies

#### 3.2.2.2.1 General

The Importer AE accepts Associations from external DICOM C-STORE SCUs to provide storage on the McKesson Radiology™ system of DICOM Composite SOP Instances. The Importer AE can send a request for establishing an Association to an SCU if an SCU sends a Storage Commitment request and then drops the Association before the Storage Commitment N-EVENT-REPORT Request can be sent.

The DICOM Standard Application Context Name is always proposed:

**Table 13: DICOM Application Context for Importer AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

#### 3.2.2.2.2 Number of Associations

The Importer AE places configurable limitations on the number of simultaneous connections it will support. Once the Importer AE accepts an Association, a spawned child task will receive any images transmitted on that Association and store them on the hard drive. The default maximum number of Associations is 10 per connecting host. It is possible to restrict the number of hosts that can connect with the Importer AE so the combination of these settings can restrict the maximum number of Associations.

**Table 14: Number of Simultaneous Associations as an Acceptor for Importer AE**

Maximum number of simultaneous Associations	Unlimited <sup>3</sup>
---	------------------------

The Importer AE can also request new Associations in order to send Storage Commitment N-EVENT-REPORT Requests. The Importer AE cannot request simultaneous Associations with the same remote AE, so the maximum number of simultaneous Associations depends upon the number of remote AEs that the Importer AE will need to open Associations with in order to send the Storage Commitment N-EVENT-REPORT Requests.

**Table 15: Number of Simultaneous Associations as a Requestor for Importer AE**

Maximum number of simultaneous Associations	Unlimited
---	-----------

#### 3.2.2.2.3 Asynchronous Nature

The Importer AE does not provide asynchronous communication (multiple outstanding transactions over a single Association). All Association requests must be completed and acknowledged before a new operation can be initiated.

**Table 16: Asynchronous Nature as an SCP for Importer AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

#### 3.2.2.2.4 Implementation Identifying Information

**Table 17: DICOM Implementation Class and Version for Importer AE**

Implementation Class UID	1.2.840.113711.9
Implementation Version Name	V1.0

### 3.2.2.3 Association Initiation Policies

#### 3.2.2.3.1 Activity – Require New Association for Storage Commitment


<sup>3</sup> Default maximum is 10 per host permitted to connect to the Importer AE.

### 3.2.2.3.1.1 Description and Sequencing of Activity

The Importer AE can act as an Association Requestor in the case where the SCU issues a Storage Commitment N-ACTION and then immediately drops the Association. The Importer AE can then send a request for establishing an Association to the SCU in order to send the corresponding Storage Commitment N-EVENT-REPORT. The Importer AE can also be configured to always request a new Association to send the Storage Commitment N-EVENT-REPORT rather than trying to send it over the original Association requested by the SCU.

In order to successfully handle Storage Commitment N-ACTION Requests, the Importer AE must have already received the referenced SOP Instances. That is, the Importer AE cannot properly handle a Storage Commitment N-ACTION Request that is sent to it before the SOP Instances it references are sent to the Importer.

**Figure 3: Sequencing of Activity – Require New Association for Storage Commitment**

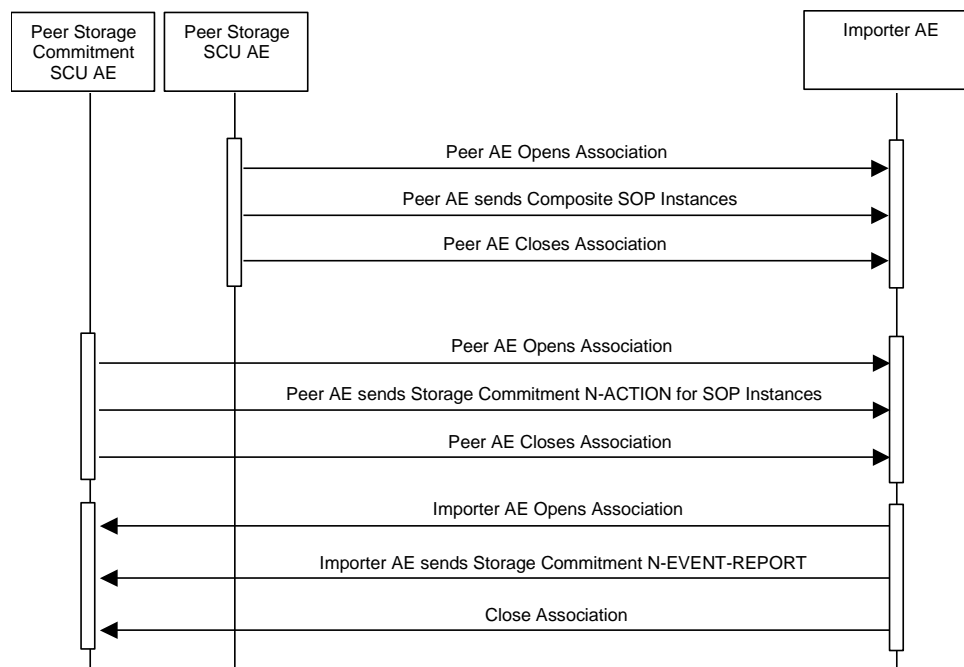

Note that the remote Storage Commitment SCU AE and Storage SCU AE could be a single AE, in which case the remote AE could send both the Composite SOP Instances and the Storage Commitment N-ACTION over the same Association. However, the Importer AE would still require that the Composite SOP Instances be sent before the Storage Commitment N-ACTION referencing them is sent.

The following sequencing constraints illustrated in Figure 3 apply to the Importer AE for handling Storage Commitment Push Model Requests using a new Association:

1. Remote AE opens an Association with the Importer AE.
2. Remote AE requests Storage Commitment of Composite SOP Instance(s) (remote sends N-ACTION-RQ and Importer AE responds with N-ACTION-RSP to indicate that it received the request).
3. Remote AE closes the Association before the Importer AE can successfully send the Storage Commitment Push Model Notification (N-EVENT-REPORT-RQ).
4. Importer AE opens a new Association with the remote AE.
5. Importer AE sends Storage Commitment Push Model Notification (N-EVENT-REPORT). More than one can be sent over a single Association if multiple Notifications are outstanding.
6. Importer AE closes the Association with the remote AE.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 35

### 3.2.2.3.1.2 Proposed Presentation Contexts

The Importer AE will propose Presentation Contexts as shown in the following table:

**Table 18: Importer AE Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

### 3.2.2.3.1.3 SOP Specific Conformance as an Association Requestor

#### 3.2.2.3.1.3.1 SOP Specific Conformance - Storage Commitment

Standard conformance is provided to the DICOM Storage Commitment Push Model SOP Class as an SCP.

The associated activity with the Storage Commitment Push Model Service is the communication by the Importer AE to remote AEs that it has committed to permanently store Composite SOP Instances that have been sent to it. It thus allows remote AEs to determine whether the McKesson Radiology™ system has taken responsibility for the archiving of specific SOP Instances so that they can be flushed from the remote AE system.

By default, the Importer AE will initiate a new Association to a remote AE that sent a Storage Commitment Push Model request only if the original Association over which this was sent is no longer open. Otherwise it will send the N-EVENT-REPORT Request over the original Association requested by the SCU. However, the Importer AE can be configured to always request a new Association to send the N-EVENT-REPORT Request.

The Importer AE creates files called Service Logs that can be used to monitor its status and diagnose any problems that may arise. If any error occurs during DICOM communication then appropriate messages are always output to these Service Logs. In addition, error messages may be output as alerts to the User Interface in certain cases.

If the request by the Importer AE to establish an Association fails for any reason (i.e. fail to connect with remote AE's TCP/IP port, Association Request is Rejected by remote AE, etc.) then the Importer AE will not try again later to send the N-EVENT-REPORT Request. If such a failure occurs then the remote AE will have to resend the Storage Commitment Push Model N-ACTION Request.

The Importer AE will exhibit the following Behavior according to the Status Code value returned in a Storage Commitment Push Model N-EVENT-REPORT Response from a destination SCU:

**Table 19: Importer AE N-EVENT-REPORT Response Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCU has successfully received the Storage Commitment report. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
Refused	Out of Resources	A700 – A7FF	This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Data Set does not match SOP Class	A900 – A9FF	This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Cannot	C000 –	This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-

Service Status	Further Meaning	Error Code	Behavior
	Understand	CFFF	REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Warning	Attribute List Error	0107	Storage Commitment report transmission is considered successful. A warning indication is output to the Service Logs. No indication is posted to the User Interface.
Warning	Attribute Value Out of Range	0116	Storage Commitment report transmission is considered successful. A warning indication is output to the Service Logs. No indication is posted to the User Interface.
*	*	Any other status code	This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.2.3.1.3.2 Association Requestor Communication Failure Behavior

The Behavior of the Importer AE during communication failure when it is acting as an Association Requestor is summarized in the following table:

**Table 20: Importer AE Communication Failure Behavior as an Association Requestor**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Association A-P-ABORTed by the SCU or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.2.4 Association Acceptance Policy

#### 3.2.2.4.1 Activity – Receive Images and Storage Commitment Requests


##### 3.2.2.4.1.1 Description and Sequencing of Activity

The Importer AE accepts Association Requests only if they propose one or more Presentation Contexts that the Importer AE actually supports. If none of the requested Presentation Contexts are accepted, then the Association Request itself is rejected. The Importer AE can be configured to only accept Associations requested by certain hosts (using TCP/IP address).

The default behavior of the Importer AE is to always attempt to send a Storage Commitment Push Model Notification (N-EVENT-REPORT) over the same Association opened by the remote AE to send the request (N-ACTION). If the Importer AE receives a request to close the Association either before sending the Notification or before receiving the corresponding N-EVENT-REPORT-RSP, then it will open a new Association to send the Notification. Refer to section 3.2.2.3 for the details.

In order to successfully handle Storage Commitment N-ACTION Requests, the Importer AE must have already received the referenced SOP Instances. That is, the Importer AE cannot properly handle a Storage Commitment N-ACTION Request that is sent to it before the SOP Instances it references are sent to the Importer

**Figure 4: Sequencing of Activity – Single Association for Storage and Storage Commitment**

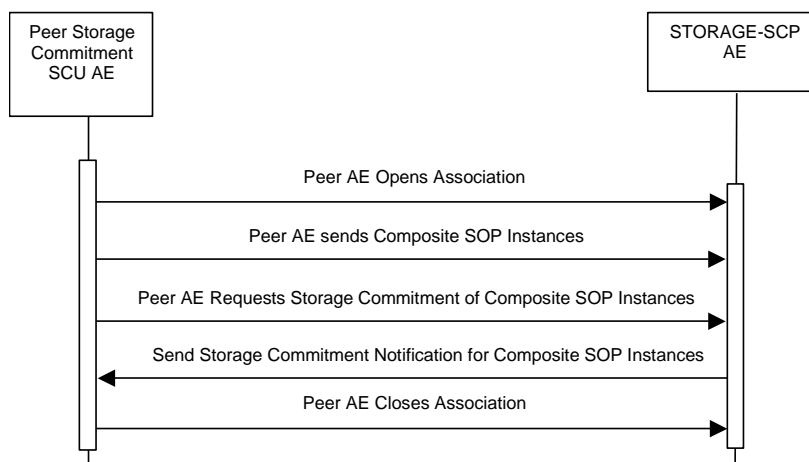

The following sequencing constraints illustrated in Figure 4 apply to the Importer AE for handling Storage Commitment Push Model Requests over the original Association:

1. Remote AE opens an Association with the Importer AE.
2. Remote AE sends zero or more Composite SOP Instances.
3. Remote AE requests Storage Commitment of Composite SOP Instance(s) (remote sends N-ACTION-RQ and Importer AE responds with N-ACTION-RSP to indicate that it received the request).
4. STORAGE-SCP AE sends Storage Commitment Push Model Notification request (N-EVENT-REPORT-RQ) and successfully receives Notification response (N-EVENT-REPORT-RSP) from remote AE.
5. Remote AE closes the Association.

If the Importer AE receives a request to close the Association from the remote AE before sending the Notification request (N-EVENT-REPORT-RQ) or when expecting to receive a Notification response (N-EVENT-REPORT-RSP), then it will open a new Association to send (or resend) the Notification. Refer to 3.2.2.2 for the details.

The Importer AE has a configurable timeout value for the maximum amount of time that it will wait on an open Association for a new request from a remote AE. A remote AE can reset this timer by sending a Verification request (C-ECHO-RQ). This can act as a useful mechanism for a remote AE to maintain an active Association if the length of time between sending Storage or Storage Commitment requests is long (such as when using a single Association to send images as they are acquired during an exam).

The Importer AE may reject Association attempts as shown in the Table below. The Result, Source and Reason/Diag columns represent the values returned in the corresponding fields of an ASSOCIATE-RJ PDU (see PS 3.8, Section 9.3.4). The following abbreviations are used in the Source column:

- a) 1 – DICOM UL service-user
- b) 2 – DICOM UL service-provider (ASCE related function)
- c) 3 – DICOM UL service-provider (Presentation related function)

**Table 21: Importer AE Association Rejection Reasons**

Result	Source	Reason/Diag	Explanation
2 – rejected-transient	c	2 – local-limit-exceeded	The (configurable) maximum number of simultaneous Associations has been reached. An Association request with the same parameters may succeed at a

Result	Source	Reason/Diag	Explanation
			later time.
1 – rejected-permanent	a	2 – application-context-name-not-supported	The Association request contained an unsupported Application Context Name. An association request with the same parameters will not succeed at a later time.
1 – rejected-permanent	b	1 – no-reason-given	The Association request could not be parsed. An Association request with the same format will not succeed at a later time. Usually this is only returned if the Importer AE has not been configured to allow the remote AE host to connect.

### 3.2.2.4.1.2 Accepted Presentation Contexts

The Importer AE will accept any **Presentation Context** containing:

1. An abstract syntax selected from Table 12
2. One or more Transfer Syntaxes selected from
3. Table 22

**Table 22: Importer AE Accepted Transfer Syntaxes**

Transfer Syntax		Role	Extended Negotiation
Name	UID		
DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
DICOM JPEG Baseline Process 1	1.2.840.10008.1.2.4.50	SCP	None
DICOM JPEG Extended Process 2 & 4	1.2.840.10008.1.2.4.51	SCP	None
DICOM JPEG Lossless Proc 14	1.2.840.10008.1.2.4.57	SCP	None
DICOM JPEG Lossless 1st Order Prediction	1.2.840.10008.1.2.4.70	SCP	None
DICOM JPEG 2000 (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
DICOM JPEG 2000	1.2.840.10008.1.2.4.91	SCP	None
DICOM RLE	1.2.840.10008.1.2.5	SCP	None
Wavelet (Private)	1.2.840.113711.1.2.100.1	SCP	None

NOTE1: The Wavelet Transfer Syntax is implemented using the Pegasus Imaging Corporation's Medical Image Toolkit.

### 3.2.2.4.1.3 SOP Specific Conformance as an Association Acceptor

#### 3.2.2.4.1.3.1 SOP Specific Conformance – Verification

The Importer AE provides standard conformance to the Verification SOP Class as an SCP.

#### 3.2.2.4.1.3.2 SOP Specific Conformance – Storage

The Importer AE does not have any dependencies on the number of Associations used to send images to it. Images belonging to more than one study or series can be sent over a single or multiple Associations. Images belonging to a single study or series can also be sent over different Associations. There is no limit on either the number of SOP Instances or the maximum amount of total SOP Instance data that can be transferred over a single Association.

The Importer AE provides Level 2 DICOM conformance to the Importing SOP Class. It is configured to retain the original DICOM data in DICOM Part 10 compliant file format. In addition, all Private and SOP Class Extended Elements are maintained in the DICOM format files.

In addition to saving all Elements in files, a subset of the Elements are stored in the McKesson Radiology™ system database to support query and retrieval requests and also allow updating of patient, study, and series information by user input, or demographic and study-related messages. Refer to Table 183:

Significant Elements in Received Images in the Annex for the list of Elements that are checked and/or processed upon receiving a Composite SOP Instance.

The associated Real-World Activity with the C-STORE service is the storage of medical imaging data on a designated hard disk. The Importer AE will return a failure status if it is unable to store the Composite SOP Instances onto the hard disk. After sending the C-STORE-RSP for a failure status, Importer AE will abort the association.

When receiving a compressed image from a C-STORE SCU, the Importer AE will not decompress and recompress an image to another compression format. Also, Importer AE shall not lossy compress an image that has already been subjected to lossy compression. How Importer AE performs this lossy compression check is by inspecting the value of the DICOM element (0028,2110) Lossy image processing in the DICOM image header. A value of 01 means the Image has been subjected to lossy compression and a value of 00 means the Image has NOT been subjected to lossy compression.

For the purposes of display, refer to Table 181: Supported Composite Image SOP Classes for Display in the Annex. In addition, information regarding the support for certain image-related characteristics can be found in Table 183.

It is preferred that optimal Window Center and Width values be specified in the DICOM Image Objects if they have greater than 8 bits of image data stored per sample. If optimal Window Center and Width values cannot be provided, then it is preferred that none are included, as McKesson Radiology™ is capable of estimating values using histogram analysis.

The Importer AE provides support for Storage Commitment Push Model. The Importer AE expects the SCU to open an Association, send one or more images, and then send the Storage Commitment Request for those images. The Importer will then send the N-EVENT Report over this same Association. If it cannot do so, then it will open a new Association with the SCU and send the N-EVENT-REPORT over the new Association.

The Importer AE returns one of the following status codes in a C-STORE Response:

**Table 23: Importer AE Returned C-STORE-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The Importer AE has successfully received, parsed, and saved to file the received C-STORE-RQ Composite SOP Instance. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
Refused	Out of Resources	A700	The Importer AE does not have enough disk space to store the C-STORE-RQ Composite SOP Instance. The SOP Instance will not be saved. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Data Set does not match SOP Class	A900	The Importer AE has determined that the C-STORE-RQ Composite SOP Instance is missing mandatory Elements specified for the SOP Class. This will only occur if the missing Elements or values prevent the Importer AE from successfully adding the Composite SOP Instance to the system database. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Cannot Understand	C000	Indicates that the Importer AE cannot parse the C-STORE-RQ Data Set. The SOP Instance will not be saved. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Warning	Coercion of Data Elements	B000	Indicates that the Importer AE coerced one or more Element values of the C-STORE-RQ Composite SOP Instance. Refer to Table 183: Significant Elements in Received Images of the Annex for descriptions of those Elements that can be coerced. Note that return of this status is normally disabled as some SCUs treat it as an Error code rather than a Warning.



Service Status	Further Meaning	Error Code	Behavior
			A warning indication is output to the Service Logs. No indication is posted to the User Interface.

The Importer will never delete any received images that can be successfully parsed and contain all the necessary information to add the image to the database (see the table of significant DICOM elements defined earlier). The images will always be archived to media of some sort (WORM, DLT etc.). Images are only flushed from the hard disk storage if they have been successfully archived to the media.

### 3.2.2.4.1.3.3 SOP Specific Conformance – Storage Commitment

The associated Activity with the Storage Commitment Push Model service is the communication by the Importer AE to remote AEs that it has committed to permanently store Composite SOP Instances that have been sent to it. It thus allows remote AEs to determine whether the McKesson Radiology™ system has taken responsibility for the archiving of specific SOP Instances so that they can be flushed from the remote AE system.

The Importer AE takes the list of Composite SOP Instance UIDs specified in a Storage Commitment Push Model N-ACTION Request and checks if they are present in the McKesson Radiology™ system database. As long as the Composite SOP Instance UIDs are present in the database, the Importer AE will consider those Composite SOP Instance UIDs to be successfully archived. The Importer AE does not require the Composite SOP Instances to actually be successfully written to archive media in order to commit to responsibility for maintaining these SOP Instances.

Once the Importer AE has checked for the existence of the specified Composite SOP Instances, it will then attempt to send the Notification request (N-EVENT-REPORT-RQ). The default behavior is to attempt to send this Notification over the same Association that was used by the remote AE to send the original N-ACTION Request. If the Association has already been released or Message transfer fails for some reason, then the Importer AE will attempt to send the N-EVENT-REPORT-RQ over a new Association. The Importer AE can be configured to always open a new Association in order to send the Notification request. Refer to 3.2.2.3.1.3 for SOP Specific Conformance when the Importer AE acts as an Association Requestor.

The Importer AE will not cache Storage Commitment Push Model N-ACTION Requests that specify Composite SOP Instances that have not yet been transferred to the Importer AE. If a remote AE sends a Storage Commitment Push Model N-ACTION Request before the specified Composite SOP Instances are later sent, the Importer AE will not commit to responsibility for such SOP Instances.

The Importer AE does not support the optional Storage Media File-Set ID & UID attributes in the N-ACTION Request.

The McKesson Radiology™ system never automatically deletes Composite SOP Instances from the archive. The absolute persistence of SOP Instances and the maximum archiving capacity for such SOP Instances is dependent on the archiving media and capacity used by the McKesson Radiology™ system and is dependent on the actual specifications of the purchased system. It is necessary to check the actual system specifications to determine these characteristics.

The Importer AE will support Storage Commitment Push Model requests for Composite SOP Instances of any of the Storage SOP Classes that are also supported by the Importer AE as an SCP. For a complete listing refer to Table 12: SOP Class Conformance of Importer AE.

The Importer AE returns one of the following status codes in an N-ACTION Response:

**Table 24: Importer AE Returned N-ACTION-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The Importer AE has successfully received the Storage Commitment Push Model

Service Status	Further Meaning	Error Code	Behavior
			N-ACTION Request and can process the commitment request for the indicated SOP Instances. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
Error	Processing Failure	0110	Indicates that the Storage Commitment Push Model N-ACTION Request cannot be parsed by the Importer AE or it cannot be fully processed due to a database or system failure. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Missing Attribute	0120	Indicates that the Storage Commitment Push Model N-ACTION Request cannot be processed by the Importer AE because a required attribute is missing from the N-ACTION Request Data Set. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Missing Attribute Value	0121	Indicates that the Storage Commitment Push Model N-ACTION Request cannot be processed because a Type 1 attribute in the N-ACTION Request Data Set does not specify a value. An error indication is output to the Service Logs. No indication is posted to the User Interface.

Refer to Table 19: Importer AE N-EVENT-REPORT Response Status Handling Behavior, for the behavior that the Importer AE will exhibit according to the Status Code value returned in a Storage Commitment Push Model N-EVENT-REPORT Response from a destination SCU.

#### 3.2.2.4.1.3.4 Association Acceptor Communication Failure Behavior

If a communication failure occurs while the Importer AE is trying to handle a Verification Service or Storage Service task or just waiting for the next Request Message on an open Association, then the Importer AE will exhibit the following behavior:

**Table 25: Importer AE Communication Failure Behavior as an Association Acceptor while handling a Verification or Storage Task**

Exception	Behavior
Timeout expiry for an expected DICOM Message Request (DIMSE level timeout). The default timeout for waiting on an open Association to receive the next DICOM Message is 60 minutes.	The Association is aborted using a DICOM A-P-ABORT. This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If any Composite SOP Instances have been successfully received and parsed prior to the failure, then they will still be archived rather than discarded.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout). The default timeout when trying to read from or write to an open socket is 3 minutes.	The Association is aborted using a DICOM A-P-ABORT. This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If any Composite SOP Instances have been successfully received and parsed prior to the failure, then they will still be archived rather than discarded.
Association A-ABORTed by the SCU or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If any Composite SOP Instances have been successfully received and parsed prior to the failure, then they will still be archived rather than discarded.

If a communication failure occurs while the Importer AE is trying to handle a Storage Commitment Push Model task (any point after a Storage Commitment N-ACTION-RQ has been received), then the Importer AE will exhibit the following behavior:

**Table 26: Importer AE Communication Failure Behavior as an Association Acceptor while handling a Storage Commitment Push Model Task**

Exception	Behavior
Timeout expiry for an expected DICOM Message Request (DIMSE level timeout). The default timeout for waiting on an open Association to receive the next DICOM Message is 60 minutes.	The Association is aborted using a DICOM A-P-ABORT. This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If a Storage Commitment N-ACTION-RQ has already been received, then the Importer AE will no longer try to process it, regardless of whether it has already sent the corresponding N-ACTION-RSP or N-EVENT-REPORT-RQ. The remote AE will have to resend the N-ACTION-RQ.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout). The default timeout when trying to read from or write to an open socket is 3 minutes.	The Association is aborted using a DICOM A-P-ABORT. This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If a Storage Commitment N-ACTION-RQ has already been received, then the Importer AE will no longer try to process it, regardless of whether it has already sent the corresponding N-ACTION-RSP or N-EVENT-REPORT-RQ. The remote AE will have to resend the N-ACTION-RQ.
Association A-ABORTed by the SCU or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If a Storage Commitment N-ACTION-RQ has already been received, then the Importer AE will no longer try to process it, regardless of whether it has already sent the corresponding N-ACTION-RSP or N-EVENT-REPORT-RQ. The remote AE will have to resend the N-ACTION-RQ.

#### 3.2.2.4.1.3.5 Presentation Context Acceptance Criterion

The Importer AE will only accept a Presentation Contexts specified by a SOP Class from Table 12 and having at least one Proposed Transfer Syntax from Table 22. More than one proposed Presentation Context will be accepted for the same Abstract Syntax if the Transfer Syntax is supported, whether or not it is the same as another Accepted Presentation Context.

The Importer AE can be configured to reject valid Presentation Contexts if the host for the remote AE is not listed in a local configuration file. In addition, a valid Presentation Context can be rejected if the maximum limit on the number of simultaneous processes has been reached.

The Importer AE does not check for and will accept duplicate Presentation Contexts.

#### 3.2.2.4.1.3.6 Transfer Syntax Selection Policies

The default behavior of the Importer AE supports the Implicit VR Little Endian and Explicit VR Little Endian Transfer Syntaxes for all Associations. In addition, some explicit JPEG Lossy and JPEG Lossless compression Transfer Syntaxes are supported, as defined in Table 22.

The JPEG 2000 Lossy, JPEG 2000 Lossless, RLE, and Wavelet (Private) Transfer Syntaxes can also be enabled via configuration; however, these are not enabled by default. The Importer AE can be configured to accept a subset of any of these syntaxes, with the inclusion of Implicit VR Little Endian being mandatory. It can also be configured to compress images once they are received using these various compression options.

The default preferred acceptance order for Transfer Syntaxes for the Importer AE (from highest preference to lowest) is: Little Endian Explicit, Little Endian Implicit, JPEG Lossy, and JPEG Lossless (if all these contexts are proposed). This order of preference is configurable.

### 3.2.3 Query/Retrieve Server AE Specification

#### 3.2.3.1 SOP Classes

The Query/Retrieve Server AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 27: SOP Class Conformance of Query/Retrieve Server AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	No	Yes
<b>Query/Retrieve</b>			
Patient Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	No	Yes
Patient Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	No	Yes
Study Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	No	Yes
Study Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	No	Yes
Patient Study Only Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	No	Yes
Patient Study Only Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	No	Yes
<b>Workflow Management</b>			
Modality Worklist Information Model	1.2.840.10008.5.1.4.31	No	Yes
<b>Transfer</b>			
12-lead ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	No
Ambulatory ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	No
Basic Voice Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	No
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	No
General Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.2	Yes	No
Arterial Pulse Waveform	1.2.840.10008.5.1.4.1.1.9.5.1	Yes	No
Respiratory Waveform	1.2.840.10008.5.1.4.1.1.9.6.1	Yes	No
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11	Yes	No
Comprehensive Structured Report	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	Yes	No
Mammography CAD Structured Report	1.2.840.10008.5.1.4.1.1.88.50	Yes	No
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Yes	No
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Yes	No
Colon CAD SR Document	1.2.840.10008.5.1.4.1.1.88.69	Yes	No
Implantation Plan SR Document	1.2.840.10008.5.1.4.1.1.88.70	Yes	No
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Yes	No
Encapsulated CDA IOD	1.2.840.10008.5.1.4.1.1.104.2	Yes	No
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Yes	No
CT Image	1.2.840.10008.5.1.4.1.1.2	Yes	No
Digital X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	Yes	No
Digital X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	No
Digital Mammography Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.2	Yes	No
Digital Mammography Image (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	No
Breast Tomosynthesis Image	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	No
Digital Intra-oral X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	Yes	No
Digital Intra-oral X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	No
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	No

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 44

DICOM SOP Class Name	SOP Class UID	SCU	SCP
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1	Yes	No
Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.2	Yes	No
Pseudo-Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.3	Yes	No
Blending Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.4	Yes	No
XA/XRF Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.5	Yes	No
Hardcopy Color Image	1.2.840.10008.5.1.1.1.30	Yes	No
Hardcopy Grayscale Image	1.2.840.10008.5.1.1.1.29	Yes	No
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	No
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	Yes	No
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	Yes	No
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	Yes	No
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Yes	No
MR Image	1.2.840.10008.5.1.4.1.1.4	Yes	No
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	No
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	Yes	No
Nuclear Medicine Image (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	No
Positron Emission Tomography Image	1.2.840.10008.5.1.4.1.1.128	Yes	No
Raw Data	1.2.840.10008.5.1.4.1.1.66	Yes	No
Spatial Registration	1.2.840.10008.5.1.4.1.1.66.1	Yes	No
Spatial Fiducials	1.2.840.10008.5.1.4.1.1.66.2	Yes	No
Deformable Spatial Registration	1.2.840.10008.5.1.4.1.1.66.3	Yes	No
Segmentation	1.2.840.10008.5.1.4.1.1.66.4	Yes	No
Surface Segmentation	1.2.840.10008.5.1.4.1.1.66.5	Yes	No
Real World Value Mapping	1.2.840.10008.5.1.4.1.1.67	Yes	No
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Yes	No
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Yes	No
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Yes	No
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	No
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Yes	No
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Yes	No
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Yes	No
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	No
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	No
RT Beams Delivery Instruction	1.2.840.10008.5.1.4.34.7	Yes	No
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Yes	No
Stand-alone Curve	1.2.840.10008.5.1.4.1.1.9	Yes	No
Stand-alone Modality LUT	1.2.840.10008.5.1.4.1.1.10	Yes	No
Stand-alone Overlay	1.2.840.10008.5.1.4.1.1.8	Yes	No
Stand-alone VOI LUT	1.2.840.10008.5.1.4.1.1.11	Yes	No
Standalone PET Curve	1.2.840.10008.5.1.4.1.1.129	Yes	No
Stored Print	1.2.840.10008.5.1.1.1.27	Yes	No
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Yes	No
Ultrasound Image (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	No
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Yes	No
Ultrasound Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	No
VL Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	No
VL Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	No
VL Slide-Coordinates Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	No
VL Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	No
VL Image (Retired)	1.2.840.10008.5.1.4.1.1.77.1	Yes	No

DICOM SOP Class Name	SOP Class UID	SCU	SCP
VL Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.77.2	Yes	No
Video Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1.1	Yes	No
Video Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2.1	Yes	No
Video Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4.1	Yes	No
Ophthalmic Photography 8 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.1	Yes	No
Ophthalmic Photography 16 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.2	Yes	No
Stereometric Relationship	1.2.840.10008.5.1.4.1.1.77.1.5.3	Yes	No
X-Ray Angiographic Bi-Plane Image (retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	No
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Yes	No
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Yes	No
X-Ray Radiation Dose Structured Report	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes
Lensometry Measurements	1.2.840.10008.5.1.4.1.1.78.1	Yes	No
Autorefractometry Measurements	1.2.840.10008.5.1.4.1.1.78.2	Yes	No
Keratometry Measurements	1.2.840.10008.5.1.4.1.1.78.3	Yes	No
Subjective Refraction Measurements	1.2.840.10008.5.1.4.1.1.78.4	Yes	No
Visual Acuity Measurements	1.2.840.10008.5.1.4.1.1.78.5	Yes	No
Spectacle Prescription Report	1.2.840.10008.5.1.4.1.1.78.6	Yes	No
Ophthalmic Axial Measurements	1.2.840.10008.5.1.4.1.1.78.7	Yes	No
Intraocular Lens Calculations	1.2.840.10008.5.1.4.1.1.78.8	Yes	No
Macular Grid Thickness and Volume Report	1.2.840.10008.5.1.4.1.1.79.1	Yes	No
Ophthalmic Visual Field Static Perimetry Measurements	1.2.840.10008.5.1.4.1.1.80.1	Yes	No
Basic Structured Display IOD	1.2.840.10008.5.1.4.1.1.131	Yes	No
Generic Implant Template	1.2.840.10008.5.1.4.43.1	Yes	No
Implant Assembly Template	1.2.840.10008.5.1.4.44.1	Yes	No
Implant Template Group	1.2.840.10008.5.1.4.45.1	Yes	No
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	Yes	No
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	Yes	No
Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	Yes	No
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Yes	No
Radiopharmaceutical Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.68	Yes	No

The Query/Retrieve Server AE implements SOP Classes of the Query/Retrieve Service Class as an SCP. It also supports the Modality Worklist SOP Class as an SCP. The Query/Retrieve Server AE can handle requests from external devices to query the McKesson Radiology™ system database for patient, study and series demographics, and Modality Worklists. It also handles requests for the retrieval of Composite SOP Instances.

The Query/Retrieve Server AE has one main task running on a McKesson Radiology™ system. It acts as an Association Acceptor, waiting for remote AEs acting as SCUs to request an Association. When the main task receives a request to open a new Association from a remote AE, it will spawn a child task for handling messages sent by the remote AE. These child tasks will both receive the query or retrieval requests sent by the remote AE and return any necessary responses with the matching information. In addition, a child process will attempt to handle any retrieval request by opening a new Association with the specified C-MOVE Destination AE and send any matching Composite SOP Instances over this Association. Thus, each child task can also act as an Association Requestor in addition to handling Associations requested by a remote AE. After each attempt to send a Composite SOP Instance using a C-STORE Request, a C-MOVE Response is sent to the remote AE that sent the retrieval request (the C-MOVE SCU) indicating whether the transfer was successful or not.

### 3.2.3.2 Association Establishment Policies

#### 3.2.3.2.1 General

The Query/Retrieve Server AE will accept Associations as an SCP for the Query/Retrieve Service C-FIND, and C-MOVE SOP Classes. It will also accept Associations as an SCP for the Modality Worklist SOP Class.

The Query/Retrieve Server AE will initiate Associations to send Composite SOP Instances in response to a C-MOVE Request. It will attempt to open a new Association with the C-MOVE Destination AE specified in the C-MOVE Request.

The DICOM Standard Application Context Name is always proposed:

**Table 28: DICOM Application Context for Query/Retrieve Server AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

### 3.2.3.2.2 Number of Associations

Each time the Query/Retrieve Server AE accepts an Association Request, a child process will be spawned to process any query or retrieval requests. The maximum number of child processes, and thus the maximum number of simultaneous Associations that can be processed, is set by configuration.

**Table 29: Number of Simultaneous Associations for Query/Retrieve Server AE acting as an SCP**

Maximum number of simultaneous Associations	Unlimited <sup>4</sup>
---	------------------------

If a child process receives a C-MOVE Request, then a new Association will also be requested by the Query/Retrieve Server AE in order to send images to the C-MOVE Destination AE. This means that each child process can also request a new Association and thus the Query/Retrieve Server AE can have multiple simultaneous requested Associations.

**Table 30: Number of Simultaneous Associations for Query/Retrieve Server AE acting as an SCU**

Maximum number of simultaneous Associations	Unlimited <sup>5</sup>
---	------------------------

### 3.2.3.2.3 Asynchronous Nature

Negotiation of multiple outstanding transactions is not supported.

**Table 31: Asynchronous Nature for Query/Retrieve Server AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

### 3.2.3.2.4 Implementation Identifying Information

**Table 32: DICOM Implementation Class and Version for Query/Retrieve Server AE**

Implementation Class UID	1.2.840.113711.3
Implementation Version Name	V1.0

### 3.2.3.3 Association Initiation Policy

#### 3.2.3.3.1 Activity – Remote AE requests the retrieval of images

##### 3.2.3.3.1.1 Description and Sequencing of Activity

<sup>4</sup> Default maximum is 10 per host permitted to connect to the Query/Retrieve Server AE.

<sup>5</sup> Default maximum is 10 per host permitted to connect to the Query/Retrieve Server AE.

When a remote AE submits a C-MOVE request to McKesson Radiology™, the Query/Retrieve Server AE looks in its database to find any matches for the submitted request. If there are Composite SOP Instances that match the C-MOVE request, then the Query/Retrieve Server AE will attempt to open an Association and transfer the requested SOP Instances. An Association Request is sent to the specified C-MOVE Destination AE and, upon successful negotiation of the required Presentation Context, the transfer is started. In all cases an attempt will be made to transmit all the indicated SOP Instances in a single Association, but this may not always be possible. The Association will be released when all the SOP Instances have been sent. If an error occurs during transmission over an open Association then the transfer is halted. The Query/Retrieve Server AE will not attempt to independently retry the image export.

The Query/Retrieve Server AE does not support the unsolicited sending of SOP Instances using the DICOM Storage Service Class. It will only send SOP Instances in response to a C-MOVE Request from a remote AE.

### **3.2.3.3.1.2 Proposed Presentation Contexts**

The Query/Retrieve Server AE can propose the same Presentation Contexts as the Sender AE when it attempts to transfer Composite SOP Instances in response to a C-MOVE Request. As such, it can propose any one or more of the Transfer Syntaxes in Table 9: Sender AE Proposed Transfer Syntaxes for each of the abstract syntaxes listed in Table 4: SOP Class Conformance of Sender AE (same as SOP Classes with Role of SCU listed in Table 27: SOP Class Conformance of Query/Retrieve Server AE). Each proposed Presentation Context contains a single Transfer Syntax. Multiple Transfer Syntaxes per abstract syntax would be proposed with multiple Presentation Contexts.

### **3.2.3.3.1.3 SOP Specific Conformance as an Association Requestor**

#### **3.2.3.3.1.3.1 SOP Specific Conformance - Storage**

The Query/Retrieve Server AE will attempt to transfer all requested SOP Instances to the C-MOVE Destination AE specified in a C-MOVE Request. For each C-STORE Response received from the C-MOVE Destination AE, the Query/Retrieve Server AE will return a C-MOVE Response to the AE that sent the original C-MOVE Request. Each C-MOVE Response will indicate the appropriate Status Code based on the Status Code of the corresponding C-STORE Response. The Association will be properly released after the Query/Retrieve Server AE has attempted to transfer all requested SOP Instances. The Query/Retrieve Server AE will continue to attempt to transfer any remaining SOP Instances even if a failure Status Code is returned in a particular C-STORE Response.

When a Composite SOP Instance is selected for transmission from McKesson Radiology™, the content of the object will be the same as when it was originally received unless patient demographic or study-related information is altered. In such cases, the latest values in the database will replace the original information in the SOP Instance. Thus, the set of optional tags contained in DICOM objects going out from McKesson Radiology™ depends on the information that was received. For the list of patient, study, and series attributes that can be updated by the Query/Retrieve Server AE when a SOP Instance is exported please refer to 7.1.5: Sender AE and Query/Retrieve Server AE Element Modification

The Query/Retrieve Server AE cannot be configured to automatically resend Composite SOP Instances when the Status Code returned in a C-STORE Response is considered to indicate a failure. Failure indications are not output to the User Interface if an error occurs during the handling of a C-MOVE retrieval request.

The Query/Retrieve Server AE will exhibit the following behavior according to the Status Code value returned in a C-STORE Response from the C-STORE SCP (the C-MOVE Destination AE):



**Table 33: Query/Retrieve Server AE C-STORE Response Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has successfully stored the exported SOP Instance. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
Refused	Out of Resources	A700 – A7FF	This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend the SOP Instance. However, it will continue trying to send any remaining SOP Instances requested by the C-MOVE-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Data Set does not match SOP Class	A900 – A9FF	This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend the SOP Instance. However, it will continue trying to send any remaining SOP Instances requested by the C-MOVE-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Error	Cannot Understand	C000 – CFFF	This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend the SOP Instance. However, it will continue trying to send any remaining SOP Instances requested by the C-MOVE-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Warning	Coercion of Data Elements	B000	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. No indication is posted to the User Interface.
Warning	Element Discarded	B006	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. No indication is posted to the User Interface.
Warning	Data Set does not match SOP Class	B007	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. No indication is posted to the User Interface.
Warning	Attribute List Error	0107	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. No indication is posted to the User Interface.
Warning	Attribute Value Out of Range	0116	SOP Instance transmission is considered successful. A warning indication is output to the Service Logs so that there is a record of the SCP returning a Warning Status. No indication is posted to the User Interface.
*	*	Any other status code	This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend the SOP Instance. However, it will continue trying to send any remaining SOP Instances requested by the C-MOVE-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 49

### 3.2.3.3.1.3.2 Association Requestor Communication Failure Behavior

The Behavior of the Query/Retrieve Server AE during communication failure when acting as an Association Requestor is summarized in the following table:

**Table 34: Query/Retrieve Server AE Communication Failure Behavior as an Association Requestor**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend any of the SOP Instances that were not successfully transferred. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend any of the SOP Instances that were not successfully transferred. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. The Query/Retrieve Server AE does not attempt to resend any of the SOP Instances that were not successfully transferred. An error indication is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.3.4 Association Acceptance Policy


#### 3.2.3.4.1 Activity – External system queries McKesson Radiology™

##### 3.2.3.4.1.1 Description and Sequencing of Activity

The Query/Retrieve Server AE accepts Associations only if they have valid Presentation Contexts. If none of the requested Presentation Contexts are accepted, then the Association Request itself is rejected. It can be configured to only accept Associations with certain hosts (using TCP/IP address) and/or Application Entity Titles.

If the Query/Retrieve Server AE receives a query (C-FIND) request, then the response(s) will be sent over the same Association used to send the C-FIND-Request.

If the Query/Retrieve Server AE receives a retrieval (C-MOVE) request, then the responses will be sent over the same Association used to send the C-MOVE-Request. The Query/Retrieve Server AE will send the requested Composite SOP Instances to the C-MOVE Destination AE. After each attempt to send a SOP Instance, the Query/Retrieve Server AE sends a C-MOVE Response indicating whether the transfer was successful or not. Once the Query/Retrieve Server AE has finished attempting to transfer all the requested SOP Instances, it sends a final C-MOVE Response indicating the overall status of the attempted retrieval.

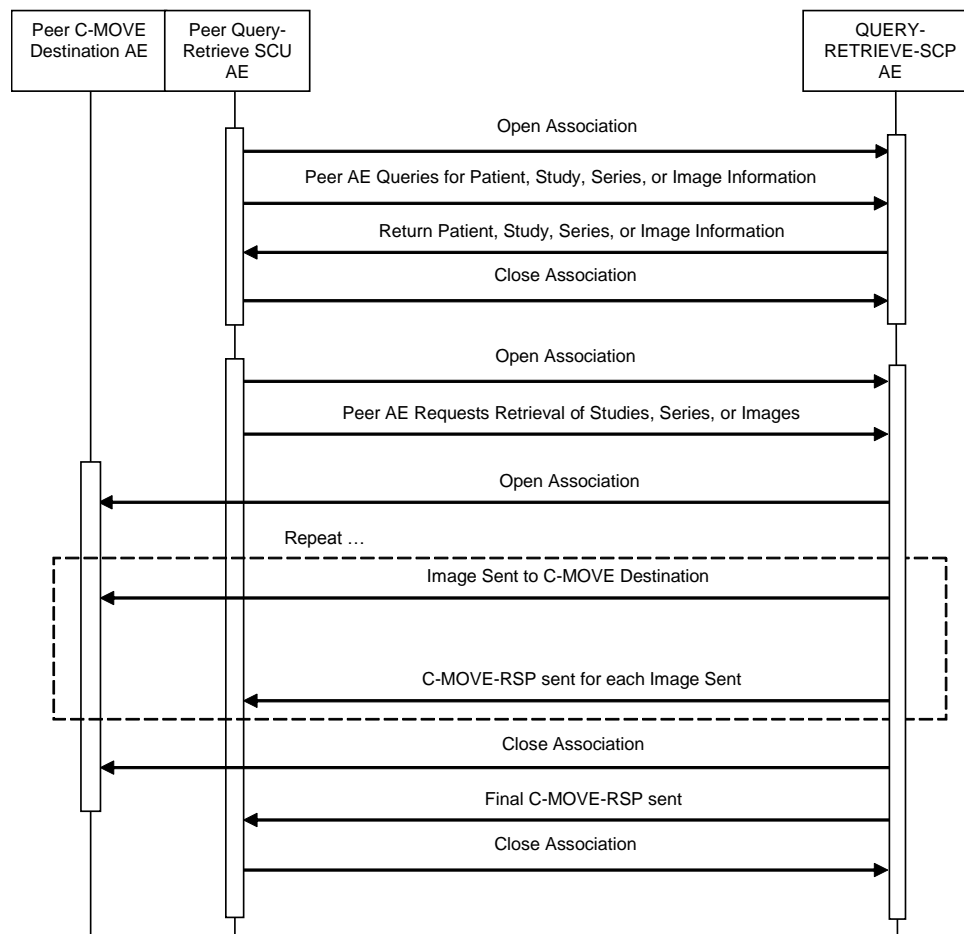**Figure 5: Sequencing of Activity – Handling Query and Retrieval Requests**

The following sequencing constraints illustrated in figure 5 apply to the Query/Retrieve Server AE for handling queries (C-FIND-Requests):

1. Remote AE opens an Association with the Query/Retrieve Server AE.
2. Remote AE sends a C-FIND-RQ Message
3. Query/Retrieve Server AE returns a C-FIND-RSP Message to the remote AE with matching information. A C-FIND-RSP is sent for each entity matching the identifier specified in the C-FIND-RQ. A final C-FIND-RSP is sent indicating that the matching is complete.
4. Remote AE closes the Association. Note that the remote AE does not have to close the Association immediately. Further C-FIND or C-MOVE Requests can be sent over the Association before it is closed.

The following sequencing constraints illustrated in figure 5 apply to the Query/Retrieve Server AE for handling retrievals (C-MOVE-Requests):

1. Remote AE opens an Association with the Query/Retrieve Server AE.
2. Remote AE sends a C-MOVE-RQ Message
3. Query/Retrieve Server AE sends the Composite SOP Instances to the remote C-MOVE Destination AE as indicated in the C-MOVE-RQ.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 51

4. After each attempt to send a SOP Instance, the Query/Retrieve Server AE returns a C-MOVE-RSP indicating this success or failure of the transfer.
5. Once the Query/Retrieve Server AE has completed all attempts to transfer the SOP Instances to the C-MOVE Destination AE, the Query/Retrieve Server AE sends a final C-MOVE-RSP indicating the overall success or failure of the retrieval.
6. Remote AE closes the Association. Note that the remote AE does not have to close the Association immediately. Further C-FIND or C-MOVE Requests can be sent over the Association before it is closed.

The Query/Retrieve Server AE may reject Association attempts as shown in the table below. The Result, Source and Reason/Diag columns represent the values returned in the corresponding fields of an ASSOCIATE-RJ PDU (see PS 3.8, Section 9.3.4). The following abbreviations are used in the Source column:

- a) 1 – DICOM UL service-user
- b) 2 – DICOM UL service-provider (ASCE related function)
- d) 3 – DICOM UL service-provider (Presentation related function)

**Table 35: Query/Retrieve Server AE Association Rejection Reasons**

Result	Source	Reason/Diag	Explanation
2 – rejected-transient	c	2 – local-limit-exceeded	The (configurable) maximum number of simultaneous Associations for the remote AE host has been reached. An Association request with the same parameters may succeed at a later time.
1 – rejected-permanent	a	2 – application-context-name-not-supported	The Association request contained an unsupported Application Context Name. An association request with the same parameters will not succeed at a later time.
1 – rejected-permanent	b	1 – no-reason-given	The Association request could not be parsed. An Association request with the same format will not succeed at a later time. Usually this is only returned if the Query/Retrieve Server AE has not been configured to allow the remote AE host to connect to it. The Query/Retrieve Server AE can be configured to allow only specific host names to open Associations with it. Note that it cannot currently be configured to only allow specific calling and/or called AE Titles when forming Associations.

### 3.2.3.4.1.2 Accepted Presentation Contexts

The Query/Retrieve Server AE may accept any one or more of the following Presentation Contexts:

**Table 36: Query/Retrieve Server AE Accepted Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Patient Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Patient Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Patient Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Patient Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Study Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Study Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Study Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Study Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Patient Study Only Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Patient Study Only Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Patient Study Only Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Patient Study Only Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Modality Worklist Information Model	1.2.840.10008.5.1.4.31	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Modality Worklist Information Model	1.2.840.10008.5.1.4.31	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None

### 3.2.3.4.1.3 SOP Specific Conformance as an Association Acceptor

#### 3.2.3.4.1.3.1 SOP Specific Conformance – Verification

Standard conformance is provided to the DICOM Verification Service Class as an SCP.

#### 3.2.3.4.1.3.2 SOP Specific Conformance – Query (C-FIND)

The Query/Retrieve Server AE supports hierarchical queries and not relational queries. There are no attributes always returned by default. Only those attributes requested in the query identifier are returned. Query responses always return values from the McKesson Radiology™ database. Exported SOP Instances are always updated with the latest values in the database prior to export. Thus, a change in patient demographic information will be contained in both the C-FIND Responses and any Composite SOP Instances exported to a C-MOVE Destination AE.

By default, the Query/Retrieve Server AE is configured to not check for Cancel Requests sent by a remote AE. This is done to improve performance, as it does not have to spend time periodically checking if a remote AE has sent a Cancel Request over the Association. However, if it is known that a remote AE can send Cancel Requests, then the Query/Retrieve Server AE can be configured to handle them properly.

The Query/Retrieve Server AE implements support for the IHE Technical Framework version 5.5 (Year 6). All required attributes are supported at the Patient, Study, Series and Image levels.

#### Patient Root Information Model

All required search keys on each of the four levels (Patient, Study, Series, and Image) are supported. However, the Patient ID (0010,0020) key must be fully stated if the Patient's Name (0010,0010) is not present in the query (e.g. McKesson Radiology™ does not support queries for patients having the patient ID of "123\*" when this is the only search criterion).

#### Study Root Information Model

All the required search keys on each of the three levels (Study, Series, and Image) are supported. There is, however, a caveat that applies to the Study Time (0008,0030) — it cannot be used as the only search key on the Study level. If it is used in conjunction with the other supported search keys on the Study level, it can be used in the matching criteria.

#### Patient/Study Only Information Model

All the required search keys on the Patient and Study levels are supported. The Patient ID (0010,0020) key must be fully stated if the Patient's Name (0010,0010) is not present in the query.

**Table 37: Patient Root C-FIND SCP Supported Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient's Name (See NOTE7)	0010,0010	PN	S,*,U also DICOM

			FUZZY LOGIC if MIMA
Patient ID	0010,0020	LO	UNIQUE
Issuer of Patient ID (See NOTE3)	0010,0021	LO	S,U (MIMA), NONE otherwise.
Other patient IDs Sequence (See NOTE4)	0010,1002	SQ	SQ
> Patient ID	0010,0020	LO	NONE
>Issuer of Patient ID	0010,0021	LO	NONE
Patient's Birth Date	0010,0030	DA	S,U
Patient's Birth Time	0010,0032	TM	S,U
Patient's Sex	0010,0040	CS	S,U
Patient's Weight	0010,1030	DS	NONE
Medical Alerts	0010,2000	LO	NONE
Contrast Allergies	0010,2110	LO	NONE
Pregnancy Status	0010,21C0	US	NONE
<b>Study Level</b>			
Study Date	0008,0020	DA	S,R,U
Study Time	0008,0030	TM	R,U
Accession Number	0008,0050	SH	S,*,U
Issuer of Accession Number Sequence (See NOTE5)	0008,0051	SQ	SQ
>Local Namespace Entity ID	0040,0031	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID	0040,0032	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID Type	0040,0033	CS	S,U (MIMA), NONE otherwise
Study ID	0020,0010	SH	S,*,U
Study Instance UID	0020,000D	UI	UNIQUE,L
Referring Physician's Name	0008,0090	PN	S,*,U
Study Description	0008,1030	LO	S,*,U
Modalities in Study	0008,0061	CS	S,*,U
Number of Study Related Series	0020,1206	IS	NONE
Number of Study Related Instances	0020,1208	IS	NONE
Instance Availability (see NOTE2)	0008,0056	CS	NA
<b>Series Level</b>			
Modality	0008,0060	CS	S,U
Series Number	0020,0011	IS	S,*,U
Series Instance UID	0020,000E	UI	UNIQUE,L
Number of Series Related Instances	0020,1209	IS	NONE
Performing Physician's Name (see NOTE1)	0008,1050	PN	S,*,U
Operator's Name	0008,1070	PN	S,*,U
Series Description	0008,103E	LO	S,*,U
Request Attribute Sequence	0040,0275	SQ	SQ
>Requested Procedure ID	0040,1001	SH	S,*,U
>Scheduled Procedure Step ID	0040,0009	SH	S,*,U
Performed Procedure Step Start Date	0040,0244	DA	S,R,U
Performed Procedure Step Start Time	0040,0245	TM	R,U
Instance Availability (see NOTE2)	0008,0056	CS	NA
Institution Name (See NOTE6)	0008,0080	LO	NONE
Institution Code Sequence (See NOTE6)	0008,0082	SQ	SQ
>Code Value	0008,0100	SH	S,U (MIMA), NONE otherwise

>Coding Scheme Designator	0008,0102	SH	S,U (MIMA), NONE otherwise
>Coding Scheme Version	0008,0103	SH	S,U (MIMA), NONE otherwise
>Code Meaning	0008,0104	LO	S,U (MIMA), NONE otherwise
<b>Image Level</b>			
SOP Instance UID	0008,0018	UI	UNIQUE,L
SOP Class UID	0008,0016	UI	U,L
Content Date	0008,0023	DA	NONE
Content Time	0008,0033	TM	NONE
Retrieve AE Title	0008,0054	AE	NONE
Referenced Series Sequence	0008,1115	SQ	SQ
>Series Instance UID	0020,000E	UI	NONE
>Referenced Image Sequence	0008,1140	SQ	SQ
>>Referenced SOP Class UID	0008,1150	UI	NONE
>>Referenced SOP Instance UID	0008,1155	UI	NONE
Instance Number	0020,0013	IS	S,U
Rows	0028,0010	US	NONE
Columns	0028,0011	US	NONE
Bits Allocated	0028,0100	US	NONE
Number of Frames	0028,0008	IS	NONE
Observation DateTime	0040,A032	DT	NONE
Concept Name Code Sequence	0040,A043	SQ	SQ
>Code Value	0008,0100	SH	S*,U
>Coding Scheme Designator	0008,0102	SH	S*,U
>Coding Scheme Version	0008,0103	SH	NONE
>Code Meaning	0008,0104	LO	NONE
Verifying Observer Sequence	0040,A073	SQ	SQ
>Verifying Organization	0040,A027	LO	NONE
>Verification DateTime	0040,A030	DT	S,R,U
>Verifying Observer Name	0040,A075	PN	S*,U
>Verifying Observer Identification Code Sequence	0040,A088	SQ	SQ
>>Code Value	0008,0100	SH	NONE
>>Coding Scheme Designator	0008,0102	SH	NONE
>>Coding Scheme Version	0008,0103	SH	NONE
>>Code Meaning	0008,0104	LO	NONE
Referenced Request Sequence	0040,A370	SQ	SQ
>Accession Number	0008,0050	SH	NONE
>Study Instance UID	0020,000D	UI	NONE
>Requested Procedure Code Sequence	0032,1064	SQ	SQ
>>Code Value	0008,0100	SH	NONE
>>Coding Scheme Designator	0008,0102	SH	NONE
>>Coding Scheme Version	0008,0103	SH	NONE
>>Code Meaning	0008,0104	LO	NONE
>Requested Procedure ID	0040,1001	SH	NONE
Completion Flag	0040,A491	CS	S*,U
Verification Flag	0040,A493	CS	S*,U
Content Template Sequence	0040,A504	SQ	SQ
>Template Identifier	0040,DB00	CS	NONE
Presentation Label	0070,0080	CS	NONE

Presentation Description	0070,0081	LO	NONE
Presentation Creation Date	0070,0082	DA	NONE
Presentation Creation Time	0070,0083	TM	NONE
Presentation Creator's Name	0070,0084	PN	NONE
Instance Availability (see NOTE2)	0008,0056	CS	NA

**Table 38: Study Root C-FIND SCP Supported Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Study Level</b>			
Patient's Name (See NOTE7)	0010,0010	PN	S,*,U also DICOM FUZZY LOGIC if MIMA
Patient ID	0010,0020	LO	S,U
Issuer of Patient ID (See NOTE 3)	0010,0021	LO	S,U (MIMA), NONE otherwise.
Other patient IDs Sequence (See NOTE4)	0010,1002	SQ	SQ
> Patient ID	0010,0020	LO	NONE
>Issuer of Patient ID	0010,0021	LO	NONE
Patient's Birth Date	0010,0030	DA	S,U
Patient's Birth Time	0010,0032	TM	S,U
Patient's Sex	0010,0040	CS	S,U
Patient's Weight	0010,1030	DS	NONE
Medical Alerts	0010,2000	LO	NONE
Contrast Allergies	0010,2110	LO	NONE
Pregnancy Status	0010,21C0	US	NONE
Study Date	0008,0020	DA	S,R,U
Study Time	0008,0030	TM	R,U
Accession Number	0008,0050	SH	S,*,U
Issuer of Accession Number Sequence (See NOTE5)	0008,0051	SQ	SQ
>Local Namespace Entity ID	0040,0031	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID	0040,0032	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID Type	0040,0033	CS	S,U (MIMA), NONE otherwise
Study ID	0020,0010	SH	S,*,U
Study Instance UID	0020,000D	UI	UNIQUE,L
Referring Physician's Name	0008,0090	PN	S,*,U
Study Description	0008,1030	LO	S,*,U
Modalities in Study	0008,0061	CS	S,*,U
Number of Study Related Series	0020,1206	IS	NONE
Number of Study Related Instances	0020,1208	IS	NONE
Instance Availability (see NOTE2)	0008,0056	CS	NA
<b>Series Level</b>			
Modality	0008,0060	CS	S,U
Series Number	0020,0011	IS	S,*,U
Series Instance UID	0020,000E	UI	UNIQUE,L
Number of Series Related Instances	0020,1209	IS	NONE
Performing Physician's Name (see NOTE1)	0008,1050	PN	S,*,U
Operator's Name	0008,1070	PN	S,*,U
Series Description	0008,103E	LO	S,*,U



Request Attribute Sequence	0040,0275	SQ	SQ
>Requested Procedure ID	0040,1001	SH	S,*,U
>Scheduled Procedure Step ID	0040,0009	SH	S,*,U
Performed Procedure Step Start Date	0040,0244	DA	S,R,U
Performed Procedure Step Start Time	0040,0245	TM	R,U
Instance Availability (see NOTE2)	0008,0056	CS	NA
Institution Name (See NOTE6)	0008,0080	LO	NONE
Institution Code Sequence (See NOTE6)	0008,0082	SQ	SQ
>Code Value	0008,0100	SH	S,U (MIMA), NONE otherwise
>Coding Scheme Designator	0008,0102	SH	S,U (MIMA), NONE otherwise
>Coding Scheme Version	0008,0103	SH	S,U (MIMA), NONE otherwise
>Code Meaning	0008,0104	LO	S,U (MIMA), NONE otherwise
<b>Image Level</b>			
SOP Instance UID	0008,0018	UI	UNIQUE,L
SOP Class UID	0008,0016	UI	U,L
Content Date	0008,0023	DA	NONE
Content Time	0008,0033	TM	NONE
Retrieve AE Title	0008,0054	AE	NONE
Referenced Series Sequence	0008,1115	SQ	SQ
>Series Instance UID	0020,000E	UI	NONE
>Referenced Image Sequence	0008,1140	SQ	SQ
>>Referenced SOP Class UID	0008,1150	UI	NONE
>>Referenced SOP Instance UID	0008,1155	UI	NONE
Instance Number	0020,0013	IS	S,U
Rows	0028,0010	US	NONE
Columns	0028,0011	US	NONE
Bits Allocated	0028,0100	US	NONE
Number of Frames	0028,0008	IS	NONE
Observation DateTime	0040,A032	DT	NONE
Concept Name Code Sequence	0040,A043	SQ	SQ
>Code Value	0008,0100	SH	S,*,U
>Coding Scheme Designator	0008,0102	SH	S,*,U
>Coding Scheme Version	0008,0103	SH	NONE
>Code Meaning	0008,0104	LO	NONE
Verifying Observer Sequence	0040,A073	SQ	SQ
>Verifying Organization	0040,A027	LO	NONE
>Verification DateTime	0040,A030	DT	S,R,U
>Verifying Observer Name	0040,A075	PN	S,*,U
>Verifying Observer Identification Code Sequence	0040,A088	SQ	SQ
>>Code Value	0008,0100	SH	NONE
>>Coding Scheme Designator	0008,0102	SH	NONE
>>Coding Scheme Version	0008,0103	SH	NONE
>>Code Meaning	0008,0104	LO	NONE
Referenced Request Sequence	0040,A370	SQ	SQ
>Accession Number	0008,0050	SH	NONE
>Study Instance UID	0020,000D	UI	NONE
>Requested Procedure Code Sequence	0032,1064	SQ	SQ

>>Code Value	0008,0100	SH	NONE
>>Coding Scheme Designator	0008,0102	SH	NONE
>>Coding Scheme Version	0008,0103	SH	NONE
>>Code Meaning	0008,0104	LO	NONE
>Requested Procedure ID	0040,1001	SH	NONE
Completion Flag	0040,A491	CS	S,*,U
Verification Flag	0040,A493	CS	S,*,U
Content Template Sequence	0040,A504	SQ	SQ
>Template Identifier	0040,DB00	CS	NONE
Presentation Label	0070,0080	CS	NONE
Presentation Description	0070,0081	LO	NONE
Presentation Creation Date	0070,0082	DA	NONE
Presentation Creation Time	0070,0083	TM	NONE
Presentation Creator's Name	0070,0084	PN	NONE
Instance Availability (see NOTE2)	0008,0056	CS	NA

**Table 39: Patient/Study Only Root C-FIND SCP Supported Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient's Name (See NOTE7)	0010,0010	PN	S,*,U also DICOM FUZZY LOGIC if MIMA
Patient ID	0010,0020	LO	UNIQUE
Issuer of Patient ID (See NOTE3)	0010,0021	LO	S,U (MIMA), NONE otherwise.
Other patient IDs Sequence (See NOTE4)	0010,1002	SQ	SQ
> Patient ID	0010,0020	LO	NONE
>Issuer of Patient ID	0010,0021	LO	NONE
Patient's Birth Date	0010,0030	DA	S,U
Patient's Birth Time	0010,0032	TM	S,U
Patient's Sex	0010,0040	CS	S,U
Patient's Weight	0010,1030	DS	NONE
Medical Alerts	0010,2000	LO	NONE
Contrast Allergies	0010,2110	LO	NONE
Pregnancy Status	0010,21C0	US	NONE
<b>Study Level</b>			
Study Date	0008,0020	DA	S,R,U
Study Time	0008,0030	TM	R,U
Accession Number	0008,0050	SH	S,*,U
Issuer of Accession Number Sequence (See NOTE5)	0008,0051	SQ	SQ
>Local Namespace Entity ID	0040,0031	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID	0040,0032	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID Type	0040,0033	CS	S,U (MIMA), NONE otherwise
Study ID	0020,0010	SH	S,*,U
Study Instance UID	0020,000D	UI	UNIQUE,L
Referring Physician's Name	0008,0090	PN	S,*,U
Study Description	0008,1030	LO	S,*,U
Modalities in Study	0008,0061	CS	S,*,U
Number of Study Related Series	0020,1206	IS	NONE

Number of Study Related Instances	0020,1208	IS	NONE
Performing Physician's Name (see NOTE1)	0008,1050	PN	S,*,U
Instance Availability (see NOTE2)	0008,0056	CS	NA

The types of Matching supported by the Query/Retrieve Server AE Query (C-FIND) SCP:

- S - indicates Single Value Matching is supported.
- R - indicates Range Matching is supported.
- \* - indicates Wildcard Matching is supported.
- U - indicates Universal Matching is supported.
- L - indicates that UID lists Matching are supported.
- SQ - indicates that Sequence Matching is supported.
- NONE - indicates that no matching is supported, but that values for this Element are returned if requested (i.e. universal matching).
- UNIQUE - indicates that this is the Unique Key for that query level, in which case Universal Matching or Single Value Matching is supported depending on the query level.
- NA - indicates that no matching is supported, but the values for this Element will be returned whether it is requested or not.
- DICOM - indicates DICOM Fuzzy Semantic Matching (MIMA) support so that variations in the spelling of a patient's name in different domains, phonetic matching (e.g. a query for Swain" might as well return "Swayne"), or patient name components order-insensitivity (e.g. a query for "Smith^Mary" might well return "Mary^Smith") can still be handled.
- FUZZY - However, McKesson Radiology™ shall only support case-insensitivity of patient name.
- LOGIC

NOTE1: By default, McKesson Radiology™ returns Performing Physician's Name (0008,1050) at the Series Level. However, it can be configured to return it at the Study Level.

NOTE2: McKesson Radiology™ supports the Instance Availability attribute (0008,0056) which defines how rapidly composite object instance(s) become available for transmission from McKesson Radiology™ after a C-MOVE retrieval request. McKesson Radiology™ will return one of three possible values for this attribute:

- "ONLINE" if all the SOP Instances are immediately available because they all have a cache location.
- "NEARLINE" if all SOP Instances can be retrieved from accessible archive locations, even if some do not have a cache location.
- "OFFLINE" if some of the SOP Instances are archived, but they are not accessible from their archived location(s).

McKesson Radiology™ supporting the Multiple Identity Resolution option of the IHE MIMA Profile shall support the query match keys as a Query SCP in the above tables. McKesson Radiology™ shall handle Patient ID and Accession Number Assigning Authorities, and Institution Information in Queries as follows:

NOTE3: Patient ID Assigning Authority in Queries

McKesson Radiology™ receiving query requests shall establish the Assigning Authority of an included Patient ID value from the Issuer of Patient ID (0010,0021) attribute that is explicitly present in the received query request identifier, or if absent, from the preconfigured Assigning Authority of the Patient ID associated with the querying system.

If there is no Patient ID (0010,0020) value included in the query request then McKesson Radiology™ shall establish the Patient ID Assigning Authority to be used for all responses from the Issuer of Patient ID (0010,0021) attribute that is explicitly present in the received query request identifier, or if absent, from the preconfigured Assigning Authority of the patient ID associated with the querying system.

The value of a returned Patient ID (0010,0020) shall correspond to the Assigning Authority specified in the query, or if absent, the preconfigured Assigning Authority associated with the querying system. McKesson Radiology™ shall use its knowledge of the cross-referencing of

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 59

patient identifiers to return the appropriate Patient ID value. If there is no such patient ID then it shall be returned zero length.

**NOTE4: Other Patient IDs in Queries**

McKesson Radiology™ shall be capable of including all patient identifiers known to it in the Other Patient IDs Sequence (0010,1002) as a list of return key values.

At a minimum McKesson Radiology™ shall include in the Other Patient IDs Sequence (0010,1002) the destination patient ID value, if it exists.

**NOTE5: Accession Number Assigning Authority in Queries**

McKesson Radiology™ receiving query requests shall establish the Assigning Authority of an included Accession Number value from the Issuer of Accession Number Sequence (0008,0051) attribute that is explicitly present in the received query request identifier, or if absent, from the preconfigured Assigning Authority of the Accession Number associated with the querying system.

If there is no Accession Number (0008,0050) value included in the query request then McKesson Radiology™ shall establish the Accession Number Assigning Authority to be used for all responses from the Accession Number Sequence (0008,0051) attribute that is explicitly present in the received query request identifier, or if absent, from the preconfigured Assigning Authority of the Accession Number associated with the querying system.

The value of a returned Accession Number shall correspond to the Assigning Authority specified in the query, or if absent, the preconfigured Assigning Authority associated with the querying system. If the Accession Number of a matching Study does not correspond to this Assigning Authority then it shall be returned zero length.

In the case where the Issuer of Accession Number Sequence (0008,0051) attribute is sent with no value, McKesson Radiology™ can return Accession Number values from any Assigning Authority.

**NOTE6: Institution in Queries**

McKesson Radiology™ receiving query requests shall support Institution Code Sequence (0008,0082) as a Matching Key for Series, or SOP Instances acquired at a certain Institution. The Institution Name (0008,0080) attribute value shall be included in the query response if the attribute is included in the Query identifier.

**NOTE7: DICOM Fuzzy Semantic Matching**

McKesson Radiology™ supporting the Multiple Identity Resolution option shall support the DICOM Fuzzy Semantic Matching of Person Names option. However, McKesson Radiology™ shall only support the case-insensitivity of patient name. We do not support the true variations in the spelling of a patient's name.

The Query/Retrieve Server AE returns one of the following status codes in a C-FIND Response:

**Table 40: Query/Retrieve Server AE Returned C-FIND-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The Query/Retrieve Server AE has successfully finished sending all matches in previous C-FIND-RSPs. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
Failed	Data Set does not match SOP Class	A900	The Query/Retrieve Server AE has determined that the C-FIND-RQ query identifier is missing mandatory Elements for the specified SOP Class and Query Level. This will only occur if the missing Elements or values prevent the Query/Retrieve Server AE from successfully querying the McKesson Radiology™

Service Status	Further Meaning	Error Code	Behavior
			database. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Failed	Unable to Process	C001	The Query/Retrieve Server AE cannot process the C-FIND-RQ because it cannot query the McKesson Radiology™ database for some reason. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Cancel	Sub-operations terminated due to Cancel Indication	FE00	Indicates that the Query/Retrieve Server AE received a Cancel Request from the remote AE. Note that this can only occur if the Query/Retrieve Server AE is configured to actually check for and handle Cancel Requests. A warning indication is output to the Service Logs. No indication is posted to the User Interface.
Pending	Matches are continuing – Current Match is supplied	FF00	The Query/Retrieve Server AE is successfully sending a match in the C-FIND-RSP, and will continue to send further C-FIND-RSPs. Note that the Query/Retrieve Server AE does not check the C-FIND-RQ query identifier to see if there are Optional Elements that it does not support, so it never returns FF01 (Pending) - Matches are continuing but one or more Optional Keys were not supported. Success indication message is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.3.4.1.3.3 SOP Specific Conformance – Retrieve (C-MOVE)

The Query/Retrieve Server AE will try to establish an Association with a DICOM Application Entity named by the external C-MOVE SCU (through a C-MOVE Destination AE Title) to perform C-STORE operations on requested images. One or more of the Image Storage Presentation Contexts listed in Table 9 will be negotiated.

By default, the Query/Retrieve Server AE is configured to not check for Cancel Requests sent by a remote AE. This is done to improve performance as it does not have to spend time periodically checking if a remote AE has sent a Cancel Request over the Association. However, if it is known that a remote AE can send Cancel Requests, then the Query/Retrieve Server AE can be configured to handle them properly.

If the Query/Retrieve Server AE cannot handle the received C-MOVE Request, then a C-MOVE Response will be returned with the appropriate error Status Code. If the Request can be handled, then the Query/Retrieve Server AE will return a C-MOVE Response to the C-MOVE SCU after each C-STORE Response from the SCP has been received. The C-MOVE Response reports the number of remaining SOP Instances to transfer, as well as the number of SOP Instances transferred having a successful, failed, or warning status. The Association will be properly released after the Query/Retrieve Server AE has attempted to transfer all requested SOP Instances. The Query/Retrieve Server AE will continue to attempt to transfer any remaining SOP Instances even if a failure Status Code is returned in a particular C-STORE response, or the Association with the C-MOVE SCU has been lost.

MIMA specifies different behavior responding to Query SCU that can handle Issuer of Patient ID and Issuer of Accession Number attributes versus Query SCU that cannot handle those attributes where a default value for the unsupported attribute should be configurable for the Query SCU on the Query SCP.

The Query/Retrieve Server AE supporting the Multiple Identity Resolution option of the IHE MIMA Profile shall meet the following requirements when handling received C-MOVE Requests:

- If there is a preconfigured default Patient ID Assigning Authority for the C-MOVE Destination Application Entity then the Query/Retrieve Server AE shall specify a Patient ID value from this Assigning Authority in the SOP Instances sent to the C-MOVE Destination Application Entity. If there is no Patient ID value defined for this preconfigured default Assigning Authority then the Patient ID value shall be left blank.

- If there is no preconfigured default Patient ID Assigning Authority for the C-MOVE Destination Application Entity then the Query/Retrieve Server AE can specify a Patient ID value from any Assigning Authority in the SOP Instances. It shall be assumed that the C-MOVE Destination Application Entity is capable of handling the corresponding Patient ID Assigning Authority information conveyed in the SOP Instances.
- If there is a preconfigured default Accession Number Assigning Authority for the C-MOVE Destination Application Entity then the Query/Retrieve Server AE shall only specify an Accession Number value from this Assigning Authority in the SOP Instances sent to the C-MOVE Destination Application Entity. If there is no Accession Number value defined for this preconfigured default Assigning Authority then the Accession Number value shall be left blank.
- If there is no preconfigured default Accession Number Assigning Authority for the C-MOVE Destination Application Entity then the Query/Retrieve Server AE can specify an Accession Number value from any Assigning Authority in the SOP Instances. It shall be assumed that the C-MOVE Destination Application Entity is capable of handling the corresponding Accession Number Assigning Authority information conveyed in the SOP Instances.

For a summary of the MIMA identifiers convey in the SOP Instances for export see Table 187

The Query/Retrieve Server AE supports the following Elements depending on the Information Model used for the C-MOVE Request:

**Table 41: Patient Root C-MOVE SCP Supported Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient ID	0010,0020	LO	UNIQUE
<b>Study Level</b>			
Study Instance UID	0020,000D	UI	UNIQUE, L
<b>Series Level</b>			
Series Instance UID	0020,000E	UI	UNIQUE
<b>Image Level</b>			
SOP Instance UID	0008,0018	UI	UNIQUE

**Table 42: Study Root C-MOVE SCP Supported Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Study Level</b>			
Study Instance UID	0020,000D	UI	UNIQUE,L
<b>Series Level</b>			
Series Instance UID	0020,000E	UI	UNIQUE
<b>Image Level</b>			
SOP Instance UID	0008,0018	UI	UNIQUE

**Table 43: Patient/Study Only C-MOVE SCP Supported Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient ID	0010,0020	LO	UNIQUE
<b>Study Level</b>			
Study Instance UID	0020,000D	UI	UNIQUE, L

The types of Matching requested by the Query/Retrieve Server AE Retrieve (C-MOVE) SCP:

L - indicates that UID lists can be sent.

UNIQUE - indicates that a single Unique Key value can be sent.

Query/Retrieve Server AE returns one of the following status codes in a Query/Retrieve C-MOVE Response:

**Table 44: Query/Retrieve Server AE Returned C-MOVE-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Sub-operations complete – No failures	0000	The Query/Retrieve Server AE has successfully finished sending all SOP Instances to the C-MOVE Destination AE and will no longer be sending any additional C-MOVE-RSPs. Success indication message is output to the Service Log. No indication is posted to the User Interface.
Warning	Sub-operations complete – One or more failures	B000	The Query/Retrieve Server AE has finished trying to send all SOP Instances to the C-MOVE Destination AE and will no longer be sending any additional C-MOVE-RSPs. However, one or more of the SOP Instances were not successfully sent to the C-MOVE Destination AE. The C-MOVE Response fields indicate the number of SOP Instances transferred having a successful, failed, or warning status. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Refused	Move destination unknown	A801	The Destination Application Entity named in the C-MOVE Request is unknown to Query-Retrieve Server AE. Error message is output to the Service Log. No indication is posted to the User Interface.
Failed	Identifier does not match SOP Class	A900	The Query/Retrieve Server AE has determined that the C-MOVE-RQ query identifier is missing mandatory Elements for the specified C-MOVE SOP Class and Query Level. This will only occur if the missing Elements or values prevent the Query/Retrieve Server AE from successfully querying the McKesson Radiology™ database for matching SOP Instances. An error indication is output to the Service Log. No indication is posted to the User Interface.
Failed	Unable to Process	C000	The Query/Retrieve Server AE cannot process the C-MOVE-RQ because it could not parse the C-MOVE Request identifier or cannot query the McKesson Radiology™ database for some reason. An error indication is output to the Service Log. No indication is posted to the User Interface.
Cancel	Matching terminated due to Cancel Indication	FE00	Indicates that the Query/Retrieve Server AE received a Cancel Request from the remote AE. Note that this can only occur if the Query/Retrieve Server AE is configured to actually check for and handle Cancel Requests. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Pending	Matches are continuing – Current Match is supplied	FF00	The Query/Retrieve Server AE has attempted to send a SOP Instance to the C-MOVE Destination AE and further C-MOVE Responses will be sent. The C-MOVE Response fields indicates the number of remaining SOP Instances to transfer, as well as the number of SOP Instances transferred having a successful, failed, or warning status. If full tracing is enabled, then the contents of the C-MOVE Response are output to the Service Log. No indication is posted to the User Interface.

#### 3.2.3.4.1.3.4

#### SOP Specific Conformance – Modality Worklist

Matching on Optional Matching Keys is not supported. Type 3 Return Keys are not supported.

By default, the Query/Retrieve Server AE is configured to not check for Cancel Requests sent by a remote AE. This is done to improve performance, as it does not have to spend time periodically checking if a remote AE has sent a Cancel Request over the Association. However, if it is known that a remote AE can send Cancel Requests, then the Query/Retrieve Server AE can be configured to handle them properly.

The following table lists the Attributes that it can return in a Modality Worklist C-FIND Response. It also specifies the types of matching supported for an Attribute's value, as well as whether a default or actual value is returned for an Attribute. The default values are used only if the scheduling information is entered through the McKesson Radiology™ user interface or the Modality Worklist SCP that McKesson Radiology™ queried for this scheduling data does not return valid values.

**Table 45: Significant Worklist Attributes**

Module Name Attribute Name	Tag ID	VR	Types of Matching	Returned Value	Default Value
<b>Scheduled Procedure Step</b>					
Scheduled Procedure Step Sequence	0040, 0100	SQ	U	V	
> Scheduled Station AE Title	0040, 0001	AE	NONE	D	"UNKNOWN"
> Scheduled Procedure Step Start Date	0040, 0002	DA	R,S,*,U	V	
> Scheduled Procedure Step Start Time	0040, 0003	TM	NONE	D	6:00 AM
> Scheduled Procedure Step End Date	0040, 0004	DA	R,S,*,U	V	
> Modality	0008, 0060	CS	S,*,U NONE	D	6477
> Scheduled Performing Physician's Name	0040, 0006	PN	NONE	D	6477
> Scheduled Procedure Step Description	0040, 0007	LO	NONE	D	"UNASSIGNED"
> Scheduled Station Name	0040, 0010	SH	NONE	D	6477
> Scheduled Procedure Step Location	0040, 0011	SH	NONE	D	6477
> Scheduled Procedure Step ID	0040, 0009	SH	NONE	V	
<b>Requested Procedure</b>					
Requested Procedure Code Sequence (See NOTE1)	0032, 1064	SQ	U	V	
>Code Value	0008, 0100	SH	NONE	V	
>Coding Scheme Designator	0008, 0102	SH	NONE	D	"UNKNOWN"
>Coding Scheme Version	0008, 0103	SH	NONE	D	"1.0"
>Code Meaning	0008, 0104	LO	NONE	V	
Requested Procedure ID	0040, 1001	SH	NONE	V	
Requested Procedure Description	0032, 1060	LO	NONE	D	"UNASSIGNED"
Study Instance UID	0020, 000D	UI	NONE	V	
Requested Procedure Priority	0040, 1003	SH	NONE	D	6477
Patient Transport Arrangements	0040, 1004	LO	NONE	D	6477
Reference Study Sequence	0008, 1110	SQ	NONE	D	Empty Sequence
<b>Imaging Service Request</b>					
Accession Number	0008, 0050	SH	S,U	V	
Referring Physician's Name	0008, 0090	PN	NONE	D	6477
<b>Visit Identification</b>					
Visit Admission ID	0038, 0010	LO	NONE	D	6477
<b>Visit Status</b>					
Current Patient Location	0038, 0300	LO	NONE	D	6477
<b>Patient Identification</b>					
Patient Name	0010, 0010	PN	S,*,U	V	
Patient ID	0010, 0020	LO	S,U	V	
Issuer of Patient ID	0010, 0021	LO	NONE	V	
<b>Patient Demographic</b>					
Patient Birth Date	0010, 0030	DA	S,*,U	V	
Patient Gender	0010, 0040	CS	NONE	V	
Patient Weight	0010, 1030	DS	NONE	D	6477
Patient Confidentiality	0040, 3001	LO	NONE	D	6477



Referenced Patient Sequence	0008, 1120	SQ	NONE	D	Empty Sequence
<b>Patient Medical</b>					
Patient State	0038, 0500	LO	NONE	D	6373
Pregnancy Status	0010, 21C0	US	NONE	D	6373
Patient Medical Alerts	0010, 2000	LO	NONE	D	6373
Patient Contrast Allergies	0010, 2110	LO	NONE	D	6373
Patient Special Needs	0038, 0050	LO	NONE	D	6373

NOTE1: The Modality Worklist query only returns the Requested Procedure Code Sequence (0032,1064) if the McKesson Radiology™ system is configured for IHE Compliant queries.

The Types of Matching supported by the Query/Retrieve Server AE Modality Worklist SCP:

- S - indicates Single Value Matching is supported.
- R - indicates Range Matching is supported.
- \* - indicates Wildcard Matching is supported.
- U - indicates Universal Matching is supported.
- NONE - indicates that no matching is supported, but that values for this Element are returned if requested (i.e. universal matching).

The Returned Value supported by the Query/Retrieve Server AE Modality Worklist SCP:

- V - indicates a valid value is returned.
- D - indicates a default hard-coded value is returned. The default values are used only if the scheduling information is entered through the McKesson Radiology™ user interface or the Modality Worklist SCP that McKesson Radiology™ queried for this scheduling data does not return valid values.

The Query/Retrieve Server AE returns one of the following status codes in a Modality Worklist C-FIND Response:

**Table 46: Query/Retrieve Server AE Returned C-FIND-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The Query/Retrieve Server AE has successfully finished sending all Modality Worklist matches in previous C-FIND-RSPs. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
Failed	Data Set does not match SOP Class	A900	The Query/Retrieve Server AE has determined that the C-FIND-RQ query identifier is missing mandatory Elements for the Modality Worklist SOP Class. This will only occur if the missing Elements or values prevent the Query/Retrieve Server AE from successfully querying the McKesson Radiology™ database. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Failed	Unable to Process	C001	The Query/Retrieve Server AE cannot process the Modality Worklist C-FIND-RQ because it cannot query the McKesson Radiology™ database for some reason. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Cancel	Sub-operations terminated due to Cancel Indication	FE00	Indicates that the Query/Retrieve Server AE received a Cancel Request from the remote AE. Note that this can only occur if the Query/Retrieve Server AE is configured to actually check for and handle Cancel Requests. A warning indication is output to the Service Logs. No indication is posted to the User Interface.
Pending	Matches are continuing – Current Match is supplied	FF00	The Query/Retrieve Server AE is successfully sending a match in the C-FIND-RSP, and will continue to send further C-FIND-RSPs. Note that the Query/Retrieve Server AE does not check the C-FIND-RQ query identifier to see if there are Optional Elements that it does not support, so it never returns FF01 (Pending) - Matches are continuing but one or more Optional Keys

Service Status	Further Meaning	Error Code	Behavior
			were not supported. Success indication message is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.3.4.1.3.5 Association Acceptor Communication Failure Behavior

The Behavior of the Query/Retrieve Server AE during communication failure when it is acting as an Association Acceptor is summarized in the following table:

**Table 47: Query/Retrieve Server AE Communication Failure Behavior**

Exception	Behavior
Timeout expiry for an expected DICOM Message Request (DIMSE level timeout). The default timeout for waiting on an open Association to receive the next DICOM Message is 60 minutes.	The Association is aborted using a DICOM A-P-ABORT. This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If Query/Retrieve Server AE is in the process of sending images to a C-MOVE Destination AE, then it will continue to do so even if the Association with the C-MOVE SCU has been lost.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout). The default timeout when trying to read from or write to an open socket is 3 minutes.	The Association is aborted using a DICOM A-P-ABORT. This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If Query/Retrieve Server AE is in the process of sending images to a C-MOVE Destination AE, then it will continue to do so even if the Association with the C-MOVE SCU has been lost.
Association A-ABORTed by the SCU or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. An error indication is output to the Service Logs. No indication is posted to the User Interface. If Query/Retrieve Server AE is in the process of sending images to a C-MOVE Destination AE, then it will continue to do so even if the Association with the C-MOVE SCU has been lost.

### 3.2.3.4.1.3.6 Presentation Context Acceptance Criteria

The Query/Retrieve Server AE will only accept the Presentation Contexts specified in Table 36: Query/Retrieve Server AE Accepted Presentation Contexts.

The Query/Retrieve Server AE can be configured to reject valid Presentation Contexts if the external DICOM host is not listed in a local configuration file. In addition, a valid Presentation Context can be rejected if the maximum limit on the number of simultaneous processes has been reached.

The Query/Retrieve Server AE does not check for, and will accept, duplicate Presentation Contexts.

### 3.2.3.4.1.3.7 Transfer Syntax Selection Policies

The Query/Retrieve Server AE supports only the Implicit VR Little Endian and Explicit VR Little Endian Transfer Syntaxes when acting in the Role of an SCP. If both of these are proposed in a single Presentation Context and the SOP Class is supported, then the default behavior is to accept the Implicit VR Little Endian Transfer Syntax.

## 3.2.4 Query/Retrieve Client AE Specification

### 3.2.4.1 SOP Classes

The Query/Retrieve Client AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 66

**Table 48: SOP Class Conformance of Query/Retrieve Client AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Query/Retrieve</b>			
Patient Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	No
Patient Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	No
Study Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	No
Study Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No
Patient Study Only Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Yes	No
Patient Study Only Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	Yes	No

The Query/Retrieve Client AE implements the C-FIND Query and C-MOVE Retrieval SOP Classes as an SCU. It can act as a SCU to query for patient, study and series demographic information as well as retrieve all SOP Instances in a study or series. It can act in direct response to input from the user interface, or when triggered to do so by the McKesson Radiology™ system.

The Query/Retrieve Client AE has one task running on a McKesson Radiology™ system. It acts as an Association Requestor, requesting a new Association when the user of the system requests that a query or retrieval request be sent to a remote AE.

### **3.2.4.2 Association Establishment Policies**

#### **3.2.4.2.1 General**

The Query/Retrieve Client AE will initiate a new Association when the user requests that a remote AE be queried for certain patient, study, or series information. It will also initiate a new Association when it is triggered to retrieve all SOP Instances in a study or series from a remote AE.

The DICOM Standard Application Context Name is always proposed:

**Table 49: DICOM Application Context for Query/Retrieve Client AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

#### **3.2.4.2.2 Number of Associations**

The Query/Retrieve Client AE will only open one Association at a time with a remote AE.

**Table 50: Number of Simultaneous Associations for Query/Retrieve Client AE**

Maximum number of simultaneous Associations	1
---	---

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 67

### 3.2.4.2.3 Asynchronous Nature

Negotiation of multiple outstanding transactions is not supported.

**Table 51: Asynchronous Nature for Query/Retrieve Client AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

### 3.2.4.2.4 Implementation Identifying Information

**Table 52: DICOM Implementation Class and Version for Query/Retrieve Client AE**

Implementation Class UID	1.2.840.113711.10
Implementation Version Name	V1.0

### 3.2.4.3 Association Initiation Policy

#### 3.2.4.3.1 Activity – Users Send Query Request to Remote AE


##### 3.2.4.3.1.1 Description and Sequencing of Activity

If the user of a McKesson Radiology™ system uses the user interface to specify that a query or retrieval request be sent to a remote AE, then a single attempt will be made. If the query or retrieval request fails, for whatever reason, then no retry will be performed.

In order for the user interface to be used to request the retrieval of SOP Instances from a remote AE, the user must first query the remote AE to get the key values (Patient ID, Study UID, etc. ) for the SOP Instances to be retrieved. Once the key values have been identified, then the user interface can be used to request the retrieval.

In addition to the user directly requesting the retrieval of SOP Instances, the McKesson Radiology™ system can do this automatically. This will occur if the user wants to view a certain study and the McKesson Radiology™ system knows that the SOP Instances for the study have to first be retrieved from a remote AE before they can be displayed. This can occur if the McKesson Radiology™ system is configured to use a remote AE as the archive, and the SOP Instances have been flushed from the McKesson Radiology™ system after they were sent to the remote AE.

Before the Query/Retrieve Client AE sends a C-MOVE-RQ to retrieve items, it will first verify that the remote AE really has the SOP Instances to be retrieved. This will occur regardless of whether the retrieval is being triggered directly by the user or automatically by the McKesson Radiology™ system. In some cases this can result in a duplicate C-FIND query being sent to the remote AE, first in response to a query initiated through the user interface, and then a second query to verify that the SOP Instances can really be retrieved.

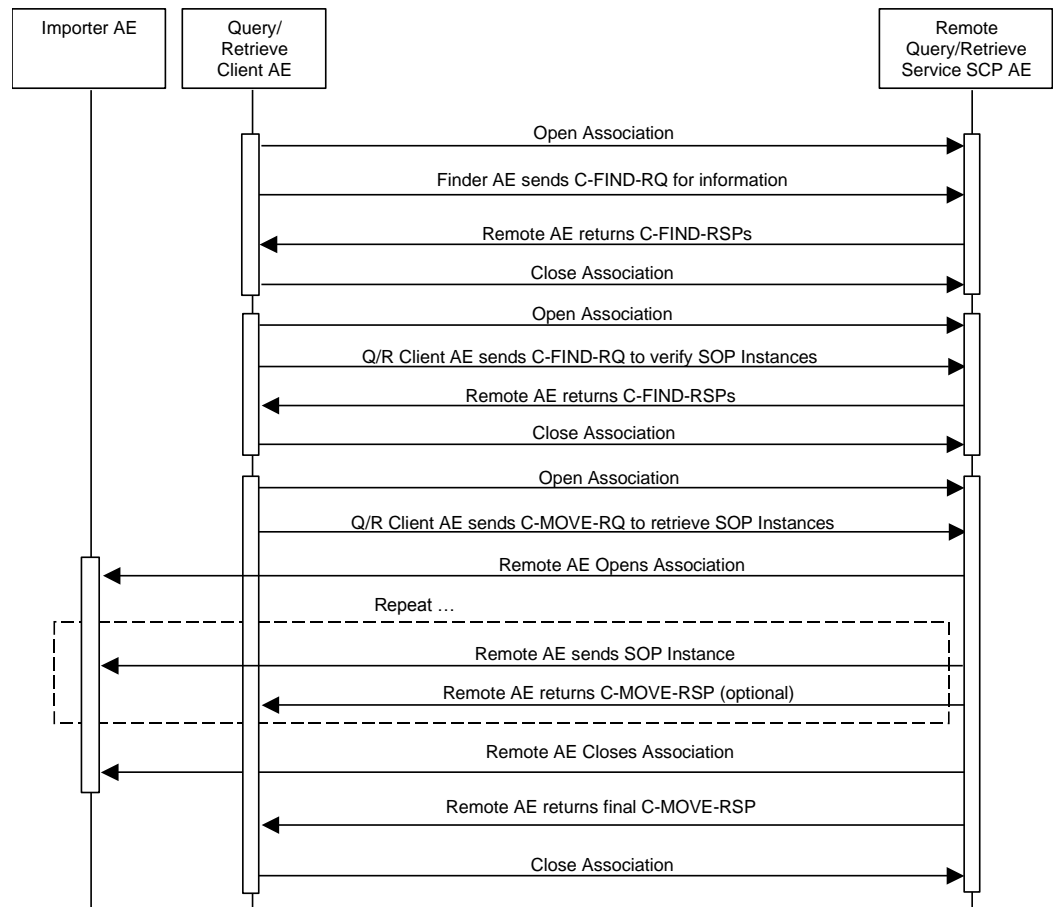**Figure 6: Sequencing of Activity – Sending Query and Retrieval Requests****3.2.4.3.1.2****Proposed Presentation Contexts**

The Query/Retrieve Client AE may propose any one or more of the following Presentation Contexts:

**Table 53: Query/Retrieve Client AE Proposed Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Patient Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Study Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Study Root Q/R Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Patient Study Only Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Patient Study Only Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

**3.2.4.3.1.3 SOP Specific Conformance as an Association Requestor****3.2.4.3.1.3.1 SOP Specific Conformance – Query (C-FIND)**

The Query/Retrieve Client AE provides standard conformance to the supported C-FIND SOP Classes. The Query/Retrieve Client AE does not support Relational Queries.

All three query information models — Patient Root, Study Root, and Patient/Study Only Root — is supported. If more than one information model is negotiated on an Association, and it is possible to use more than one of the negotiated information models to form a query, the following information model will be used (in order of preference):

1. Study Root Information Model
2. Patient Root Information Model
3. Patient/Study Only Information Model

All queries are initiated at the highest level of the information model (the PATIENT or STUDY level depending on the SOP Class used), and then for each response received, recursively repeated at the next lower levels (the STUDY, and then SERIES, and then IMAGE levels, if using the Patient Root query information model), in order to completely elucidate the “tree” of instances available on the remote AE (from which the user may subsequently request a retrieval at any level).

The Query/Retrieve Client AE has a default setting for the maximum number of matching responses it can receive from a remote AE. If the remote AE is going to exceed this number, then the Query/Retrieve Client AE will issue a Cancel Request to the remote AE to stop it from returning further matches. By default, this maximum number is 500.

Unexpected attributes returned in a C-FIND Response (those not requested) are ignored. Requested optional return attributes that are not returned by the SCP are also ignored. Non-matching responses returned by the SCP due to unsupported (hopefully optional) matching keys are not filtered locally by the Query/Retrieve Client AE and thus will still be presented in the browser. The Query/Retrieve Client AE attempts to filter out duplicate responses, but only for responses that have duplicate key values. For example, if the Query/Retrieve Client AE issues a Study Root Study Level query, and multiple matching responses have the same Patient ID and Study UID, then the Query/Retrieve Client AE will filter these so that they are presented as a single matching response.

The Query/Retrieve Client AE can be triggered to issue a query either by user input through the user interface or by the McKesson Radiology™ system itself. The responses to a C-FIND query are presented in the user interface only in the case where the user initiated the query.

The Query/Retrieve Client AE can include the following Elements in a C-FIND Request depending on the Query Root model and the Query level:

**Table 54: Patient Root C-FIND SCU Requested Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient's Name	0010,0010	PN	S,*,U
Patient ID	0010,0020	LO	UNIQUE
Issuer of Patient ID (See NOTE1)	0010,0021	LO	S,U (MIMA), NONE otherwise.
Patient's Birth Date	0010,0030	DA	S,U
Patient's Sex	0010,0040	CS	S,U
<b>Study Level</b>			
Study Date	0008,0020	DA	S,R,U
Study Time	0008,0030	TM	R,U
Accession Number	0008,0050	SH	S,*,U
Issuer of Accession Number Sequence (See NOTE2)	0008,0051	SQ	SQ

>Local Namespace Entity ID	0040,0031	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID	0040,0032	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID Type	0040,0033	CS	S,U (MIMA), NONE otherwise
Study ID	0020,0010	SH	S*,U
Study Instance UID	0020,000D	UI	UNIQUE,L
Referring Physician's Name	0008,0090	PN	S*,U
Study Description	0008,1030	LO	S*,U
Modalities in Study	0008,0061	CS	S*,U
<b>Series Level</b>			
Modality	0008,0060	CS	S,U
Series Number	0020,0011	IS	S*,U
Series Instance UID	0020,000E	UI	UNIQUE
Request Attribute Sequence	0040,0275	SQ	S*,U
> Requested Procedure ID	0040,1001	SH	S*,U
> Scheduled Procedure Step ID	0040,0009	SH	S*,U
Performed Procedure Step Start Date	0040,0244	DA	S,R,U
Performed Procedure Step Start Time	0040,0245	TM	R,U
<b>Image Level</b>			
Instance Number	0020,0013	IS	S*,U
SOP Instance UID	0008,0018	UI	UNIQUE

Table 55: Study Root C-FIND SCU Requested Elements

Description/Module	Tag ID	VR	Types of Matching
<b>Study Level</b>			
Patient's Name	0010,0010	PN	S*,U
Patient ID	0010,0020	LO	S,U
Issuer of Patient ID (See NOTE1)	0010,0021	LO	S,U (MIMA), NONE otherwise.
Patient's Birth Date	0010,0030	DA	S,U
Patient's Sex	0010,0040	CS	S,U
Study Date	0008,0020	DA	S,R,U
Study Time	0008,0030	TM	R,U
Accession Number	0008,0050	SH	S*,U
Issuer of Accession Number Sequence (See NOTE2)	0008,0051	SQ	SQ
>Local Namespace Entity ID	0040,0031	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID	0040,0032	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID Type	0040,0033	CS	S,U (MIMA), NONE otherwise
Study ID	0020,0010	SH	S*,U
Study Instance UID	0020,000D	UI	UNIQUE,L
Referring Physician's Name	0008,0090	PN	S*,U
Study Description	0008,1030	LO	S*,U
Modalities in Study	0008,0061	CS	S*,U
<b>Series Level</b>			
Modality	0008,0060	CS	S,U

Series Number	0020,0011	IS	S,*U
Series Instance UID	0020,000E	UI	UNIQUE
Request Attribute Sequence	0040,0275	SQ	S,*U
> Requested Procedure ID	0040,1001	SH	S,*U
> Scheduled Procedure Step ID	0040,0009	SH	S,*U
Performed Procedure Step Start Date	0040,0244	DA	S,R,U
Performed Procedure Step Start Time	0040,0245	TM	R,U
<b>Image Level</b>			
Instance Number	0020,0013	IS	S,*U
SOP Instance UID	0008,0018	UI	UNIQUE

**Table 56: Patient/Study Only C-FIND SCU Requested Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient's Name	0010,0010	PN	S,*U
Patient ID	0010,0020	LO	UNIQUE
Issuer of Patient ID (See NOTE1)	0010,0021	LO	S,U (MIMA), NONE otherwise.
Patient's Birth Date	0010,0030	DA	S,U
Patient's Sex	0010,0040	CS	S,U
<b>Study Level</b>			
Study Date	0008,0020	DA	S,R,U
Study Time	0008,0030	TM	R,U
Accession Number	0008,0050	SH	S,*U
Issuer of Accession Number Sequence (See NOTE2)	0008,0051	SQ	SQ
>Local Namespace Entity ID	0040,0031	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID	0040,0032	UT	S,U (MIMA), NONE otherwise
>Universal Entity ID Type	0040,0033	CS	S,U (MIMA), NONE otherwise
Study ID	0020,0010	SH	S,*U
Study Instance UID	0020,000D	UI	UNIQUE,L
Referring Physician's Name	0008,0090	PN	S,*U
Study Description	0008,1030	LO	S,*U
Modalities in Study	0008,0061	CS	S,*U

The types of Matching requested by the Query/Retrieve Client AE Query (C-FIND) SCU:

- S - indicates the identifier attribute can specify Single Value Matching.
- R - indicates Range Matching.
- \* - indicates Wildcard Matching.
- U - indicates Universal Matching.
- L - indicates that UID lists can be sent.
- NONE - indicates that no matching can be requested, but that values for this Element are requested to be returned (i.e. universal matching).
- UNIQUE - indicates that this is the Unique Key for that query level, in which case Universal Matching or Single Value Matching can be requested depending on the query level.

McKesson Radiology™ supports the Multiple Identity Resolution option of the IHE MIMA Profile. As such it can include the Patient ID and Accession Number Assigning Authorities as Matching Keys for DICOM Prefetch Queries. The inclusion of Patient ID and Accession Number Assigning Authorities as Matching Keys for general C-FIND queries is not supported.



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 72

**NOTE1: Patient ID Assigning Authority in Queries**

McKesson Radiology™ acting as a Query SCU for DICOM Prefetch can include a value for the Issuer of Patient ID (0010,0021) as a Matching Key in order to unambiguously identify the assigning authority for an included Patient ID value, or indicate which Patient ID assigning authority shall be used in responses if no Patient ID value is included.

**NOTE2: Accession Number Assigning Authority in Queries**

McKesson Radiology™ acting as a Query SCU for DICOM Prefetch can include values for the Issuer of Accession Number Sequence (0008,0051) as Matching Keys in order to unambiguously identify the assigning authority for an included Accession Number value, or indicate which Accession Number assigning authority shall be used in responses if no Accession Number value is included.

The Query/Retrieve Client AE will exhibit the following behavior according to the Status Code value returned in a C-FIND Response from the Remote AE acting as the SCP:

**Table 57: Query/Retrieve Client AE C-FIND-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully finished sending all matches in previous C-FIND-RSPs. Success indication message is output to the Service Log. If a user directly initiated the query using the user interface, then resulting matching information is output to the user interface. If the McKesson Radiology™ system initiated the query, then matching information is not output to the user interface.
Failed	Identifier does not match SOP Class	A900	This is treated as a failure. The Query/Retrieve Client AE does not attempt to resend the C-FIND-RQ. The Association is closed. An error indication is output to the Service Log. An error indication is posted to the User Interface only if the query was initiated through the user interface. Any previously returned matching information is discarded and not output to the user interface.
Failed	Unable to Process	C001	This is treated as a failure. The Query/Retrieve Client AE does not attempt to resend the C-FIND-RQ. The Association is closed. An error indication is output to the Service Log. An error indication is posted to the User Interface only if the query was initiated through the user interface. Any previously returned matching information is discarded and not output to the user interface.
Cancel	Sub-operations terminated due to Cancel Indication	FE00	Indicates that the remote AE received a Cancel Request sent by the Query/Retrieve Client AE and will no longer return further matches. A warning indication is output to the Service Logs but not to the user interface. If a user directly initiated the query using the user interface, then resulting matching information is output to the user interface. If the McKesson Radiology™ system initiated the query, then matching information is not output to the user interface.
Pending	Matches are continuing – However one or more Optional Keys were not supported.	FF01	Query/Retrieve Client AE continues to wait for further C-FIND-RSPs. The remote AE has successfully returned a match in the C-FIND-RSP, and will continue to send further C-FIND-RSPs. However, the remote AE does not support one or more Optional Keys in the query identifier of the C-FIND-RQ. Warning indication message is output to the Service Logs. No indication is posted to the User Interface. Matching information will not be displayed until final C-FIND-RSP is returned.
Pending	Matches are continuing – Current Match is supplied	FF00	Query/Retrieve Client AE continues to wait for further C-FIND-RSPs. The remote AE has successfully returned a match in the C-FIND-RSP, and will continue to send further C-FIND-RSPs. Success indication message is output to the Service Logs. No indication is posted to the User Interface. Matching information will not be

Service Status	Further Meaning	Error Code	Behavior
			displayed until final C-FIND-RSP is returned.
*	*	Any other status code	This is treated as a failure. The Query/Retrieve Client AE does not attempt to resend the C-FIND-RQ. The Association is closed. An error indication is output to the Service Logs. An error indication is posted to the User Interface only if the query was initiated through the user interface. Any previously returned matching information is discarded and not output to the user interface.

### 3.2.4.3.1.3.2 SOP Specific Conformance - Retrieval (C-MOVE)

The Query/Retrieve Client AE provides standard conformance to the supported C-MOVE SOP Classes. All three information models — Patient Root, Study Root, and Patient/Study Only Root — are supported.

A retrieval will be performed at the STUDY, SERIES or IMAGE level depending on what level of entity has been selected by the user in the user interface browser, or by the McKesson Radiology™ to retrieve SOP Instances that have been archived to a remote AE.

The Query/Retrieve Client AE never issues Cancel Requests while retrieving SOP Instances.

The C-MOVE Request is sent to the AE that was specified in the Retrieve AE attribute returned in the related C-FIND-RSP by the remote AE. The instances are retrieved to the McKesson Radiology™ system's database by specifying the C-MOVE Destination AE as the AE Title of the Importer AE. This implies that the remote C-MOVE SCP must be pre-configured to determine the presentation address corresponding to the Importer AE. The Importer AE will have to be configured to either allow any host to send to it, or to allow the host of the Storage Service SCU that the C-MOVE SCP will use.

The Query/Retrieve Client AE completely ignores whatever activities are taking place in relation to the Importer AE that is receiving the retrieved SOP Instances. There is no attempt by the Query/Retrieve Client AE to confirm that SOP Instances have actually been successfully received or stored.

Whether or not completely or partially successfully retrievals are made available on the McKesson Radiology™ system to the user is purely dependent on the success or failure of the C-STORE sub-operations, not on any explicit action by the Query/Retrieve Client AE. Whether or not the remote AE attempts to retry any failed C-STORE sub-operations is beyond the control of the Query/Retrieve Client AE.

If the Association on which the C-MOVE-RQ was issued is aborted for any reason, whether or not the C-STORE sub-operations continue is dependent on the remote AE; the Importer AE will continue to accept Associations and Storage operations regardless.

**Table 58: Patient Root C-MOVE SCU Requested Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient ID	0010,0020	LO	UNIQUE
<b>Study Level</b>			
Study Instance UID	0020,000D	UI	UNIQUE
<b>Series Level</b>			
Series Instance UID	0020,000E	UI	UNIQUE
<b>Image Level</b>			
SOP Instance UID	0008,0018	UI	UNIQUE

**Table 59: Study Root C-MOVE SCU Requested Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Study Level</b>			
Study Instance UID	0020,000D	UI	UNIQUE
<b>Series Level</b>			
Series Instance UID	0020,000E	UI	UNIQUE
<b>Image Level</b>			
SOP Instance UID	0008,0018	UI	UNIQUE

**Table 60: Patient/Study Only C-MOVE SCU Requested Elements**

Description/Module	Tag ID	VR	Types of Matching
<b>Patient Level</b>			
Patient ID	0010,0020	LO	UNIQUE
<b>Study Level</b>			
Study Instance UID	0020,000D	UI	UNIQUE

The types of Matching requested by the Query/Retrieve Client AE Retrieve (C-MOVE) SCU:

L - indicates that UID lists can be sent.

UNIQUE - indicates that a single Unique Key value can be sent.

The Query/Retrieve Client AE will exhibit the following behavior according to the Status Code value returned in a C-MOVE Response from the Remote AE acting as the SCP:

**Table 61: Query/Retrieve Client AE C-MOVE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Sub-operations complete – No failures	0000	<p>The remote AE has successfully finished sending all SOP Instances to the C-MOVE Destination AE and will no longer be sending any additional C-MOVE-RSPs</p> <p>Success indication message is output to the Service Log.</p> <p>If a user directly initiated the retrieval using the user interface, then the retrieved SOP Instances will be displayed in the user interface. If the McKesson Radiology™ system initiated the retrieval, then the retrieved SOP Instances are not automatically displayed in the user interface.</p>
Warning	Sub-operations complete – One or more failures	B000	<p>The remote AE has finished trying to send all SOP Instances to the C-MOVE Destination AE and will no longer be sending any additional C-MOVE-RSPs. However, one or more of the SOP Instances were not successfully sent to the C-MOVE Destination AE. The C-MOVE Response fields indicate the number of SOP Instances transferred having a successful, failed, or warning status.</p> <p>A warning indication is output to the Service Log.</p> <p>If a user directly initiated the retrieval using the user interface, a warning that some SOP Instances were not successfully retrieved is displayed in the user interface. If the McKesson Radiology™ system initiated the retrieval, then the retrieved SOP Instances are not automatically displayed in the user interface.</p> <p>Any successfully retrieved SOP Instances will be discarded and will not be displayed in the user interface whether the user or the McKesson Radiology™ system initiated the retrieval.</p>
Refused	Move destination unknown	A801	<p>This is treated as a failure. The Query/Retrieve Client AE does not automatically attempt to resend the C-MOVE-RQ. The Association is closed.</p> <p>An error indication is output to the Service Log.</p> <p>An error indication is posted to the User Interface only if the retrieval was initiated through the user interface. Any successfully retrieved SOP Instances will be discarded and will not be displayed in the user interface if the user initiated the retrieval.</p>
Failed	Identifier does	A900	<p>This is treated as a failure. The Query/Retrieve Client AE does not automatically</p>

Service Status	Further Meaning	Error Code	Behavior
	not match SOP Class		attempt to resend the C-MOVE-RQ. The Association is closed. An error indication is output to the Service Log. An error indication is posted to the User Interface only if the retrieval was initiated through the user interface. Any successfully retrieved SOP Instances will be discarded and will not be displayed in the user interface if the user initiated the retrieval.
Failed	Unable to Process	C000	This is treated as a failure. The Query/Retrieve Client AE does not automatically attempt to resend the C-MOVE-RQ. The Association is closed. An error indication is output to the Service Log. An error indication is posted to the User Interface only if the retrieval was initiated through the user interface. Any successfully retrieved SOP Instances will not be discarded and will be displayed in the user interface if the user initiated the retrieval.
Cancel	Matching terminated due to Cancel Indication	FE00	This is treated as a failure because the Query/Retrieve Client AE never issues Cancel Requests for C-MOVE Requests. The Query/Retrieve Client AE does not automatically attempt to resend the C-MOVE-RQ. The Association is closed. An error indication is output to the Service Log. An error indication is posted to the User Interface only if the retrieval was initiated through the user interface. Any successfully retrieved SOP Instances will be discarded and will not be displayed in the user interface if the user initiated the retrieval.
Pending	Matches are continuing – Current Match is supplied	FF00	The Query/Retrieve Client AE continues to wait for further C-MOVE-RSPs. If full tracing is enabled, then the contents of the C-MOVE Response are output to the Service Log. No indication is posted to the User Interface.
*	*	Any other status code	This is treated as a failure. The Query/Retrieve Client AE does not attempt to resend the C-MOVE-RQ. The Association is closed. An error indication is output to the Service Logs. An error indication is posted to the User Interface only if the retrieval was initiated through the user interface. Any successfully retrieved SOP Instances will be discarded and will not be displayed in the user interface if the user initiated the retrieval.

## 3.2.4.3.1.3.3

## Association Requestor Communication Failure Behavior

The Behavior of the Query/Retrieve Client AE during communication failure when acting as an Association Requestor is summarized in the following table:

**Table 62: Query/Retrieve Client AE Communication Failure Behavior**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Query/Retrieve Client AE does not automatically attempt to resend the C-FIND-RQ or C-MOVE-RQ. An error indication is output to the Service Logs. An error indication is posted to the User Interface only if the query was initiated through the user interface. If this occurs while waiting for a C-FIND-RSP, then any previously returned matching information is discarded and not output to the user interface. If this occurs while waiting for a C-MOVE-RSP, then any previously retrieved SOP Instances are not discarded.

Exception	Behavior
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Query/Retrieve Client AE does not automatically attempt to resend the C-FIND-RQ or C-MOVE-RQ. An error indication is output to the Service Logs. An error indication is posted to the User Interface only if the query was initiated through the user interface. If this occurs while waiting for a C-FIND-RSP, then any previously returned matching information is discarded and not output to the user interface. If this occurs while waiting for a C-MOVE-RSP, then any previously retrieved SOP Instances are not discarded.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. The Query/Retrieve Client AE does not automatically attempt to resend the C-FIND-RQ or C-MOVE-RQ. An error indication is output to the Service Logs. An error indication is posted to the User Interface only if the query was initiated through the user interface. If this occurs while waiting for a C-FIND-RSP, then any previously returned matching information is discarded and not output to the user interface. If this occurs while waiting for a C-MOVE-RSP, then any previously retrieved SOP Instances are not discarded.

### 3.2.4.4 Association Acceptance Policy

The Query/Retrieve Client AE does not accept Associations.

## 3.2.5 Modality Worklist Client AE Specification

### 3.2.5.1 SOP Classes

The Modality Worklist Client AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 63: SOP Class Conformance of Modality Worklist Client AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Workflow Management</b>			
Modality Worklist Information Model	1.2.840.10008.5.1.4.31	Yes	No

The Modality Worklist Client AE implements the Modality Worklist SOP Class as an SCU. The Modality Worklist Client AE can query a remote AE for a Modality Worklist.

The Modality Worklist Client AE is a single task running on a McKesson Radiology™ system. It acts as an Association Requestor, opening a new Association when it is triggered to query a remote AE for the latest Modality Worklist. If enabled, it will be triggered periodically by the McKesson Radiology™ system to query a remote AE for the Modality Worklist.

### 3.2.5.2 Association Establishment Policies

#### 3.2.5.2.1 General

The Modality Worklist Client AE will initiate a new Association when it is triggered to query a remote AE for the Modality Worklist.

The DICOM Standard Application Context Name is always proposed:

**Table 64: DICOM Application Context for Modality Worklist Client AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

#### 3.2.5.2.2 Number of Associations

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 77

The Modality Worklist Client AE will only open one Association at a time with a remote AE to be queried.

**Table 65: Number of Simultaneous Associations for Modality Worklist Client AE**

Maximum number of simultaneous Associations	1
---	---

### 3.2.5.2.3 Asynchronous Nature

Negotiation of multiple outstanding transactions is not supported.

**Table 66: Asynchronous Nature for Modality Worklist Client AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

### 3.2.5.2.4 Implementation Identifying Information

**Table 67: DICOM Implementation Class and Version for Modality Worklist Client AE**

Implementation Class UID	1.2.840.113711.12
Implementation Version Name	V1.0

### 3.2.5.3 Association Initiation Policy

#### 3.2.5.3.1 Activity – Update Modality Worklist

##### 3.2.5.3.1.1 Description and Sequencing of Activity

The request for an updated Modality Worklist is automatically initiated at specific configurable time intervals. By default, a query to update the Modality Worklist is initiated every 15 minutes.

By default, the Modality Worklist Client AE only queries for the Scheduled Procedure Steps on the day the query is sent. However, it can be configured to also query for those Steps scheduled for future days.

Upon initiation of the request, the Modality Worklist Client AE will build an identifier for the C-FIND Request, initiate an Association to send it, and wait for the Modality Worklist C-FIND Responses. After retrieval of all C-FIND Responses, the Modality Worklist Client AE will access the local McKesson Radiology™ database to add or update patient demographic and study data.

To protect the system from overflow, the Modality Worklist Client AE will limit the number of processed Modality Worklist C-FIND Responses to a configurable maximum. The default maximum value is 200. Once this amount has been reached, the Modality Worklist Client AE will send a Cancel Request to the remote AE acting as the Modality Worklist SCP. The results of a Modality Worklist query are never displayed directly to a user of the McKesson Radiology™ system as the information is only used to update the database and/or to provide this same information if the McKesson Radiology™ Query Server AE is configured to act as a Modality Worklist SCP.

##### 3.2.5.3.1.2 Proposed Presentation Contexts

The Modality Worklist Client AE may propose the following Presentation Context:

**Table 68: Modality Worklist Client AE Proposed Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Modality Worklist Information Model	1.2.840.10008.5.1.4.31	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

**3.2.5.3.1.3 SOP Specific Conformance as an Association Requestor****3.2.5.3.1.3.1 SOP Specific Conformance - Modality Worklist**

The following table lists the Attributes that the Modality Worklist Client AE can include in a Modality Worklist C-FIND Request identifier. It also specifies whether a matching value can be specified and the type of matching. Unexpected Attributes returned in a C-FIND Response are ignored.

**Table 69: Modality Worklist Client AE Requested Elements**

Module Name Attribute Name	Tag ID	VR	Types of Matching
<b>Scheduled Procedure Step</b>			
Scheduled Procedure Step Sequence	0040, 0100	SQ	NONE
> Scheduled Station AE Title	0040, 0001	AE	S,*,U
> Scheduled Procedure Step Start Date	0040, 0002	DA	R,S,*,U
> Scheduled Procedure Step Start Time	0040, 0003	TM	NONE
> Scheduled Procedure Step End Date	0040, 0004	DA	NONE
> Modality	0008, 0060	CS	S,*,U
> Scheduled Performing Physician's Name	0040, 0006	PN	S,*,U
> Scheduled Procedure Step Description	0040, 0007	LO	S,*,U
> Scheduled Station Name	0040, 0010	SH	S,*,U
> Scheduled Procedure Step Location	0040, 0011	SH	S,*,U
> Scheduled Procedure Step ID	0040, 0009	SH	NONE
<b>Requested Procedure</b>			
Requested Procedure Code Sequence	0032,1064	SQ	NONE
>Code Value	0008, 0100	SH	NONE
Requested Procedure ID	0040,1001	SH	NONE
Requested Procedure Description	0032, 1060	LO	NONE
Study Instance UID	0020, 000D	UI	NONE
Requested Procedure Priority	0040, 1003	SH	NONE
Patient Transport Arrangements	0040, 1004	LO	NONE
Reference Study Sequence	0008, 1110	SQ	NONE
<b>Imaging Service Request</b>			
Accession Number	0008, 0050	SH	NONE
Referring Physician's Name	0008, 0090	PN	NONE
<b>Visit Identification</b>			
Visit Admission ID	0038, 0010	LO	NONE
<b>Visit Status</b>			
Current Patient Location	0038, 0300	LO	NONE
<b>Patient Identification</b>			
Patient Name	0010, 0010	PN	NONE
Patient ID	0010, 0020	LO	NONE
<b>Patient Demographic</b>			
Patient Birth Date	0010, 0030	DA	NONE
Patient Gender	0010, 0040	CS	NONE
Patient Weight	0010, 1030	DS	NONE
Patient Confidentiality	0040, 3001	LO	NONE
Referenced Patient Sequence	0008, 1120	SQ	NONE
<b>Patient Medical</b>			
Patient State	0038, 0500	LO	NONE
Pregnancy Status	0010, 21C0	US	NONE
Patient Medical Alerts	0010, 2000	LO	NONE

Patient Contrast Allergies	0010, 2110	LO	NONE
Patient Special Needs	0038, 0050	LO	NONE

The types of Modality Worklist Matching that can be requested by the Modality Worklist Client AE:

- S - indicates the identifier attribute can specify Single Value Matching.
- R - indicates Range Matching.
- \* - indicates Wildcard Matching.
- U - indicates Universal Matching.
- L - indicates that UID lists can be sent.
- NONE - indicates that no matching can be requested, but that values for this Element are requested to be returned (i.e. universal matching).

The Modality Worklist Client AE will exhibit the following behavior according to the Status Code value returned in a C-FIND Response from the Remote AE acting as the SCP:

**Table 70: Modality Worklist Client AE C-FIND-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully finished sending all matches in previous C-FIND-RSPs. Success indication message is output to the Service Log. Resulting matching information is output to the user interface.
Failed	Data Set does not match SOP Class	A900	This is treated as a failure. The Modality Worklist Client AE does not attempt to resend the C-FIND-RQ. The Association is closed. An error indication is output to the Service Log. No indication is posted to the User Interface.
Failed	Unable to Process	C001	This is treated as a failure. The Modality Worklist Client AE does not attempt to resend the C-FIND-RQ. The Association is closed. An error indication is output to the Service Log. No indication is posted to the User Interface.
Cancel	Sub-operations terminated due to Cancel Indication	FE00	Indicates that the remote AE received a Cancel Request sent by the Modality Worklist Client AE and will no longer return further matches. A warning indication is output to the Service Logs but not to the user interface. Resulting matching information is output to the user interface.
Pending	Matches are continuing – However one or more Optional Keys were not supported.	FF01	Modality Worklist Client AE continues to wait for further C-FIND-RSPs. The remote AE has successfully returned a match in the C-FIND-RSP, and will continue to send further C-FIND-RSPs. However, the remote AE does not support one or more Optional Keys in the query identifier of the C-FIND-RQ. Warning indication message is output to the Service Logs. No indication is posted to the User Interface.
Pending	Matches are continuing – Current Match is supplied	FF00	Modality Worklist Client AE continues to wait for further C-FIND-RSPs. The remote AE has successfully returned a match in the C-FIND-RSP, and will continue to send further C-FIND-RSPs. Success indication message is output to the Service Logs. No indication is posted to the User Interface.
*	*	Any other status code	This is treated as a failure. The Modality Worklist Client AE does not attempt to resend the C-FIND-RQ. The Association is closed. An error indication is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.5.3.1.3.2

### Association Requestor Communication Failure Behavior

The Behavior of the Modality Worklist Client AE during communication failure when acting as an Association Requestor is summarized in the following table:



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 80

**Table 71: Modality Worklist Client AE Communication Failure Behavior**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Modality Worklist Client AE does not automatically attempt to resend the C-FIND-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Modality Worklist Client AE does not automatically attempt to resend the C-FIND-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. The Modality Worklist Client AE does not automatically attempt to resend the C-FIND-RQ. An error indication is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.5.4 Association Acceptance Policy

The Modality Worklist Client AE does not accept Associations.

### 3.2.6 Print Management AE Specification

The Print Management AE provides Standard Conformance to the following DICOM V3.0 Meta SOP Classes:

**Table 72: Meta SOP Class Conformance of Print Management AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Print Management</b>			
Basic Grayscale Print Management	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management	1.2.840.10008.5.1.1.18	Yes	No

This corresponds to conformance to the following SOP Classes:

**Table 73: SOP Class Conformance of Print Management AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Print Management</b>			
Basic Film Session	1.2.840.10008.5.1.1.1	Yes	No
Basic Film Box	1.2.840.10008.5.1.1.2	Yes	No
Basic Grayscale Image Box	1.2.840.10008.5.1.1.4	Yes	No
Basic Color Image Box	1.2.840.10008.5.1.1.4.1	Yes	No
Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No

In addition, the Print Management AE supports the following optional SOP Classes:

**Table 74: Optional SOP Class Conformance of Print Management AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Print Management</b>			
Basic Annotation Box	1.2.840.10008.5.1.1.15	Yes	No

The Print Management AE will try to use the Basic Color Print Management SOP Class for color images and the Basic Grayscale Print Management SOP Class for grayscale images. However, if the printer only

supports one of these SOP Classes, then image data will be converted if necessary so that it can still be sent to the printer. In addition, if both color and grayscale images need to be printed to the same piece of film, then the Print Management AE will try to use the Basic Color Print Management SOP Class and convert the color images to grayscale if this SOP Class is actually supported.

The Print Management AE can be configured to propose the Basic Annotation Box SOP Class. If a printer supports this, then the Print Management AE can specify text annotations to be printed on the film with the image(s).

There can be one Print Management AE per DICOM printer that McKesson Radiology™ is configured to use. Thus, the Print Management AE can print simultaneously to multiple printers; However, it cannot simultaneously send multiple print tasks to a single DICOM printer.

### 3.2.6.1 Association Establishment Policies

#### 3.2.6.1.1 General

The Print Management AE will initiate a new Association when the user requests that certain image(s) be printed. Also, McKesson Radiology™ can be configured to automatically print any images that are sent to it (received via the Importer AE). If the Association is broken or some other Association related error is detected, the Association will be aborted. The Print Management AE can be configured to automatically resend images to the printer if such an error occurs.

The DICOM Standard Application Context Name is always proposed:

**Table 75: DICOM Application Context for Print Management AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

The maximum PDU size that will be offered is configurable, and by default is 16,384 bytes.

#### 3.2.6.1.2 Number of Associations

There can be one Print Management AE process per DICOM printer on the network. Each Print Management AE process is configured to send only to a single DICOM printer and each process can only attempt to open one Association at a time. Thus, the maximum possible number of simultaneous Associations is limited to the number of DICOM printers that the McKesson Radiology™ is configured to use.

**Table 76: Number of Simultaneous Associations for Print Management AE**

Maximum number of simultaneous Associations	(number of configured DICOM printers)
---	---------------------------------------

#### 3.2.6.1.3 Asynchronous Nature

The Print Management AE does not provide asynchronous communication (multiple outstanding transactions over a single Association). All Association requests must be completed and acknowledged before a new operation can be initiated.

**Table 77: Asynchronous Nature for Print Management AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

#### 3.2.6.1.4 Implementation Identifying Information

**Table 78: DICOM Implementation Class and Version for Print Management AE**

Implementation Class UID	1.2.840.113711.2
Implementation Version Name	V1.0

### 3.2.6.2 Association Initiation Policy


#### 3.2.6.2.1 Activity – Images Sent to Printer

##### 3.2.6.2.1.1 Description and Sequencing of Activity

An Association is initiated with the named DICOM printer either when a McKesson Radiology™ user selects images to be printed and submits the list of images to the Print Management AE, or when the McKesson Radiology™ is configured to automatically print received images. If the user initiates the printing of images, then they can specify how the image should be processed by using the workstation's image processing tools. In addition, they can select the desired film format and number of copies. If McKesson Radiology™ is configured to automatically print the images, then the default configured image processing, film format, and number of copies will be used.

A new Association will be opened for each print job. The following figure shows the sequencing of the DICOM Messaging involved. The Print Management AE can support N-EVENT-REPORT Requests that are sent by a DICOM Printer at any time over the open Association, even when actually expecting a Response Message of some sort.

**Figure 7: Sequencing of Activity – Images Sent to Printer**

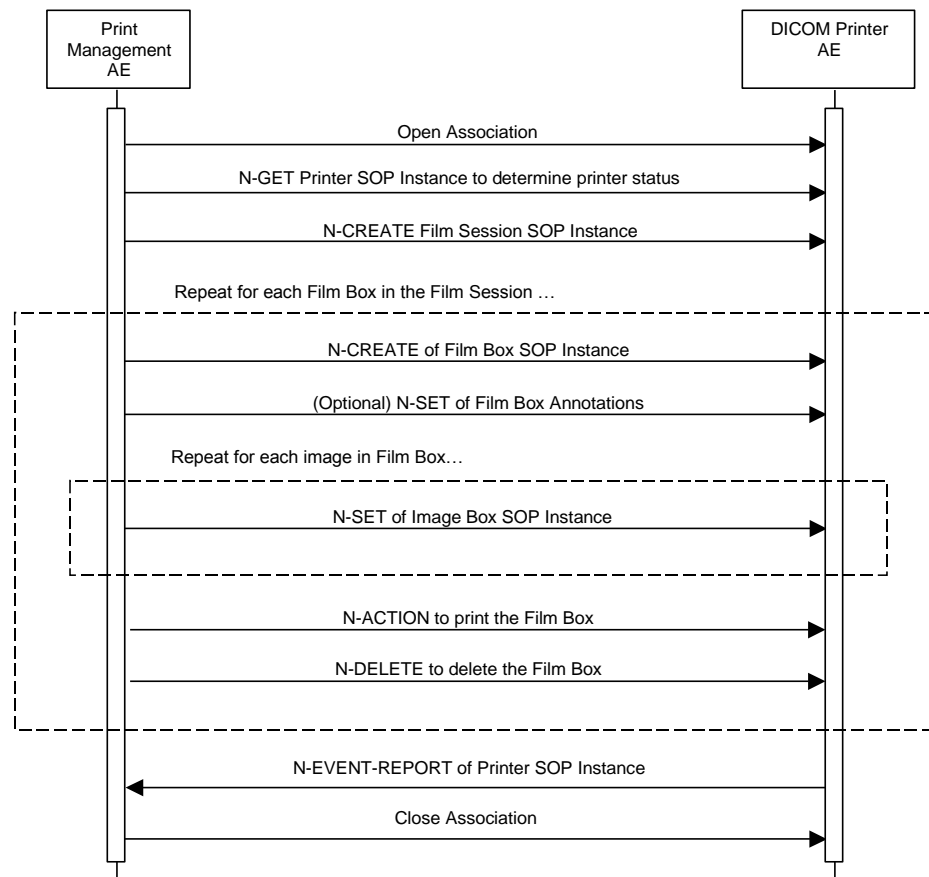

##### 3.2.6.2.1.2 Proposed Presentation Contexts

The Print Management AE may propose the following Presentation Contexts:

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 83

**Table 79: Proposed Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Basic Grayscale Print Management	1.2.840.10008.5.1.1.9	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Basic Color Print Management	1.2.840.10008.5.1.1.18	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Basic Annotation Box	1.2.840.10008.5.1.1.15	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

### 3.2.6.2.1.3 SOP Specific Conformance as an Association Requestor

The following sections detail the SOP Specific Conformance of the Print Management AE as an Association Requestor for each of the SOP Classes that make up the Basic Grayscale and Basic Color Print Management Meta SOP Classes. In addition, there is a section explaining the SOP Specific Conformance for the Basic Annotation Box SOP Class.

If an error or warning condition is detected during a print-job, then an error is posted to the Examine Print Jobs status window of the McKesson Radiology™ user interface. The Print Management AE can be configured to automatically retry a number of times to complete a print-job if some failure occurs.

The tables in this section can use the following terms for Presence of Value of an Attribute:

- VNAP - Value Not Always Present (Attribute is present but value can be zero length)
- ANAP - Attribute Not Always Present
- ALWAYS - Always present with a value
- EMPTY - Attribute is sent without a value

The tables in this section can use the following terms for Source of an Attribute's value:

- USER - Attribute value source is from User input (if user initiates print-job)
- AUTO - Attribute value is generated automatically
- CONFIG - Attribute value is Configurable
- PRINTER - Attribute value will be returned by the Printer

#### 3.2.6.2.1.3.1 SOP Specific Conformance - Printer SOP Class

The Print Management AE uses the Printer SOP Class to obtain information about the current printer status by sending an N-GET Request before even attempting to create a Film Session. This way, it can abort the print task and notify the user of any problems if the printer indicates there is a problem of some sort. The attributes obtained via N-GET are listed in the Table below:

**Table 80: Print Management AE Printer SOP Class N-GET-RQ Attributes**

Attribute Name	Tag ID	VR	Value	Presence of Value <sup>6</sup>	Source
Printer Status	2110, 0010	CS	To be returned by Printer	EMPTY	PRINTER
Printer Status Info	2110, 0020	CS	To be returned by Printer	EMPTY	PRINTER
Printer Name	2110, 0030	LO	To be returned by Printer	EMPTY	PRINTER
Manufacturer	0008, 0070	LO	To be returned by Printer	EMPTY	PRINTER
Manufacturer Model	0008, 1090	LO	To be returned by Printer	EMPTY	PRINTER
Device Serial Number	0018, 1000	LO	To be returned by Printer	EMPTY	PRINTER
Software Version	0018, 1020	LO	To be returned by Printer	EMPTY	PRINTER
Date of Last Calibration	0018, 1200	DA	To be returned by Printer	EMPTY	PRINTER

<sup>6</sup> Attributes do not have a value in the N-GET-RQ. It is up to the DICOM printer to return values in the N-GET-RSP.

Time of Last Calibration	0018, 1201	TM	To be returned by Printer	EMPTY	PRINTER
--------------------------	------------	----	---------------------------	-------	---------

It is mandatory for the SCP to return a value for the Printer Status (2110,0010). The returned value will be handled as follows:

- NORMAL - The print-job continues to be printed.
- FAILURE - The print-job is aborted. Error message is output to the Service Log. If initiated by the user, then an error indication is posted to the Examine Print Jobs status window.
- WARNING - The print-job continues to be printed. Warning is output to the Service Log. The Examine Print Jobs status window does not currently support warning indications.

The Print Management AE will exhibit the following behavior according to the Status Code value returned in an N-GET Response from the Remote AE acting as the Print Management SCP:

**Table 81: Print Management AE N-GET-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully returned the printer status information. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is Released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

The Print Management AE is capable of receiving an N-EVENT-REPORT Request from the Print Management SCP at any time over an open Association.

The Print Management AE will exhibit the following behavior according to the Event Type ID value specified in an N-EVENT-REPORT Request from the Remote AE acting as the Print Management SCP:

**Table 82: Print Management AE N-EVENT-REPORT-RQ Event Type ID Behavior**

Event Type Name	Event Type ID	Behavior
Normal	1	The Print Management AE continues completing the print-job. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	2	The Print Management AE continues completing the print-job. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Failure	3	This is treated as a failure. The print-job is aborted and the Association is Released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
*	*	This is treated as a failure. The print-job is aborted and the Association is Released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

### 3.2.6.2.1.3.2

### SOP Specific Conformance - Film Session SOP Class

The Print Management AE does not use collation, so it does not send N-ACTION or N-DELETE Requests for a Film Session. Thus, it only sends N-CREATE Requests for Film Sessions. The Attributes supplied in an N-CREATE Request for a Film Session are listed below:

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 85

**Table 83: Print Management AE Film Session SOP Class N-CREATE-RQ Attributes**

Attribute Name	Tag ID	VR	Value	Presence of Value <sup>7</sup>	Source
Number of Copies	2000, 0010	IS	1 to N if User, 1 if Config	ALWAYS	USER, CONFIG
Print Priority	2000, 0020	CS	HIGH, MED	ALWAYS	USER, CONFIG
Medium Type	2000, 0030	CS	BLUE FILM, CLEAR FILM, PAPER	ALWAYS	CONFIG
Film Destination	2000, 0040	CS	MAGAZINE, PROCESSOR	ALWAYS	CONFIG

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Session N-CREATE Response from the Remote AE acting as the Print Management SCP:

**Table 84: Print Management AE Film Session N-CREATE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully created the Film Session. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute Value Out of Range	0116	The remote AE has created the Film Session. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute List Error	0107	The remote AE has created the Film Session. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Memory allocation not supported	B600	The remote AE has created the Film Session. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
*	*	Any other status code	This is treated as a failure. The print-job is aborted. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

### 3.2.6.2.1.3.3 SOP Specific Conformance - Film Box SOP Class

The Print Management AE does not use collation, so it must send an N-ACTION Request to print each Film Box and an N-DELETE Request to delete each Film Box. In addition, it must of course send an N-CREATE Request to create each Film Box.

The Attributes supplied in an N-CREATE Request for a Film Box are listed below:

**Table 85: Print Management AE Film Box SOP Class N-CREATE-RQ Attributes**

Attribute Name	Tag ID	VR	Value	Presence of Value <sup>8</sup>	Source
Image Display Format	2010, 0010	CS	STANDARD\1,1 STANDARD\2,2 STANDARD\3,3 STANDARD\3,4 ...	ALWAYS	USER, CONFIG
Referenced Film Session Sequence	2010, 0500	SQ		ALWAYS	AUTO

<sup>7</sup> Attributes do not have a value in the N-GET-RQ. It is up to the DICOM printer to return values in the N-GET-RSP.

<sup>8</sup> Attributes do not have a value in the N-GET-RQ. It is up to the DICOM printer to return values in the N-GET-RSP.

>Referenced SOP Class UID	0008, 1150	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO
>Referenced SOP Instance UID	0008, 1155	UI	From created Film Session SOP Instance	ALWAYS	AUTO
Film Orientation	2010, 0040	CS	PORTRAIT, LANDSCAPE	ALWAYS	USER, CONFIG
Film Size ID	2010, 0050	CS	14INX17IN, 14INX14IN, 11INX14IN, 11INX11IN, 85INX11IN, 8INX10IN	ALWAYS	CONFIG
Magnification Type	2010, 0060	CS	REPLICATE, BILINEAR, CUBIC, NONE	VNAP	CONFIG
Smoothing Type	2010, 0080	CS	Supported values are defined in printer's Conformance Statement	VNAP	CONFIG
Border Density	2010, 0100	CS	BLACK, WHITE, 0 ... N (100ths of OD)	VNAP	CONFIG
Empty Image Density	2010, 0110	CS	BLACK, WHITE, 0 ... N (100ths of OD)	VNAP	CONFIG
Min Density	2010, 0120	US	0 ... N	VNAP	CONFIG
Max Density	2010, 0130	US	0 ... N	VNAP	CONFIG
Trim	2010, 0140	CS	YES, NO	VNAP	CONFIG
Configuration Information	2010, 0150	ST	Supported values are defined in printer's Conformance Statement	VNAP	CONFIG
Illumination	2010, 015E	US	0 ... N	VNAP	CONFIG
Reflective Ambient Light	2010, 0160	US	0 ... N	VNAP	CONFIG

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Box N-CREATE Response from the Remote AE acting as the Print Management SCP:

**Table 86: Print Management AE Film Box N-CREATE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully created the Film Box. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute Value Out of Range	0116	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute List Error	0107	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Requested Min Density or Max Density outside of printer's operating range	B605	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
*	*	Any other status code	This is treated as a failure. The print-job is aborted. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

An N-ACTION Request is issued to instruct the Remote AE acting as the Print Management SCP to print the contents of the Film Box. The SOP Instance UID of the Film Box is automatically included in the N-ACTION Request. The Action Reply argument in the N-ACTION Response is not evaluated.

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Box N-ACTION Response from the Remote AE acting as the Print Management SCP:

**Table 87: Print Management AE Film Box N-ACTION-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully accepted the film for printing. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute Value Out of Range	0116	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute List Error	0107	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Film Box SOP Instance hierarchy does not contain Image Box SOP Instances (empty page)	B603	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size is larger than Image Box size. The image has been de-magnified.	B604	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image has been decimated to fit.	B60A	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Failure	Unable to create Print Job SOP Instance; print queue is full.	C602	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
Failure	Image size is larger than Image Box size.	C603	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
Failure	Combined Print Image Size is larger than Image Box size.	C613	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

An N-DELETE Request is issued to instruct the Remote AE acting as the Print Management SCP to delete the contents of the Film Box. The SOP Instance UID of the Film Box is automatically included in the N-DELETE Request.

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Box N-ACTION Response from the Remote AE acting as the Print Management SCP:



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 88

**Table 88: Print Management AE Film Box N-DELETE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully deleted the Film Box. Success indication message is output to the Service Log. This has no impact on the Examine Print Jobs status window
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

#### 3.2.6.2.1.3.4 SOP Specific Conformance - Basic Annotation SOP Class

The Print Management AE can send N-SET Requests specifying text labels for a Film Box. In order to do this, the Print Management SCP must support the Basic Annotation Box SOP Class. The DICOM Standard does not specify exactly how a printer must implement support for the Basic Annotation Box, so even if it is supported, the DICOM Conformance Statement for the printer must be reviewed in order to determine what support is offered and how the Print Management AE must be configured to make use of this support.

For each Annotation Box that the SCP can support, the Print Management AE can be configured to send the following values in a text string:

%%	- A '%' character
%x	- Today's date
%N	- Patient's full name (lastname, firstname)
%I	- Patient's medical ID
%e	- Exam date
%t	- Exam type
%P	- Page number
%T	- Total number of pages

The Attributes supplied in an N-CREATE Request for a Basic Annotation Box are listed below:

**Table 89: Print Management AE Basic Annotation Box SOP Class N-SET-RQ Attributes**

Attribute Name	Tag ID	VR	Value	Presence of Value <sup>9</sup>	Source
Image Display Format	2010, 0010	CS	STANDARD\1,1 STANDARD\2,2 STANDARD\3,3 STANDARD\3,4 ...	ALWAYS	USER, CONFIG
Referenced Film Session Sequence	2010, 0500	SQ		ALWAYS	AUTO
>Referenced SOP Class UID	0008, 1150	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO
>Referenced SOP Instance UID	0008, 1155	UI	From created Film Session SOP Instance	ALWAYS	AUTO
Film Orientation	2010, 0040	CS	PORTRAIT, LANDSCAPE	ALWAYS	USER, CONFIG
Film Size ID	2010, 0050	CS	14INX17IN, 14INX14IN, 11INX14IN, 11INX11IN, 85INX11IN, 8INX10IN	ALWAYS	CONFIG
Magnification Type	2010, 0060	CS	REPLICATE, BILINEAR, CUBIC, NONE	VNAP	CONFIG
Smoothing Type	2010, 0080	CS	Supported values are defined in printer's Conformance Statement	VNAP	CONFIG

<sup>9</sup> Attributes do not have a value in the N-GET-RQ. It is up to the DICOM printer to return values in the N-GET-RSP.

Border Density	2010, 0100	CS	BLACK, WHITE, 0 ... N (100ths of OD)	VNAP	CONFIG
Empty Image Density	2010, 0110	CS	BLACK, WHITE, 0 ... N (100ths of OD)	VNAP	CONFIG
Min Density	2010, 0120	US	0 ... N	VNAP	CONFIG
Max Density	2010, 0130	US	0 ... N	VNAP	CONFIG
Trim	2010, 0140	CS	YES, NO	VNAP	CONFIG
Configuration Information	2010, 0150	ST	Supported values are defined in printer's Conformance Statement	VNAP	CONFIG
Illumination	2010, 015E	US	0 ... N	VNAP	CONFIG
Reflective Ambient Light	2010, 0160	US	0 ... N	VNAP	CONFIG

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Box N-CREATE Response from the Remote AE acting as the Print Management SCP:

**Table 90: Print Management AE Film Box N-CREATE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully created the Film Box. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute Value Out of Range	0116	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute List Error	0107	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Requested Min Density or Max Density outside of printer's operating range	B605	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
*	*	Any other status code	This is treated as a failure. The print-job is aborted. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

An N-ACTION Request is issued to instruct the Remote AE acting as the Print Management SCP to print the contents of the Film Box. The SOP Instance UID of the Film Box is automatically included in the N-ACTION Request. The Action Reply argument in the N-ACTION Response is not evaluated.

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Box N-ACTION Response from the Remote AE acting as the Print Management SCP:

**Table 91: Print Management AE Film Box N-ACTION-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully accepted the film for printing. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Attribute Value Out of Range	0116	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.

Service Status	Further Meaning	Error Code	Behavior
Warning	Attribute List Error	0107	The remote AE has created the Film Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Film Box SOP Instance hierarchy Does not contain Image Box SOP Instances (empty page)	B603	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size is larger than Image Box size. The image has been de-magnified.	B604	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image or combined Print Image has been decimated to fit.	B60A	The remote AE has accepted the film for printing. Warning indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Failure	Unable to create Print Job SOP Instance; print queue is full.	C602	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
Failure	Image size is larger than Image Box size.	C603	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
Failure	Combined Print Image Size is larger than Image Box size.	C613	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

An N-DELETE Request is issued to instruct the Remote AE acting as the Print Management SCP to delete the contents of the Film Box. The SOP Instance UID of the Film Box is automatically included in the N-DELETE Request.

The Print Management AE will exhibit the following behavior according to the Status Code value returned in a Film Box N-ACTION Response from the Remote AE acting as the Print Management SCP:

**Table 92: Print Management AE Film Box N-DELETE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully deleted the Film Box.

Service Status	Further Meaning	Error Code	Behavior
			Success indication message is output to the Service Log. This has no impact on the Examine Print Jobs status window
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

### 3.2.6.2.1.3.5 SOP Specific Conformance - Image Box SOP Classes

The Print Management AE can send N-SET Requests specifying image data for a Basic Grayscale Image Box or a Basic Color Image Box.

The Attributes supplied in an N-SET Request for a Basic Grayscale Image Box are listed below:

**Table 93: Print Management AE Basic Grayscale Image Box SOP Class N-SET-RQ Attributes**

Attribute Name	Tag ID	VR	Value	Presence of Value <sup>10</sup>	Source
Image Position	2020, 0010	US	1 to number of images in the Film Box	ALWAYS	AUTO
Basic Grayscale Image Sequence	2020, 0110	SQ		ALWAYS	AUTO
>Samples Per Pixel	0028, 0002	US	1	ALWAYS	AUTO
>Photometric Interpretation	0028, 0004	CS	MONOCHROME2	ALWAYS	AUTO
>Rows	0028, 0010	US	Rows in original image being printed	ALWAYS	AUTO
>Columns	0028, 0011	US	Columns in original image being printed	ALWAYS	AUTO
>Bits Allocated	0028, 0100	US	8	ALWAYS	AUTO
>Bits Stored	0028, 0101	US	8	ALWAYS	AUTO
>High Bit	0028, 0102	US	7	ALWAYS	AUTO
>Pixel Representation	0028, 0103	US	0	ALWAYS	AUTO
>Pixel Data	7FE0, 0010	OB	Processed image data	ALWAYS	AUTO
Magnification Type	2010, 0060	CS	REPLICATE, BILINEAR, CUBIC, NONE	VNAP	CONFIG
Smoothing Type	2010, 0080	CS	Supported values are defined in printer's Conformance Statement	VNAP	CONFIG
Polarity	2020, 0020	CS	NORMAL, REVERSE	VNAP	CONFIG
Requested Image Size	2020, 0030	DS	Width in mm of the image to be printed. See comments below for details.	VNAP	AUTO

The image data will be processed if necessary so that it has the characteristics defined in Table 93. If the original image pixel data being printed is not MONOCHROME2 (i.e. is MONOCHROME1, RGB, or ...), then it will be converted to have this Photometric Interpretation. The pixel data will also be converted to unsigned values if they are not already.

<sup>10</sup> Attributes do not have a value in the N-GET-RQ. It is up to the DICOM printer to return values in the N-GET-RSP.

If a Modality LUT, Slope and Intercept, VOI LUT, and/or Window and Level values are specified in the DICOM header for the image, then these will be applied during processing. If the image to be printed is currently displayed on the McKesson Radiology™ workstation, then the same processing parameters used to process the image for display will be used to process the image prior to sending it to the printer. If the original image has greater than 8 Bits Allocated per pixel, then it must be scaled down to 8 Bits Allocated per pixel before sending it to the printer. If no VOI LUT or Window and Level values are specified in the DICOM header or through the user interface, then the Print Management AE will estimate Window and Level values using histogram analysis of the pixel values.

McKesson Radiology™ systems can support the display of overlays included in the original DICOM image (either embedded or separate). McKesson Radiology™ can also be configured to automatically create overlays of its own by specifying that certain DICOM header values should be displayed as strings at certain locations on the displayed image. The Print Management AE will automatically 'burn in' all these types of overlays into the processed pixel data before it is sent to the DICOM printer. In addition, if the user adds graphic annotations to a displayed image on the McKesson Radiology™ workstation, then these annotations will also be 'burned into' the pixel data sent to the printer if the user chooses to print the image.

A value for the Requested Image Size (2020, 0030) is only sent if 'True Size' printing is configured. In order to actually calculate a value for this, the DICOM header for the image being printed must specify the size of each pixel in one of the following Attributes:

- (0028,0030) - Pixel Spacing
- (0018,1164) - Imager Pixel Spacing
- (0018,2010) - Nominal Scanned Pixel Spacing
- (3002,0011) - Image Plane Pixel Spacing

The DICOM Standard does not define exactly what a printer must do if the Requested Image Size (2020, 0030) is too large for the Image Box. The Print Management AE can be configured with the Image Box sizes that will be available on a printer for all combinations of Film Size and Image Display Format. It can be configured to not send a value for the Requested Image Size if the image will not fit in the Image Box. This will prevent the printer from taking some unwanted action if the Requested Image Size is too large.

The Print Management AE will exhibit the following behavior according to the Status Code value returned in an Image Box N-SET Response from the Remote AE acting as the Print Management SCP:

**Table 94: Print Management AE Image Box N-SET-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully set the Image Box. Success indication message is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size is larger than Image Box size. The image has been de-magnified.	0116	The remote AE has set the Image Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Requested Min Density or Max Density outside of printer's operating range.	B605	The remote AE has set the Image Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609	The remote AE has set the Image Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image or combined Print Image has been decimated to fit.	B60A	The remote AE has set the Image Box. A warning indication is output to the Service Log. Examine Print Jobs status window shows print-job as being in-progress.
Failure	Image size is larger than Image Box size.	C603	This is treated as a failure. The print-job is aborted and the Association is released.

Service Status	Further Meaning	Error Code	Behavior
			An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
Failure	Insufficient memory in printer to store the image.	C605	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
Failure	Combined Print Image Size is larger than Image Box size.	C613	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

### 3.2.6.2.1.3.6 Association Requestor Communication Failure Behavior

The Behavior of the Print Management AE during communication failure when acting as an Association Requestor is summarized in the following table:

**Table 95: Print Management AE Communication Failure Behavior**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Print Management AE can be configured to automatically retry a number of times to complete a print-job if some failure occurs. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. The Print Management AE can be configured to automatically retry a number of times to complete a print-job if some failure occurs. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. The Print Management AE can be configured to automatically retry a number of times to complete a print-job if some failure occurs. An error indication is output to the Service Logs. No indication is posted to the User Interface.

### 3.2.6.3 Association Acceptance Policy

The Print Management AE does not accept Associations.

## 3.2.7 External Notifier AE Specifications

The External Notifier AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 96: SOP Class Conformance of External Notifier AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Workflow Management</b>			
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Yes	No

The External Notifier AE will forward any Modality Performed Procedure Step Requests received by the Event Handler AE.

### 3.2.7.1 Association Establishment Policies

#### 3.2.7.1.1 General

The External Notifier AE can issue Notifications for any number of configurable events.

For each event that occurs, an Association to a subscribed third party device will be opened, and a Modality Performed Procedure Step SOP Instance will be sent.

**Table 97: DICOM Application Context for External Notifier AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

The maximum PDU size that will be offered is configurable, and by default is 16,384 bytes

#### 3.2.7.1.2 Number of Associations

One Association is opened for every destination configured to receive notifications.

The External Notifier AE can request one open Association to each Remote AE that it is configured to send notifications to, and keep these Associations open simultaneously.

**Table 98: Number of Simultaneous Associations for External Notifier AE**

Maximum number of simultaneous Associations	One per Remote AE receiving notifications
---	---

#### 3.2.7.1.3 Asynchronous Nature

The External Notifier AE does not provide asynchronous communication (multiple outstanding transactions over a single Association). All Association requests must be completed and acknowledged before a new operation can be initiated.

**Table 99: Asynchronous Nature for External Notifier AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

#### 3.2.7.1.4 Implementation Identifying Information

**Table 100: DICOM Implementation Class and Version for External Notifier AE**

Implementation Class UID	1.2.840.113711.14
Implementation Version Name	V1.0

### 3.2.7.2 Association Initiation Policy

#### 3.2.7.2.1 Activity – Event Occurs that Requires Notification of a Remote AE

##### 3.2.7.2.1.1 Description and Sequencing of Activity

An Association is initiated with the external DICOM system when a McKesson Radiology™ internal event occurs. There is no sequencing of this activity.

##### 3.2.7.2.1.2 Proposed Presentation Contexts

The External Notifier AE may propose the following Presentation Contexts:

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 95

**Table 101: External Notifier AE Proposed Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

### 3.2.7.2.1.3 SOP Specific Conformance as an Association Requestor

The External Notifier AE can be configured to notify Remote AE 'C' whenever an Modality Performed Procedure Step is created or set by forwarding the MPPS Messages (acting as an IHE Performed Procedure Step Manager).

Currently, the events listed in the following table are supported:

**Table 102: External Notifier AE Supported Events**

Event Type	Meaning
MPPSCREATE	A Modality Performed Procedure Step request has been received (N-CREATE)
MPPSSET	A Modality Performed Procedure Step has been updated (N-SET)

### 3.2.7.2.1.3.1 SOP Specific Conformance - Modality Performed Procedure Step

The External Notifier AE does not independently generate MPPS requests. It simply forwards all requests received by the Event Handler AE as-is to its configured destinations. Therefore, the attributes sent by the External Notifier AE in both the N-CREATE and N-SET messages depend solely on the originating source of the MPPS request. This behavior implements the IHE Technical Framework requirements for the Performed Procedure Step Manager Actor.

As part of the MIMA option support, the system can provide DICOM attributes conveying the Assigning Authorities of the Patient ID and Accession Number in the forwarded Performed Procedure Step N-CREATE messages, and also convey the Institution Name (0008,0080) and Institution Code Sequence (0008,0082) in the forwarded Performed Procedure Step N-CREATE messages so that the institution where the referenced SOP Instances were created is identified. If a destination system cannot handle these attributes, the system can be configured to not include these information in the forwarded message when forwarding to that destination.

The External Notifier AE will exhibit the following behavior according to the Status Code value returned in a MPPS N-CREATE Response from the Remote AE acting as the MPPS SCP:

**Table 103: External Notifier AE MPPS N-CREATE-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully created the MPPS. Success indication message is output to the Service Log. No indication is posted to the User Interface.
Warning	Attribute Value Out of Range	0116	The remote AE is considered to have created the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Warning	Attribute List Error	0107	The remote AE is considered to have created the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Warning	Memory allocation not supported	B600	The remote AE is considered to have created the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
*	*	Any	This is treated as a failure. External Notifier AE will re-attempt to create the



Service Status	Further Meaning	Error Code	Behavior
		other status code	MPPS SOP Instance a configurable maximum number of times. An error indication is output to the Service Logs. No indication is posted to the User Interface.

The External Notifier AE will exhibit the following behavior according to the Status Code value returned in a MPPS N-SET Response from the Remote AE acting as the MPPS SCP:

**Table 104: External Notifier AE MPPS N-SET-RSP Status Handling Behavior**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully set the MPPS. Success indication message is output to the Service Log. No indication is posted to the User Interface.
Warning	Attribute Value Out of Range	0116	The remote AE is considered to have set the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Warning	Attribute List Error	0107	The remote AE is considered to have set the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Warning	Performed Procedure Step Object may no longer be updated.	A710	The remote AE is considered to have set the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
Warning	Memory allocation not supported	B600	The remote AE is considered to have set the MPPS. A warning indication is output to the Service Log. No indication is posted to the User Interface.
*	*	Any other status code	This is treated as a failure. The print-job is aborted and the Association is released. An error indication is output to the Service Logs. An error indication is posted to the Examine Print Jobs status window

### 3.2.7.2.1.3.2

### Association Requestor Communication Failure Behavior

The Behavior of the External Notifier AE during communication failure is summarized in the following table:

**Table 105: External Notifier AE Communication Failure Behavior**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. Notification task is re-queued so that an attempt will be made to repeat it. There is a configured maximum number of times that a notification task can be re-queued. An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. Notification task is re-queued so that an attempt will be made to repeat it. There are a configured maximum number of times that a notification task can be re-queued. An error indication is output to the Service Logs. An error indication is also posted to the User Interface.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. Notification task is re-queued so that an attempt will be made to repeat it. There are a configured maximum number of times that a notification task can be re-queued. An error indication is output to the Service Logs. An error indication is also posted to the User Interface.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 97

### 3.2.7.3 Association Acceptance Policy

The External Notifier AE does not accept Associations.

## 3.2.8 Event Handler AE

The Event Handler AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 106: SOP Class Conformance of Event Handler AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	No	Yes
<b>Workflow Management</b>			
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	No	Yes

When a MPPS Request is received, it can be forwarded to the External Notifier AE so that it can be relayed to other Remote AEs. In addition, Scheduled Procedure Steps can be removed from the Modality Worklist provided by the Query/Retrieve Server AE if a received MPPS Message indicates that it is in progress.

### 3.2.8.1 Association Establishment Policies

#### 3.2.8.1.1 General

The Event Handler AE accepts Associations from external DICOM devices to receive event notifications.

The DICOM Standard Application Context Name is always supported:

**Table 107: DICOM Application Context for Event Handler AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

The maximum PDU size that will be offered is configurable, and by default is 16,384 bytes

#### 3.2.8.1.2 Number of Associations

The Event Handler AE places configurable limitations on the number of simultaneous connections it will support. Once the event Handler AE accepts an Association, a spawned child task will receive any messages transmitted on that Association. The default maximum number of Associations is 10 per connecting host. It is possible to restrict the number of hosts that can connect with the Event Handler AE so the combination of these settings can restrict the maximum number of Associations.

**Table 108: Number of Simultaneous Associations as an Acceptor for Event Handler AE**

Maximum number of simultaneous Associations	Unlimited <sup>11</sup>
---	-------------------------

#### 3.2.8.1.3 Asynchronous Nature

The Event Handler AE does not provide asynchronous communication (multiple outstanding transactions over a single Association). All Association requests must be completed and acknowledged before a new operation can be initiated.

**Table 109: Asynchronous Nature as an SCP for Event Handler AE**

Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

#### 3.2.8.1.4 Implementation Identifying Information

<sup>11</sup> Default maximum is 10 per host permitted to connect to the Event Handler AE.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 98

**Table 110: DICOM Implementation Class and Version for Event Handler AE**

Implementation Class UID	1.2.840.113711.15
Implementation Version Name	V1.0

### 3.2.8.2 Association Initiation Policies

The Event Handler AE does not initiate Associations.

### 3.2.8.3 Association Acceptance Policies

#### 3.2.8.3.1 Activity – External system sends notification of an event

##### 3.2.8.3.1.1 Description and Sequencing of Activity

The Event Handler AE accepts Association Requests only if they propose one or more Presentation Contexts that the Event Handler AE actually supports. If none of the requested Presentation Contexts are accepted, then the Association Request itself is rejected. The Event Handler AE can be configured to only accept Associations requested by certain hosts (using TCP/IP address).

If the Event Handler AE receives an MPPS SOP Class Request Message from a Remote AE, then it can forward this Request to the External Notifier AE. The External Notifier AE can then forward the Request Message to other Remote AEs acting as an SCP for the MPPS SOP Class. In addition, under certain circumstances, any Scheduled Procedure Step corresponding to the MPPS can be removed from the Modality Worklist.

The Event Handler AE has a configurable timeout value for the maximum amount of time that it will wait on an open Association for a new request from a remote AE. A remote AE can reset this timer by sending a Verification request (C-ECHO-RQ). This can act as a useful mechanism for a remote AE to maintain an active Association if the length of time between sending MPPS Requests is long (such as when using a single Association to send the initial Message to create an MPPS and then later Messages to update its status and information).

The Event Handler AE may reject Association attempts as shown in the Table below. The Result, Source and Reason/Diag columns represent the values returned in the corresponding fields of an ASSOCIATE-RJ PDU (see PS 3.8, Section 9.3.4). The following abbreviations are used in the Source column:

- e) 1 – DICOM UL service-user
- f) 2 – DICOM UL service-provider (ASCE related function)
- g) 3 – DICOM UL service-provider (Presentation related function)

**Table 111: Event Handler AE Association Rejection Reasons**

Result	Source	Reason/Diag	Explanation
2 – rejected-transient	c	2 – local-limit-exceeded	The (configurable) maximum number of simultaneous Associations has been reached. An Association request with the same parameters may succeed at a later time.
1 – rejected-permanent	a	2 – application-context-name-not-supported	The Association request contained an unsupported Application Context Name. An association request with the same parameters will not succeed at a later time.
1 – rejected-permanent	b	1 – no-reason-given	The Association request could not be parsed. An Association request with the same format will not succeed at a later time. Usually this is only returned if the Event Handler AE has not been configured to allow the remote AE host to connect to it. The Event Handler AE can be configured to allow only specific host names to open Associations with it. Note that it cannot currently be configured to only allow specific calling and/or called AE Titles when forming Associations.

##### 3.2.8.3.1.2 Accepted Presentation Contexts

The Event Handler AE may accept any one or more of the following Presentation Contexts:

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 99

**Table 112: Event Handler AE Accepted Presentation Contexts**

Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

### 3.2.8.3.1.3 SOP Specific Conformance as an Association Acceptor

#### 3.2.8.3.1.3.1 SOP Specific Conformance – Modality Performed Procedure Step

If the Event Handler AE receives an MPPS N-CREATE or N-SET Request Message from a Remote AE, then it can forward this to the External Notifier AE. The External Notifier AE can then forward a copy of the Request Message to other Remote AEs acting as an SCP for the MPPS SOP Class. This behavior implements the IHE Technical Framework requirements for the Performed Procedure Step Manager Actor.

In addition, under certain circumstances, any Scheduled Procedure Step corresponding to the MPPS can be removed from the Modality Worklist.

The Event Handler AE can pass all Attributes and values of an MPPS N-CREATE Request to the External Notifier AE; However, it retains only the following Attribute values in the McKesson Radiology™ database:

**Table 113: MPPS N-CREATE-RQ Attribute Values Retained by Event Handler**

Attribute Name	Tag ID	VR
Performed Procedure Step ID	(0040,0253)	SH
Performed Procedure Step UID / Affected SOP Instance UID	(0000,1000)	UI
Performed Procedure Step Start Date	(0040,0244)	DA
Performed Procedure Step Start Time	(0040,0245)	TM
Performed Procedure Step Status	(0040,0252)	CS

Upon receipt of a MPPS N-CREATE “IN PROGRESS” request, the corresponding Scheduled Procedure Step entry, if it exists, will be removed from the Modality Worklist. Future Modality Worklist queries will not return the removed entry.

The Event Handler AE returns one of the following status codes in a MPPS N-CREATE Response:

**Table 114: Event Handler AE MPPS N-CREATE-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The Event Handler AE has successfully created the MPPS. Success indication message is output to the Service Log. No indication is posted to the User Interface.
Failure	Processing Failure	0110	The Event Handler AE failed to properly parse or handle the MPPS N-CREATE Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.

The Event Handler AE can pass all Attributes and values of an MPPS N-SET Request to the External Notifier AE; However, it retains only the following Attribute values in the McKesson Radiology™ database:

**Table 115: MPPS N-SET-RQ Attributes Updated by Event Handler**

Attribute Name	Tag ID	VR
Performed Procedure Step Status	(0040,0252)	CS

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 100

Attributes may only be modified when the MPPS entry's status is "IN PROGRESS". If the status is "DISCONTINUED" or "COMPLETED", modification via an N-SET Request is not possible.

An MPPS SOP Instance will not be automatically removed from the McKesson Radiology™ system. Removal of MPPS SOP Instances requires human intervention. Once an MPPS SOP Instance has been removed, then any subsequent N-SET Requests for the SOP Instance will be rejected and an Error Status will be returned in the corresponding N-SET Response.

The Event Handler AE returns one of the following status codes in a MPPS N-CREATE Response:

**Table 116: Event Handler AE MPPS N-SET-RSP Status Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The remote AE has successfully set the MPPS. Success indication message is output to the Service Log. No indication is posted to the User Interface.
Failure	Processing Failure	0110	The Event Handler AE failed to properly parse or handle the MPPS N-SET Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.

#### 3.2.8.3.1.3.2 Association Acceptor Communication Failure Behavior

The Behavior of the Event Handler AE during communication failure when it is acting as an Association Requestor is summarized in the following table:

**Table 117: Event Handler AE Communication Failure Behavior as an Association Acceptor**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT. This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.
Association A-P-ABORTed by the SCU or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	This is treated as a failure. Importer AE does not attempt to resend the N-EVENT-REPORT Request. An error indication is output to the Service Logs. No indication is posted to the User Interface.

#### 3.2.8.3.1.3.3 Presentation Context Acceptance Criterion

The Event Handler AE will only accept the Presentation Contexts specified in Table 112.

The Event Handler AE does not check for, and will accept, duplicate Presentation Contexts.

#### 3.2.8.3.1.3.4 Transfer Syntax Selection Policies

The Event Handler AE supports only the Implicit VR Little Endian Transfer Syntax.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 101

## 3.2.9 Storage Commitment Client AE Specification

### 3.2.9.1 SOP Classes

The Storage Commitment Client AE provides Standard Conformance to the following DICOM V3.0 SOP Classes:

**Table 118: SOP Class Conformance of Storage Commitment Client AE**

DICOM SOP Class Name	SOP Class UID	SCU	SCP
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No

### 3.2.9.2 Association Establishment Policies

#### 3.2.9.2.1 General

The Storage Commitment Client AE can send a request for establishing an Association with a Storage Commitment SCP. When the association is established, an N-ACTION Request is sent to request for Storage Commitment for previously stored Composite SOP Instances. The Storage Commitment Client AE can wait for the Storage Commitment Confirmation (N-EVENT-REPORT) from the Storage Commitment SCP if the Commitment Confirmation is on the same association. The Event Handler AE will handle the Storage Commitment Confirmation (N-EVENT-REPORT) if the Storage Commitment Confirmation is on a separate association.

The DICOM Standard Application Context Name is always proposed:

**Table 119: DICOM Application Context for Storage Commitment Client AE**

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

#### 3.2.9.2.2 Number of Associations

The Storage Commitment Client AE queries the database for pending Storage Commitments jobs, dispatches these jobs to Storage Commitment worker processes that perform the Storage Commitment requests, and completes them when the Storage Commitment worker processes return the responses.

It is possible to configure multiple Storage Commitment worker processes for the Storage Commitment SCU Service. But each Storage Commitment Worker process will only attempt to open one Association at a time to the destination Storage Commitment SCP it is configured to send to. There is no limit on the number Storage Commitment worker processes (simultaneous connections) that the Storage Commitment Client AE can support. However, in the real world, this number is small since the user shall only configure one Storage Commitment worker process per DICOM archive destination.

**Table 120: Number of Simultaneous Associations as a Requestor for Storage Commitment Client AE**

Maximum number of simultaneous Associations	No hard limit <sup>12</sup>
---	-----------------------------

**Table 121: Number of Simultaneous Associations as an Acceptor for Storage Commitment Client AE**

Maximum number of simultaneous Associations	Unlimited <sup>13</sup>
---	-------------------------

<sup>12</sup> There is not hard limit to the number of simultaneous associations initiate by the Storage Commitment Client AE. However, in the real world, this number is small since the user shall only configure one Storage Commitment worker process per DICOM archive destination.

<sup>13</sup> Default maximum is 10 per host permitted to connect to the Event Handler AE.

**3.2.9.2.3 Asynchronous Nature**

The Storage Commitment Client AE does not provide asynchronous communication (multiple outstanding transactions over a single Association). All Association requests must be completed and acknowledged before a new operation can be initiated.

**Table 122: Asynchronous Nature as an SCU for Storage Commitment Client AE**


Maximum number of outstanding asynchronous transactions	1 (Not Configurable)
---	----------------------

**3.2.9.2.4 Implementation Identifying Information****Table 123: DICOM Implementation Class and Version for Storage Commitment Client AE**

Implementation Class UID	1.2.840.113711.15
Implementation Version Name	V1.0

**3.2.9.3 Association Initiation Policies****3.2.9.3.1 Activity – Send Storage Commitment Request****3.2.9.3.1.1 Description and Sequencing of Activity****3.2.9.3.2 General**

The Storage Commitment Client AE will attempt to initiate an association when requested to commit the Composite SOP Instances. When the association is established, an N-ACTION Request is sent to request storage commitment for previously stored Composite SOP Instances. After receiving the N-ACTION response from the Storage Commitment SCP, the Storage Commitment Client AE can wait for the corresponding Storage Commitment Confirmation (N-EVENT-REPORT) on the same association or release the association of the N-ACTION Request. If the Storage Commitment Client AE is configured to not wait for the N-EVENT-REPORT, it will release the association of the N-ACTION Request. The Storage Commitment SCP will be required to open a new association with the Storage Commitment Client AE to send over the N-EVENT-REPORT. The Event Handler AE is responsible for listening for the Storage Commitment Confirmation (N-EVENT-REPORT) on the new association on behalf of the Storage Commitment Client AE. The Storage Commitment SCP will close the association after sending over the N-EVENT-REPORT.

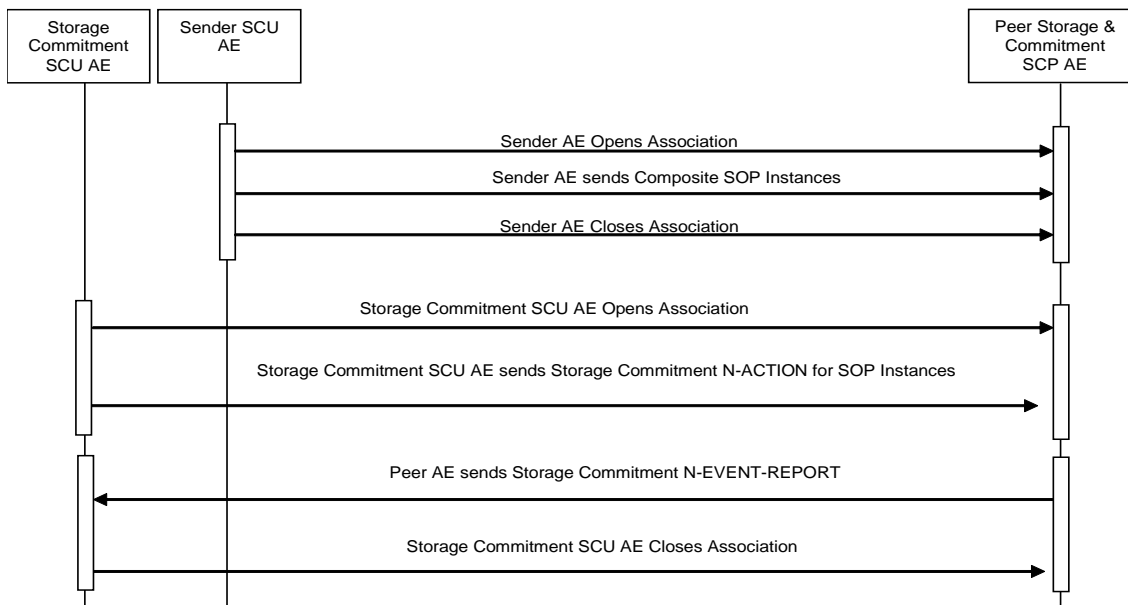**Figure 8: Sequencing of Activity – Send Storage Commitment Request**

Note that the Storage Commitment SCU Client AE shall only send Storage Commitment N-ACTION requests for previously stored Composite SOP Instances.

The following sequencing constraints illustrated in Figure 8 apply to the Storage Commitment Client AE for making Storage Commitment Push Model Requests and receiving N-EVENT-REPORT using a Single Association:

1. Storage Commitment Client AE opens an Association with Peer Storage Commitment SCP AE.
2. Storage Commitment Client AE requests Storage Commitment of Composite SOP Instance(s) (sends N-ACTION-RQ and Peer Storage Commitment SCP AE responds with N-ACTION-RSP to indicate that it received the request).
3. Peer Storage Commitment SCP AE sends Storage Commitment Push Model Notification (N-EVENT-REPORT).
4. Storage Commitment Client AE closes the Association.

### 3.2.9.3.2.1 Proposed Presentation Contexts

The Storage Commitment Client AE will propose Presentation Contexts as shown in the following table:

**Table 124: Storage Commitment Client AE Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

### 3.2.9.3.2.2 SOP Specific Conformance as an Association Requestor

#### 3.2.9.3.2.2.1 SOP Specific Conformance - Storage Commitment

Standard conformance is provided to the DICOM Storage Commitment Push Model SOP Class as an SCP.

The associated activity with the Storage Commitment Push Model Service enables the Storage Commitment Client AE to request remote AEs to make commitment to permanently store Composite SOP



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 104

Instances that have been sent to them. It thus allows McKesson Radiology™ system to safely flush the Composite SOP Instances from its local cache storage.

The Storage Commitment Client AE will send a request for establishing an Association with a remote AE. When the association is established, an N-ACTION Request is sent to request for Storage Commitment for previously stored Composite SOP Instances. The Storage Commitment Client AE can wait for the Storage Commitment Confirmation (N-EVENT-REPORT) from the remote AE if the Commitment Confirmation is on the same association. The Event Handler AE will handle the Storage Commitment Confirmation (N-EVENT-REPORT) if the Storage Commitment Confirmation is on a separate association.

The Storage Commitment Client AE creates files called Service Logs and database records that can be used to monitor its status and diagnose any problems that may arise. If any error occurs during DICOM communication then appropriate messages are always output to the Service Logs and database Storage Commitment Job records.

If the request by the Storage Commitment Client AE to establish an Association fails for any reason (i.e. fail to connect with remote AE's TCP/IP port, Association Request is Rejected by remote AE, etc.) then the Storage Commitment Client AE will try again later to send the N-ACTION Request. The number of retries (default 3) and delay between retries (default 30 min) are configurable.

The Storage Commitment Client AE will exhibit the following Behavior according to the Status Code value returned in a Storage Commitment Push Model N-ACTION Response from a destination SCP:

**Table 125: Storage Commitment Client AE N-ACTION-RSP Status Codes Handling**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The Storage Commitment Client AE has successfully Requested the Storage Commitment Push Model N-ACTION Request. Continue to listen for N-EVENT-REPORT on the same association or separate association depending on configuration.
Error	Processing Failure	0110	Indicates that the Storage Commitment Push Model N-ACTION Request cannot be parsed by the Storage Commitment SCP AE. An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created.
Error	No Such SOP Class	0112	Indicates that the Storage Commitment Push Model N-ACTION Request cannot be processed by the Storage Commitment SCP AE because a The SCP does not accept N-ACTION Request. An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created.

NOTE1: Any Error codes not 0000 is considered a failure.

The Storage Commitment Client AE will send one of the N-EVENT-REPORT Response codes to the Storage Commitment SCP after processing of the N-EVENT-REPORT Result it receives.

The Storage Commitment Client AE verifies the Transaction UID and Committed SOP Instances with the original request. If the Transaction UID and the Committed SOP Instances failed to verify then the Storage Commitment Client AE will re queue and retry the Storage Commitment Request (with a new Transaction UID). However, the Storage Commitment Client AE only returns an N-EVENT-REPORT Response status code of 0000 (Success) to indicate to that the N-EVENT-REPORT Result has been received. It will not return other status codes such as 0110 or 0119 below.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 105

**Table 126: Storage Commitment Client AE N-EVENT-REPORT Response Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	<p>The SCU has successfully received the Storage Commitment Report.</p> <ul style="list-style-type: none"> <li>- Verified the Transaction UID is the same Transaction UID in the N-ACTION Request.</li> <li>- All SOP Instances are committed</li> <li>- All SOP Instances in the Storage Commitment Report are verified with the Referenced SOP Instances.</li> </ul> <p>Success indication message is output to the Service Logs. A successful Storage Commitment database record is created. No indication is posted to the User Interface.</p>
Failure	Processing failure	0110	<p>Not Used</p> <p>Failed to parse the N-EVENT-REPORT-RQ from the Storage Commitment SCP An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.</p>
Failure	SOP Instance UID does not match	0119	<p>Not Used</p> <p>Some SOP Instances in the Storage Commitment Report do not match the SOP Instances in the Reference SOP Instance. No indication is posted to the User Interface.</p>

### 3.2.9.3.2.2.2 Association Requestor Communication Failure Behavior

The Behavior of the Storage Client AE during communication failure when it is acting as an Association Requestor is summarized in the following table:

**Table 127: Storage Commitment Client AE Communication Failure Behavior as an Association Requestor**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	<p>The Association is aborted using a DICOM A-ABORT, A-RELEASE. This is treated as a failure. Storage Commitment Client AE will attempt to resend the Storage Commitment job using the N-ACTION Request after a configurable retry delay (in minutes). An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.</p>
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	<p>The Association is aborted using a DICOM A-ABORT, A-RELEASE. This is treated as a failure. Storage Commitment Client AE will attempt to resend the Storage Commitment job using the N-ACTION Request after a configurable retry delay (in minutes). An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.</p>

Exception	Behavior
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	<p>The Association is aborted using a DICOM A-ABORT, A-RELEASE.</p> <p>This is treated as a failure. Storage Commitment Client AE will attempt to resend the Storage Commitment job using the N-ACTION Request after a configurable retry delay (in minutes).</p> <p>An error indication is output to the Service Logs.</p> <p>A failure Storage Commitment Request database record is created.</p> <p>No indication is posted to the User Interface.</p>

### 3.2.9.4 Association Acceptance Policy


#### 3.2.9.4.1 Activity – Receive Storage Commitment Response

##### 3.2.9.4.1.1 Description and Sequencing of Activity

The Storage Commitment Client AE accepts association if configured to receive N-EVENT-REPORT on a separate association.

The Storage Commitment Client AE accepts Association Requests only if the Requestor proposes one or more Presentation Contexts that the Storage Commitment Client AE actually supports. If none of the requested Presentation Contexts are accepted, then the Association Request itself is rejected. The Storage Commitment Client AE can be configured to only accept Associations requested by certain hosts (using TCP/IP address).

**Figure 9: Sequencing of Activity – Receive Storage Commitment Response in a Separate Association**

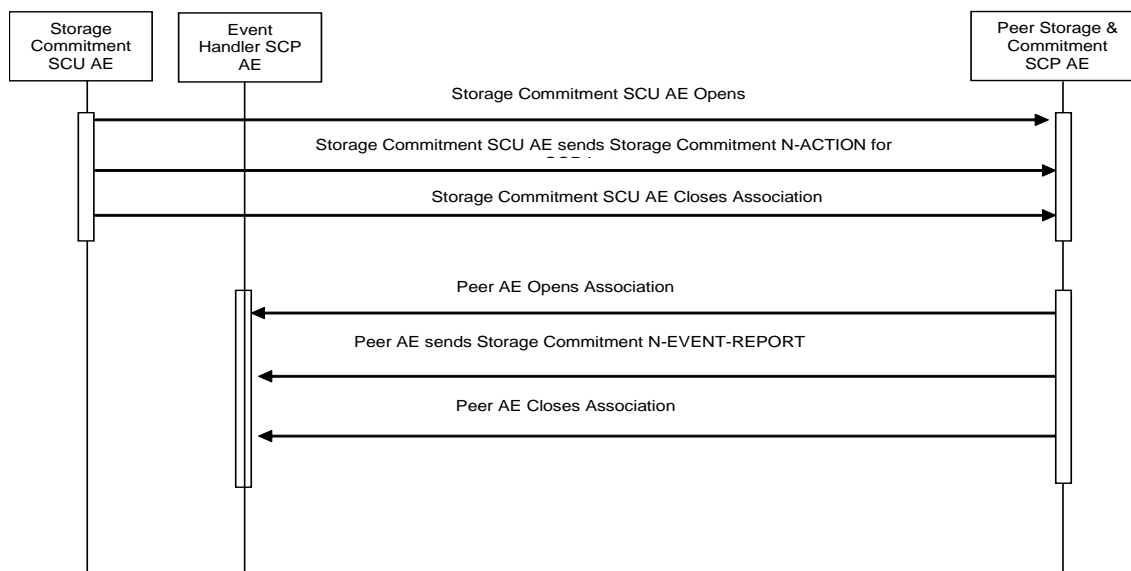

The following sequencing constraints illustrated in Figure 9 apply to the Storage Commitment Client AE for handling Storage Commitment Push Model N-EVENT-REPORT over the separate Association:

- Storage Commitment Client AE opens an Association with Peer Storage Commitment SCP AE.
- Storage Commitment Client AE requests Storage Commitment of Composite SOP Instance(s) (sends N-ACTION-RQ and Peer Storage Commitment SCP AE responds with N-ACTION-RSP to indicate that it received the request).

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 107

3. Storage Commitment Client AE closes the Association of the N-ACTION Request.
4. Peer Storage Commitment SCP AE opens a new Association.
5. Peer Storage Commitment SCP AE sends Storage Commitment Push Model Notification (N-EVENT-REPORT).
6. Peer Storage Commit SCP AE closes the Association with the Event Handler AE.

The Storage Commitment Client AE has a configurable timeout value for the maximum amount of time that it will wait on an open Association for a new request from a remote AE. A remote AE can reset this timer by sending a Verification request (C-ECHO-RQ). This can act as a useful mechanism for a remote AE to maintain an active Association if the length of time between sending requests is long. The Storage Commitment Client AE also has a configurable wait time value to wait for the N-EVENT-REPORT from the Storage Commitment SCP before failing the Storage Commitment job and resubmitting it.

The Storage Commitment Client AE may reject Association attempts as shown in the Table below. The Result, Source and Reason/Diag columns represent the values returned in the corresponding fields of an ASSOCIATE-RJ PDU (see PS 3.8, Section 9.3.4 and Event Handler AE). The following abbreviations are used in the Source column:

- h) 1 – DICOM UL service-user
- i) 2 – DICOM UL service-provider (ASCE related function)
- j) 3 – DICOM UL service-provider (Presentation related function)

**Table 128: Storage Commitment Client AE Association Rejection Reasons**

Result	Source	Reason/Diag	Explanation
2 – rejected-transient	c	2 – local-limit-exceeded	The (configurable) maximum number of simultaneous Associations has been reached. An Association request with the same parameters may succeed at a later time.
1 – rejected-permanent	a	2 – application-context-name-not-supported	The Association request contained an unsupported Application Context Name. An association request with the same parameters will not succeed at a later time.
1 – rejected-permanent	b	1 – no-reason-given	The Association request could not be parsed. An Association request with the same format will not succeed at a later time. Usually this is only returned if the Storage Commitment Client AE has not been configured to allow the remote AE host to connect.

#### 3.2.9.4.1.2 Accepted Presentation Contexts

The Importer AE will accept any **Presentation Context** containing:

4. An abstract syntax selected from Table 12
5. One or more Transfer Syntaxes selected from
6. Table 22

The Storage Commitment Client AE will accept Presentation Contexts (For N-EVENT-REPORT) as shown in the following table:

**Table 129: Storage Commitment Client AE Accepted Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

#### 3.2.9.4.1.3 SOP Specific Conformance as an Association Acceptor

##### 3.2.9.4.1.3.1 SOP Specific Conformance – Verification

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 108

The Storage Commitment Client AE provides standard conformance to the Verification SOP Class as an SCP.

### 3.2.9.4.1.3.2 SOP Specific Conformance – Storage Commitment

The Storage Commitment Client AE accepts association if configured to receive N-EVENT-REPORT on a separate association.

The Storage Commitment Client AE accepts Association Requests only if the Requestor proposes one or more Presentation Contexts that the Storage Commitment Client AE actually supports. If none of the requested Presentation Contexts are accepted, then the Association Request itself is rejected. The Storage Commitment Client AE can be configured to only accept Associations requested by certain hosts (using TCP/IP address).

The Storage Commitment Client AE will send one of the N-EVENT-REPORT Response codes to the Storage Commitment SCP after processing of the N-EVENT-REPORT Result it receives.

The Storage Commitment Client AE verifies the Transaction UID and Committed SOP Instances with the original request. If the Transaction UID and the Committed SOP Instances failed to verify then the Storage Commitment Client AE will re queue and retry the Storage Commitment Request (with a new Transaction UID). However, the Storage Commitment Client AE only returns an N-EVENT-REPORT Response status code of 0000 (Success) to indicate to that the N-EVENT-REPORT Result has been received. It will not return other status codes such as 0110 or 0119 below.

**Table 130: Storage Commitment Client AE N-EVENT-REPORT Response Codes**

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	<p>The SCU has successfully received the Storage Commitment Report.</p> <ul style="list-style-type: none"> <li>- Verified the Transaction UID is the same Transaction UID in the N-ACTION Request.</li> <li>- All SOP Instances are committed</li> <li>- All SOP Instances in the Storage Commitment Report are verified with the Referenced SOP Instances.</li> </ul> <p>Success indication message is output to the Service Logs. A successful Storage Commitment database record is created. No indication is posted to the User Interface.</p>
Failure	Processing failure	0110	<p>Not Used</p> <p>Failed to parse the N-EVENT-REPORT-RQ from the Storage Commitment SCP An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.</p>
Failure	SOP Instance UID does not match	0119	<p>Not Used</p> <p>Some SOP Instances in the Storage Commitment Report do not match the SOP Instances in the Reference SOP Instance. No indication is posted to the User Interface.</p>

### 3.2.9.4.1.3.3 Association Acceptor Communication Failure Behavior

The Behavior of the Storage Commitment Client AE during communication failure when it is acting as an Association Acceptor is summarized in the following table (See Event Handler AE):

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 109

**Table 131: Storage Commitment Client AE Communication Failure Behavior as an Association Acceptor**

Exception	Behavior
Timeout expiry for an expected DICOM Message Response (DIMSE level timeout).	The Association is aborted using a DICOM A-ABORT, A-RELEASE. This is treated as a failure. Storage Commitment Client AE will attempt to resend the Storage Commitment job using the N-ACTION Request after a configurable retry delay (in minutes). An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.
Timeout expiry for an expected DICOM PDU or TCP/IP packet (Low-level timeout).	The Association is aborted using a DICOM A-ABORT, A-RELEASE. This is treated as a failure. Storage Commitment Client AE will attempt to resend the Storage Commitment job using the N-ACTION Request after a configurable retry delay (in minutes). An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.
Association A-P-ABORTed by the SCP or the network layers indicate communication loss (i.e. low-level TCP/IP socket closure)	The Association is aborted using a DICOM A-ABORT, A-RELEASE. This is treated as a failure. Storage Commitment Client AE will attempt to resend the Storage Commitment job using the N-ACTION Request after a configurable retry delay (in minutes). An error indication is output to the Service Logs. A failure Storage Commitment Request database record is created. No indication is posted to the User Interface.

### 3.2.10 QIDO-RS Service Provider Specification

#### 3.2.10.1 QIDO-RS Search For Studies

McKesson Radiology™ supports acting as a QIDO-RS Service Provider. It searches for DICOM Studies based on the following specification.

##### 3.2.10.1.1 Command

[https://mckhost/DICOMRestService/qido/studies\[?query\]](https://mckhost/DICOMRestService/qido/studies[?query])

**Table 132: QIDO-RS Search For Studies Specification**

Parameter	Description
Media Types	Supported  “multipart/related;type=application/dicom+xml” or “application/json”
Matching Attributes	See Table 133
Return Attributes	See Table 134
Limit	Supported  The maximum number of results returned in a query is the lower of: <ul style="list-style-type: none"> <li>• If specified, the Limit parameter value</li> <li>• If the request requires a database fetch, a site configurable database fetch limit</li> <li>• A site configurable query results limit</li> </ul>

Parameter	Description
Offset	Supported
Fuzzymatching	Ignored  Fuzzy matching applies to names in general, so Referring Physicians Name is searched as well with Fuzzy Matching.  Matching is always case-insensitive and matches against the provided name as if there was a trailing wildcard regardless of what the fuzzymatching parameter is set to (either the true or false value).
Includefield	Supported  See "includefield" related entries in Table 134.

**Table 133: QIDO-RS STUDY attribute matching**

Key Word	Tag	Types of Matching
StudyDate	00080020	S, U, R
StudyTime	00080030	S, U, R
AccessionNumber	00080050	S,U
IssuerOfAccessionNumberSequence	00080051	SQ
ModalitiesInStudy	00080061	S,U,
ReferringPhysicianName	00080090	S,*U
PatientName	00100010	S,*U
PatientID	00100020	S,U
IssuerOfPatientID	00100021	S,U
StudyID	00200010	S,U
StudyInstanceUID	0020000D	UNIQUE

The types of Matching supported by the QIDO-RS Service Provider

- S - indicates Single Value Matching is supported.
- R - indicates Range Matching is supported.
- \* - indicates Wildcard Matching is supported.
- U - indicates Universal Matching is supported.
- SQ - indicates Sequence Matching is supported.
- UNIQUE - indicates that this is the unique key for this query level, in which case universal matching or single value matching is used depending on the query level.

NOTE1: Only the first value in the Issuer of Accession Number Sequence will be used as the query key. This is the key for local namespace as opposed to universal entity ID.

NOTE2: The study level query by person name (patient name or Referring Physician Name) returns wildcard matches, even without a wild card specified in the person name query.

For example, a search for "Mill" would return patients whose last names begin with "Mill", such as "Miller" and "Millen".

For each matching Study, the QIDO-RS provider shall return all attributes in accordance with Table 134:

**Table 134: QIDO-RS STUDY attribute returned**

Attribute Name	Tag
Study Date	0008, 0020
Study Time	0008, 0030

Attribute Name	Tag
Accession Number	0008, 0050
Issuer of Accession Number Sequence	0008, 0051
Instance Availability	0008, 0056
Modalities in Study	0008, 0061
Referring Physician's Name	0008, 0090
Patient Name	0010, 0010
Patient ID	0010, 0020
Issuer of Patient ID	0010, 0021
Patient's Birth Date	0010, 0030
Patient's Sex	0010, 0040
Study ID	0020, 0010
Study Instance UID	0020, 000D
Number of Study Related Series	0020, 1206
Number of Study Related Instances	0020, 1208
Retrieve URL	0008, 1190
All other Study Level DICOM Attributes passed as "includefield" query values that are defined in PS3.3 of the DICOM 3.0 standard <sup>1</sup> (Study Level Attributes are the Attributes in the General Study, Patient Study, and Clinical Trial Study Modules in PS3.3.).	
All available Study Level DICOM Attributes defined in PS3.3 of the DICOM 3.0 standard <sup>1</sup> if the "includefield" query key is included with a value of "all"	

NOTE1: An attribute shall be returned only if a value is available (e.g. Rows for a non-image object will not be returned since there is no value available).

NOTE2: Issuer of Accession Number and Issuer of Patient ID are returned to provide information on the study and patient context. See section 3.2.10.4.

### 3.2.10.2 QIDO-RS Search For Series

The QIDO-RS Service AE searches for DICOM Series based on the following specification. This includes search by study instance UID, or series instance UID, or other study and series level search attributes.

#### 3.2.10.2.1 Command

[https://mckhost/DICOMRestService/qido/studies/<study instance uid>/series\[?query\]](https://mckhost/DICOMRestService/qido/studies/<study instance uid>/series[?query])

[https://mckhost/DICOMRestService/qido/series\[?query\]](https://mckhost/DICOMRestService/qido/series[?query])

**Table 135: QIDO-RS Search For Series Specification**

Parameter	Description
Media Types	Supported  "multipart/related;type=application/dicom+xml" or "application/json"
Matching Attributes	See Table 133 and Table 136
Return Attributes	See Table 137
Offset	Supported
Limit	Supported  The maximum number of results returned in a query is the lower of: <ul style="list-style-type: none"> <li>• If specified, the Limit parameter value</li> <li>• If the request requires a database fetch, a site configurable database fetch limit</li> </ul>



Parameter	Description
	<ul style="list-style-type: none"> <li>A site configurable query results limit</li> </ul>
Includefield	Supported  See "includefield" related entries in Table 137.
Relational Queries	Supported  According to DICOM C-FIND Service, relational-queries allow any combination of keys at any level in the hierarchy.  Support for relational-queries removes the baseline restriction that a Unique Key shall be specified for all levels above the Query/Retrieve level in the C-FIND request.  McKesson Radiology™ implementation does not support instance level query keys for series level queries. Only patient, study, series level keys are supported for the series level queries.

**Table 136: QIDO-RS SERIES attribute matching**

Key Word	Tag	Types of Matching
Modality	00080060	S, U,
SeriesNumber	00200011	S, U
SeriesInstanceUID	0020000E	UNIQUE
PerformedProcedureStepStartDate	00400244	S, U, R
PerformedProcedureStepStartTime	00400245	S, U, R
RequestAttributeSequence	00400275	SQ
>ScheduledProcedureStepID	00400009	S, U
>RequestedProcedureID	00401001	S, U

The types of Matching supported by the QIDO-RS Service Provider

- S - indicates Single Value Matching is supported.
- R - indicates Range Matching is supported.
- \* - indicates Wildcard Matching is supported.
- U - indicates Universal Matching is supported.
- SQ - indicates Sequence Matching is supported.
- UNIQUE - indicates that this is the unique key for this query level, in which case universal matching or single value matching is used depending on the query level.

For each matching Series, the QIDO-RS Service Provider shall return all attributes in accordance with Table 137.

**Table 137: QIDO-RS SERIES attribute returned**

Attribute Name	Tag
Instance Availability	0008, 0056
Modality	0008, 0060
Series Description	0008, 103E
Series Number	0020, 0011
Series Instance UID	0020, 000E
Number of Series Related Instances	0020, 1209
Performed Procedure Step Start Date	0040, 0244
Performed Procedure Step Start Time	0040, 0245
Request Attribute Sequence	0040, 0275
>Scheduled Procedure Step ID	0040, 0009
>Requested Procedure ID	0040, 1001
Retrieve URL	0040, 1190

Attribute Name	Tag
All other Study or Series Level DICOM Attributes passed as "includefield" query values that are defined in PS3.3 of the DICOM 3.0 standard <sup>1</sup> (Series Level DICOM Attributes are the attributes in the General Series, Clinical Trial Series and SR Document Series Modules in PS3.3).	
All available Series Level DICOM Attributes that are defined in PS3.3 of the DICOM 3.0 standard <sup>1</sup> if the "includefield" query key is included with a value of "all"	
If {StudyInstanceUID} is not specified in the URL path, all Study-level attributes specified in Table 134	

NOTE1: An attribute shall be returned only if a value is available (e.g. Rows for a non-image object will not be returned since there is no value available).

### 3.2.10.3 QIDO-RS Search For Instances

The QIDO-RS Service AE searches for DICOM Instances based on the following specification.

#### 3.2.10.3.1 Command

For instance level query, the current implementation requires either study instance UID or Series instance UID to be specified in the URL or as query parameters.

For example, the following 2 queries are supported:

<https://mckhost/DICOMRestService/qido/studies/<study instance uid>/instances?sopinstanceuid=<sop instance uid>>

or

<https://mckhost/DICOMRestService/qido/instances?studyinstanceuid=<studyinstanceuid>&sopinstanceuid=<sop instance uid>>

But the following query is not supported:

<https://mckhost/DICOMRestService/qido/instances?sopinstanceuid=<sop instance uid>>

For each matching Instances, the QIDO-RS provider shall return all attributes in accordance with Table 138:

**Table 138: QIDO-RS Search For Instances Specification**

Parameter	Restrictions
Media Types	Supported  "multipart/related;type=application/dicom+xml" or "application/json"
Matching Attributes	See Table 133 and Table 136 and Table 139
Return Attributes	See Table 140
Offset	Supported
Limit	Supported  The maximum number of results returned in a query is the lower of: <ul style="list-style-type: none"> <li>• If specified, the Limit parameter value</li> <li>• If the request requires a database fetch, a site configurable database fetch limit</li> <li>• A site configurable query results limit</li> </ul>
Includefield	Supported  See "includefield" related entries in Table 140.
Relational Queries	Supported

Parameter	Restrictions
	<p>According to DICOM C-FIND Service, relational-queries allow any combination of keys at any level in the hierarchy.</p> <p>Support for relational-queries removes the baseline restriction that a Unique Key shall be specified for all levels above the Query/Retrieve level in the C-FIND request.</p> <p>McKesson Radiology™ Relational Instance level query implementation requires either study instance UID or series instance UID to be specified.</p>

**Table 139: QIDO-RS Instance attributes matching**

Key Word	Tag	Types of Matching
SOPClassUID	00080016	S, U
SOPInstanceUID	00080018	UNIQUE
InstanceNumber	00200013	S, U

The types of Matching supported by the QIDO-RS Service Provider

- S - indicates Single Value Matching is supported.
- R - indicates Range Matching is supported.
- \* - indicates Wildcard Matching is supported.
- U - indicates Universal Matching is supported.
- SQ - indicates Sequence Matching is supported.
- UNIQUE - indicates that this is the unique key for this query level, in which case universal matching or single value matching is used depending on the query level.

**Table 140: QIDO-RS INSTANCE attribute returned**

Attribute Name	Tag
SOP Class UID	0008, 0016
SOP Instance UID	0008, 0018
Instance Availability	0008, 0056
Rows	0028, 0010
Columns	0028, 0011
Bits Allocated	0028, 0100
Number of Frames	0028, 0008
Retrieve URL	0040, 1190
All other Study, Series or Instance Level DICOM Attributes passed as "includefield" query values that are defined in the PS3.3 of the DICOM 3.0 standard <sup>1</sup> .	
All available Instance Level DICOM Attributes that are defined in PS3.3 of the DICOM 3.0 standard <sup>1</sup> if the "includefield" query key is included with a value of "all"	
If {StudyInstanceUID} is not specified in the URL path, all Study-level attributes specified in Table 134	
If {SeriesInstanceUID} is not specified in the URL path, all Series-level attributes specified in Table 137	

NOTE1: An attribute shall be returned only if a value is available (e.g. Rows for a non-image object will not be returned since there is no value available).

### 3.2.10.4 QIDO RS Multi-Context Support

The QIDO-RS service supports specifying the context for both Patient ID and Accession Number in the URL or with the URL parameters for searches.

If both the URL and URL parameters specify context information, the URL parameters shall take precedence in setting the context for the query.

Query for only Issuer of Patient ID or Issuer of Accession Number attribute is considered to be too general so it is not supported.

If the context for the query does not match the context of the study, the accession number returned shall be blank in the QIDO-RS response.

For the study's patient, if the patient does not have a patient ID in the context for the query, the patient ID shall be returned as blank.

Example:

<https://mckhost/DICOMRestService/qido/Context/Context1/studies?patientid=123>

### 3.2.10.5 QIDO RS Limitations

Certain query types are not supported in the QIDO-RS implementation:

Searching for all studies, series, or instances in the system is not supported. These queries are too general and slow the system down.

In addition, searches solely with certain attributes are not supported:

Querying for only the issuer of patient ID is not supported.  
Querying for only the issuer of accession number sequence is not supported.  
Querying for only the modality attribute is not supported.  
Querying for only the series number is not supported.  
Querying for only the requested procedure ID is not supported.  
Querying for only the scheduled procedure step ID is not supported.  
Querying for only the performed procedure step start date is not supported.

The following shows two example queries that are not supported:

<http://mckhost/DICOMRestService/qido/studies?modalitiesinstudy=us>  
<http://mckhost/DICOMRestService/qido/series?modality=US>

### 3.2.10.6 Preference Order for Multiple Accept Headers

The QIDO-RS Service Provider supports returning data in a supported format chosen from one of the formats that the client sent in an Accept header.

The QIDO-RS Service Provider will interpret the client's priority by using the q value in the HTTPS Accept headers, and then for all formats given that have the same q value, by the order in which the client lists the formats. Note that if the format does not include a q value, this is equivalent to the client specifying a q value of 1.0. For example, if the client gives an accept header of multipart/related; type=application/dicom+xml, application/json then the response will be a multipart response with each part containing an XML file. If however the client gives application/json, multipart/related; type=application/dicom+xml then the client will get back the single part response with only JSON data contained.

### 3.2.10.7 QIDO-RS Status Codes

The QIDO-RS Service Provider shall return HTTP status codes to indicate the status of a request.

**Table 141: QIDO-RS HTTP/1.1 STATUS CODES**

HTTP Status Code	Name	Description
200	OK	The query completed and all matching results are returned in the response message body.

HTTP Status Code	Name	Description
206	Partial Content	The query completed but the number of results exceeds the query limit set by the client or the site configuration.  Some of the matching results are returned to the QIDO-RS Client.
400	Bad Request	The request could not be understood by the server
403	Forbidden	Server indicates the client did not present a recognized client certificate when the server is configured to require a client certificate.
404	Not Found	QIDO-RS Client has asked for information on a result not wholly contained in the database and a retrieval of files from archive is required to complete the request. An example is a query for an attribute that doesn't exist in the database and requires loading the DICOM instance from archive to read the information from the DICOM headers.  For data that was online, the results will be returned along with the status code of 404.  For data that was not online, the QIDO-RS Service Provider shall initiate retrieval of the data from archive.  If the QIDO-RS Client makes the same query again moments later after the data has been retrieved from archive, the data will be returned and the client should be able to get an HTTP status code of 200 for the subsequent call.
413	Request Entity Too Large	This indicates that the query was too broad and a narrower query should be requested. This is returned when the number of QIDO-RS results exceeds a site configured limit.  Some of the matching results that fit in the limit are returned to the QIDO-RS Client along with the status code of 413.

### 3.2.10.8 Connection Policies

#### 3.2.10.8.1 General

QIDO-RS Service Provider supports TLS Client Certificates for its transport level security support. QIDO-RS Service Provider will refuse a connection over TLS from a source that is not signed by a signing certificate the service is configured to allow.

#### 3.2.10.8.2 Security

QIDO-RS Service Provider supports TLS Client Certificates for its transport level security support.

QIDO-RS Service Provider supports site level configuration for Cross Origin Resource Sharing (CORS) which allows the resource to be requested from browsers running web applications served from servers in another domain than the one offering the DICOM RESTful services.

### 3.2.11 WADO-RS Service Provider Specification

#### 3.2.11.1 Supported Transfer Syntaxes/Media Types

##### 3.2.11.1.1 WADO-RS DICOM Object Transfer Syntaxes Support

The WADO-RS Service Provider supports the following transfer syntaxes for the application/dicom request type, which request DICOM instances:

**Table 142: WADO-RS DICOM object transfer syntaxes**

Transfer Syntax UID	Description	Media Type / Request Header Accept value
1.2.840.10008.1.2	DICOM Implicit VR Little Endian	application/dicom; transfer-syntax=1.2.840.10008.1.2
1.2.840.10008.1.2.1	DICOM Explicit VR Little Endian	application/dicom; transfer-syntax=1.2.840.10008.1.2.1
Unspecified	Format used is same as how McKesson Radiology™ system stored the instances internally.  This format will incur the least load on the server as the instances will be able to be transferred without having to convert the format. For WADO-RS Clients that support the formats that the system stores, it is suggested they use this request header accept value to get the best performance.	application/dicom
1.2.840.10008.1.2.2	DICOM Explicit VR Big Endian	application/dicom; transfer-syntax=1.2.840.10008.1.2.2
1.2.840.10008.1.2.4.50	DICOM JPEG Baseline Process 1	application/dicom; transfer-syntax=1.2.840.10008.1.2.4.50
1.2.840.10008.1.2.4.51	DICOM JPEG Extended Process 2 & 4	application/dicom; transfer-syntax=1.2.840.10008.1.2.4.51
1.2.840.10008.1.2.4.57	DICOM JPEG Lossless Proc 14	application/dicom; transfer-syntax=1.2.840.10008.1.2.4.57
1.2.840.10008.1.2.4.70	DICOM JPEG Lossless First Order Prediction	application/dicom; transfer-syntax=1.2.840.10008.1.2.4.70
1.2.840.10008.1.2.4.90	DICOM JPEG 2000 (Lossless Only)	application/dicom; transfer-syntax=1.2.840.10008.1.2.4.90
1.2.840.10008.1.2.4.91	DICOM JPEG 2000	application/dicom; transfer-syntax=1.2.840.10008.1.2.4.91
1.2.840.10008.1.2.5	DICOM RLE	application/dicom; transfer-syntax=1.2.840.10008.1.2.5

### 3.2.11.1.2 WADO-RS Image Transfer Syntaxes Support

The WADO-RS Service Provider supports the following transfer syntaxes for the image/dicom request type, which requests the pixel data of a DICOM images.

**Table 143: WADO-RS Image Transfer Syntaxes**

Transfer Syntax UID	Description	Media Type / Request Header Accept value
1.2.840.10008.1.2.4.50	DICOM JPEG Baseline Process 1	image/dicom+jpeg; transfer-syntax=1.2.840.10008.1.2.4.50
1.2.840.10008.1.2.4.51	DICOM JPEG Extended Process 2 & 4	image/dicom+jpeg; transfer-syntax=1.2.840.10008.1.2.4.51
1.2.840.10008.1.2.4.57	DICOM JPEG Lossless Proc 14	image/dicom+jpeg; transfer-syntax=1.2.840.10008.1.2.4.57
1.2.840.10008.1.2.4.70	DICOM JPEG Lossless First Order Prediction	image/dicom+jpeg; transfer-syntax=1.2.840.10008.1.2.4.70
1.2.840.10008.1.2.4.70	DICOM JPEG Lossless First Order Prediction	image/dicom+jpeg
1.2.840.10008.1.2.4.90	DICOM JPEG 2000 (Lossless Only)	image/dicom+jp2; transfer-syntax=1.2.840.10008.1.2.4.90
1.2.840.10008.1.2.4.90	DICOM JPEG 2000 (Lossless Only)	image/dicom+jp2

Transfer Syntax UID	Description	Media Type / Request Header Accept value
1.2.840.10008.1.2.4.91	DICOM JPEG 2000	image/dicom+jpg2; transfer-syntax=1.2.840.10008.1.2.4.91
1.2.840.10008.1.2.5	DICOM RLE	image/dicom+rle; transfer-syntax=1.2.840.10008.1.2.5
1.2.840.10008.1.2.5	DICOM RLE	image/dicom+rle

### 3.2.11.1.3 DICOM Little Endian Media-Type / Transfer Syntax Support

The WADO-RS Service Provider supports returning DICOM binary pixel data (contents of tag (7FE0, 0010))) in Little Endian format when clients send an Accept header with value application/octet-stream.

**Table 144: DICOM Little Endian Media-Type / Transfer Syntax**

Transfer Syntax UID	Description	Media Type / Request Header Accept value
n/a	Pixel data or frame data or bulk data in little endian format	application/octet-stream

### 3.2.11.1.4 Retrieve Metadata Media Type Support

**Table 145: Retrieve Metadata Media Type Support**

Media Type / Request Header Accept value	Description
multipart/related; type=application/dicom+xml or application/json	The returned metadata shall be provided in XML or JSON format.

### 3.2.11.2 HTTP Status Codes

The HTTP return codes from the McKesson Radiology™ System implementation of WADO-RS are as follows:

**Table 146: WADO-RS HTTP/1.1 STATUS CODES**

HTTP Status Code	Name	Description
200	OK	Request completed successfully and has returned all data requested.
206	Partial Content	Request completed and has returned SOME but not ALL of the requested data.  An example scenario where this response code would be encountered would be if a client requests a study that contains a structured report (not an image), and the only media types they specify they Accept are image types from the tables in the requirements "WADO-RS image transfer syntaxes".

HTTP Status Code	Name	Description
403	Forbidden	Server indicates the client did not present a recognized client certificate when the server is configured to require a client certificate.
404	Not Found	Requested data is not available in online storage.  For data that was not online, the WADO-RS Service Provider shall initiate retrieval of the data from archive.  If the WADO-RS Client makes the same retrieval request again moments later after the data has been retrieved from archive, the data will be returned and the client should be able to get an HTTP status code of 200 for the subsequent call.
406	Not Acceptable	Accept type, Transfer Syntax or decompression method not supported.
410	Gone	Requested data is not available at all in the system.

### 3.2.11.3 WADO-RS Retrieve Study

The RetrieveStudy action causes retrieval of the set of DICOM instances associated with a given study unique identifier (UID) that are then used to build the response, which can be DICOM or bulk data depending on the “Accept” type in the HTTP request header, and encapsulated in a multipart MIME response.

#### 3.2.11.3.1 Command

<https://mckhost/DICOMRestService/wado/studies/{StudyInstanceUID}>

#### 3.2.11.3.2 URL Parameters

StudyInstanceUID – the study instance UID for a single study

#### 3.2.11.3.3 WADO-RS Retrieve Study Options

The WADO-RS service shall support RetrieveStudy requests per the standard, 6.5.1.1

**Table 147: Retrieve Study Options**

Options	Description
Allowable request header Accept values	multipart/related;type=application/dicom
	Specifies that the response can be full DICOM Instances encoded in PS3.10 format. When transfer-syntax is not specified, the server can freely choose which transfer-syntax to use for each Instance (format will be same as what McKesson Radiology™ system has stored).
	multipart/related; type=application/dicom; transfer-syntax={TransferSyntaxUID}
	Specifies that the response can be full DICOM Instances encoded in PS3.10 format. The allowed Transfer Syntax UID is any chosen from Table 142



Options	Description
	multipart/related;type=application/octet-stream  Uncompressed bulk and pixel data shall be encoded in a Little Endian format using the application/octet-stream media type. See Table 144.  Specifies that the response includes instance elements with size larger than the bulk data size threshold output as bulk data in Little Endian binary format. DICOM pixel data is output in Little Endian uncompressed format.
	multipart/related; type={MediaType}  Specifies that the response can be pixel data encoded using a {MediaType} chosen from Table 143.
	SOP Classes supported in Table 12.  In addition, the WADO-RS Service Provider can be configured to exclude instances of specific SOP Classes from the retrieval results.
SOP Class	
Size Restriction	Restricted to size supported by McKesson Radiology™ System.

### 3.2.11.3.4 WADO-RS Retrieve Study Response

The WADO-RS service shall provide a response for RetrieveStudy, per standard, 6.5.1.2

#### 3.2.11.3.4.1 Response Headers

HTTP status codes include all from Table 146.

The HTTP Response contains multi-level headers. The top level HTTP response headers include standard server headers plus a Content-Type of multipart/related with a boundary parameter used to separate the attached parts.

DICOM:

Content Type

multipart/related; type=application/dicom; boundary={MessageBoundary}

Bulk Data:

Content Type

multipart/related; type=application/octet-stream; boundary={MessageBoundary}

multipart/related; type={MediaType}; boundary={MessageBoundary}

**Table 148: Part Response Header**

Part Response Header	Value
Content-Type	The media type (from table in section 3.2.11.1.1 or 3.2.11.1.2 or 3.2.11.1.3) representing the type of data in the content
Content-Location	(1) When Media Type returned is one of those in section 3.2.11.1.1  URL is the same as the associated RESTful retrieve instance call
	(2) When Media Type returned is one of those in section 3.2.11.1.3  URL value is for a bulk data URL for uncompressed bulk data element encoded in Little Endian binary format in each instance in each series in a specified study.

(3) When Media Type returned is one of those in section 3.2.11.1.2

URL value is for a bulk data URL for compressed pixel data for each frame, in each instance in each series in a specified study.

### 3.2.11.3.4.2 Response Content

**Table 149: Response Content**

A multipart response where each part contains either
1. Instance binary data for each instance in each series in the specified study in the format specified by the part's Content-Type, when the Content-Type header is a media type chosen from the table "WADO-RS DICOM object transfer syntaxes"
2. Binary bulk data or uncompressed pixel data in little endian format for each instance in each series in the specified study, when the Content-Type header is application/octet-stream. See "DICOM Little Endian Media-Type / Transfer Syntax"
3. Pixel data for each frame in each instance in each series in the specified study in the format specified by the part's Content-Type, when the Content-Type header is a media type chosen from the table "WADO-RS Image Transfer Syntaxes"

NOTE1: A requested transfer syntax of 1.2.840.10008.1.2.4.50 (DICOM JPEG Baseline Process 1) only works when the stored instance is 8 bits deep.

### 3.2.11.3.5 Retrieve Study Example

Retrieving JPEG 2000 lossy compressed frame data or JPEG 2000 lossless compressed frame data or complete DICOM binary data for each instance in explicit VR little endian format for a study

Example URL: <https://mckhost/DICOMRestService/Wado/studies/1.2.3.5>

**Table 150: Request Headers Sent**

Accept	multipart/related; type=image/dicom+jpg2; transfer-syntax=1.2.840.10008.1.2.4.91; q=0.9
Accept	multipart/related; type=image/dicom+jpg2; transfer-syntax=1.2.840.10008.1.2.4.90; q=0.8
Accept	multipart/related; type=application/dicom; transfer-syntax=1.2.840.10008.1.2.1; q=0.7

NOTE1: For WADO-RS Clients that cannot accept all DICOM formats that the system may have stored the instances internally and thus cannot use "application/dicom" as their most preferred format, the WADO-RS Client will want to explicitly specify the formats that it does support.

For the example, the multiple Accept headers has three entries, the media type of image/dicom+jpg2 with transfer syntax JPEG 2000 lossy compression format and "q"<sup>14</sup> parameter set to 0.9, and the media type of image/dicom+jpg2 with transfer syntax JPEG 2000 lossless compression format and "q" parameter set to 0.8 and the media type of application/dicom with transfer syntax explicit VR Little Endian and "q" parameter set to 0.7 means that all frames from image instances in the study will be send in JPEG 2000 lossy format, and for any instances that are not images, they will be returned as a full binary blob in explicit VR Little Endian format.

Since the McKesson Radiology™ system understands all three of the WADO-RS Client requested formats, it will respond to the WADO-RS Client using the client's preferred format and will send DICOM instances back to the client using the JPEG 2000 lossy format.

<sup>14</sup> The HTTP 1.1 specification defines the Accept HTTP header as a way for the client to tell the server what media types the client supports. The q parameter is used to tell the server what media types are preferred.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 122

### 3.2.11.4 WADO-RS Retrieve Series

The RetrieveSeries action causes retrieval of the set of DICOM instances associated with a given study and Series unique identifier (UID) that are then used to build the response, which can be DICOM or bulk data depending on the "Accept" type in the HTTP request header, and encapsulated in a multipart MIME response.

#### 3.2.11.4.1 Command

<https://mckhost/DICOMRestService/wado/studies/{StudyInstanceUID}/series/{SeriesInstanceUID}>

#### 3.2.11.4.2 URL Parameters

StudyInstanceUID – the study instance UID for a study

SeriesInstanceUID – the series UID for a series that belongs to the specified study

#### 3.2.11.4.3 WADO-RS Retrieve Series Options

The WADO-RS Service Provider shall support RetrieveSeries requests per the standard, 6.5.2.1

**Table 151: Retrieve Series Options**

Options	Description
Allowable request header Accept values	multipart/related;type=application/dicom  Specifies that the response can be full DICOM Instances encoded in PS3.10 format. When transfer-syntax is not specified, the server can freely choose which transfer-syntax to use for each Instance (format will be same as what McKesson Radiology™ system has stored).
	multipart/related; type=application/dicom; transfer-syntax={TransferSyntaxUID}  Specifies that the response can be full DICOM Instances encoded in PS3.10 format. The allowed Transfer Syntax UID is any chosen from Table 142
	multipart/related;type=application/octet-stream  Uncompressed bulk and pixel data shall be encoded in a Little Endian format using the application/octet-stream media type. See Table 144.
	 Specifies that the response includes instance elements with size larger than the bulk data size threshold output as bulk data in Little Endian binary format. DICOM pixel data is output in Little Endian uncompressed format.
	multipart/related; type={MediaType}  Specifies that the response can be pixel data encoded using a {MediaType} chosen from Table 143.
SOP Class	SOP Classes supported in Table 12  In addition, the WADOS-RS Service Provider can be configured to exclude instances of specific SOP Classes from the retrieval results.
Size Restriction	Restricted to size supported by McKesson Radiology™ System.

### 3.2.11.4.4 WADO-RS Retrieve Series Response

The WADO-RS Service Provider shall provide a response for RetrieveSeries, per standard, 6.5.2.2.

#### 3.2.11.4.4.1 Response Headers

HTTP status codes include all from Table 146.

The HTTP Response contains multi-level headers. The top level HTTP response headers include standard server headers plus a Content-Type of multipart/related with a boundary parameter used to separate the attached parts.

DICOM:

Content Type

multipart/related; type=application/dicom; boundary={MessageBoundary}

Bulk Data:

Content Type

multipart/related; type=application/octet-stream; boundary={MessageBoundary}

multipart/related; type={MediaType}; boundary={MessageBoundary}

**Table 152: Part Response Header**

Part Response Header	Value
Content-Type	The media type (from table in section 3.2.11.1.1 or 3.2.11.1.2 or 3.2.11.1.3) representing the type of data in the content
Content-Location	<p>(1) When Media Type returned is one of those in section 3.2.11.1.1</p> <p>URL is the same as the associated RESTful retrieve instance call</p> <p>(2) When Media Type returned is one of those in section 3.2.11.1.3</p> <p>URL value is for a bulk data URL for uncompressed bulk data element encoded in Little Endian binary format in each instance in a specified series.</p> <p>(3) When Media Type returned is one of those in section 3.2.11.1.2</p> <p>URL value is for a bulk data URL for compressed pixel data for each frame, in each instance in a specified series.</p>

#### 3.2.11.4.4.2 Response Content

**Table 153: Response Content**

A multipart response where each part contains either
<p>1. Instance binary data for the instance in the specified Series in the format specified by the part's Content-Type, when the Content-Type header is a media type chosen from the table in "<b>WADO-RS DICOM object transfer syntaxes</b></p> <p>2. Binary bulk data or uncompressed pixel data in little endian format for the instance in the specified series, when the Content-Type header is application/octet-stream. See "<b>DICOM Little Endian Media-Type / Transfer Syntax</b>"</p> <p>3. Pixel data for each frame in each instance in a specified series, when the Content-Type header is a media type chosen from the table in "<b>WADO-RS Image Transfer Syntaxes</b>"</p>

NOTE1: A requested transfer syntax of 1.2.840.10008.1.2.4.50 (DICOM JPEG Baseline Process 1) only works when the stored instance is 8 bits deep.

#### 3.2.11.4.5 Retrieve Series Example

Retrieving JPEG 2000 lossless compressed frame data or complete DICOM binary data for each instance for a Series.

Example URL: <https://mckhost/DICOMRestService/Wado/studies/3.4.5/series/2.3.4>

**Table 154: Request Headers Sent**

Accept	multipart/related; type=image/dicom+jp2; transfer-syntax=1.2.840.10008.1.2.4.90
Accept	multipart/related; type=application/dicom; q=0.9

NOTE1: For the example, the multiple Accept headers has two entries, the media type of image/dicom+jp2 with transfer syntax JPEG 2000 lossless compression format and no “q” parameter (equivalent to q= 1.0), and the media type of application/dicom and “q” parameter set to 0.9 means that any image instances will have their pixel data returned with JPEG 2000 lossless compression format and all instances that do not contain pixel data will be returned as a full binary blob in the format that the McKesson Radiology™ System has the instance stored in.

### 3.2.11.5 WADO-RS Retrieve Instance

The RetrieveInstance action causes retrieval of the set of DICOM instances associated with a given study, Series, and SOP Instance unique identifier (UID) that are then used to build the response, which can be DICOM or bulk data depending on the “Accept” type in the HTTP request header, and encapsulated in a multipart MIME response.

#### 3.2.11.5.1 Command

<https://mckhost/DICOMRestService/wado/studies/{StudyInstanceUID}/series/{SeriesInstanceUID}/instances/{SOPInstanceUID}>

#### 3.2.11.5.2 URL Parameters

StudyInstanceUID – the study instance UID for a study

SeriesInstanceUID – the series UID for a series that belongs to the specified study

SOPInstanceUID – the instance UID for an instance in the specified series

#### 3.2.11.5.3 WADO-RS Retrieve Instance Options

The WADO-RS service shall support RetrieveInstance requests per the standard, 6.5.3.1

**Table 155: Retrieve Instance Options**

Options	Description
Allowable request header Accept values	multipart/related;type=application/dicom
	Specifies that the response can be full DICOM Instances encoded in PS3.10 format. When transfer-syntax is not specified, the server can freely choose which transfer-syntax to use for each Instance (format will be same as what McKesson Radiology™ system has stored).
	multipart/related; type=application/dicom; transfer-syntax={TransferSyntaxUID}
	Specifies that the response can be full DICOM Instances encoded in PS3.10 format. The allowed Transfer Syntax UID is any chosen from Table 142

Options	Description
	multipart/related;type=application/octet-stream  Uncompressed bulk and pixel data shall be encoded in a Little Endian format using the application/octet-stream media type. See Table 144.  Specifies that the response includes instance elements with size larger than the bulk data size threshold output as bulk data in Little Endian binary format. DICOM pixel data is output in Little Endian uncompressed format.
	multipart/related; type={MediaType}  Specifies that the response can be pixel data encoded using a {MediaType} chosen from Table 143.
SOP Class Restrictions	SOP Classes supported in Table 12  In addition, the WADOS-RS Service Provider can be configured to exclude instances of specific SOP Classes from the retrieval results.
Size Restriction	Restricted to size supported by McKesson Radiology™ System.

### 3.2.11.5.4 WADO-RS Retrieve Instance Response

The WADO-RS Service Provider shall provide a response for RetrieveInstance, per standard, 6.5.3.2

#### 3.2.11.5.4.1 Response Headers

HTTP status codes include all from Table 146.

The HTTP Response contains multi-level headers. The top level HTTP response headers include standard server headers plus a Content-Type of multipart/related with a boundary parameter used to separate the attached parts.

DICOM:

Content Type

multipart/related; type=application/dicom; boundary={MessageBoundary}

Bulk Data:

Content Type

multipart/related; type=application/octet-stream; boundary={MessageBoundary}

multipart/related; type={MediaType}; boundary={MessageBoundary}

**Table 156: Part Response Header**

Part Response Header	Value
Content-Type	The media type (from table in section 3.2.11.1.1 or 3.2.11.1.2 or 3.2.11.1.3) representing the type of data in the content
Content-Location	(1) When Media Type returned is one of those in section 3.2.11.1.1  URL is the same as the associated RESTful retrieve instance call  (2) When Media Type returned is one of those in section 3.2.11.1.3  URL value is for a bulk data URL for uncompressed bulk data element encoded in Little Endian binary format for the specified instance.  (3) When Media Type returned is one of those in section 3.2.11.1.2

URL value is for a bulk data URL for compressed pixel data for each frame in the specified SOP Instance.
--

### 3.2.11.5.4.2 Response Content

**Table 157: Response Content**

A multipart response where each part contains either
1. Instance binary data for the instance specified in the format specified by the part's Content-Type, when the Content-Type header is a media type chosen from the table in " <b>WADO-RS DICOM object transfer syntaxes</b> "
2. Binary bulk data or uncompressed pixel data in little endian format for the instance specified, when the Content-Type header is application/octet-stream. See " <b>DICOM Little Endian Media-Type / Transfer Syntax</b> "
3. Pixel data for each frame in the specified instance, when the Content-Type header is a media type chosen from the table in " <b>WADO-RS Image Transfer Syntaxes</b> "

NOTE1: A requested transfer syntax of 1.2.840.10008.1.2.4.50 (DICOM JPEG Baseline Process 1) only works when the stored instance is 8 bits deep.

### 3.2.11.5.5 Retrieve Instance Example

Retrieving bulk data or complete DICOM binary data in Little Endian explicit VR specified instance

Example URL: <https://mckhost/DICOMRestService/Wado/studies/3.4.6/series/2.3.5/instances/1.2.3>

**Table 158: Request Headers Sent**

Accept	multipart/related; type=application/octet-stream; q=1.0
Accept	multipart/related; type=application/dicom; transfer-syntax=1.2.840.10008.1.2.1;q=0.9

NOTE1: For WADO-RS Clients that cannot accept all DICOM formats that the system may have stored the instances internally and thus cannot use "application/dicom" as their most preferred format, the WADO-RS Client will want to explicitly specify the formats that it does support.

For the example, the multiple Accept headers sent has two entries, the media type of application/octet-stream and q parameter set to 1.0 and application/dicom media type with transfer syntax set to little endian VR explicit. Since both types are applicable to image and non-image types, the matching instance will be output in the preferred type of octet-stream. All the elements that are larger than the bulk data size threshold will be output in little endian format. If the instance is an image, the pixel data will be uncompressed and output in Little Endian format.

### 3.2.11.6 WADO-RS Retrieve Frames

The Retrieveframes action causes the retrieval of the DICOM frames associated with a given study, Series, SOP Instance unique identifier (UID) and frame numbers that are then used to build the response, which is pixel data, and encapsulated in a multipart MIME response. The clients should use the WADO-RS Retrieve Metadata or a QIDO-RS instance level query to get the number of frames (0028,0008) before making this call to retrieve frames.

#### 3.2.11.6.1 Command

<https://mckhost/DICOMRestService/wado/studies/{StudyInstanceUID}/series/{SeriesInstanceUID}/instances/{SOPInstanceUID}/frames/{FrameList}>

#### 3.2.11.6.2 URL Parameters

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 127

StudyInstanceUID – the study instance UID for a study

SeriesInstanceUID – the series UID for a series that belongs to the specified study

SOPInstanceUID – the instance UID for an instance in the specified series

FrameList –Number or list of numbers that are comma separated, representing the set of frames (1 based index) that indicate what frames the client would like from the requested instance.

### 3.2.11.6.3 WADO-RS Retrieve Frames Options

The WADO-RS service shall support RetrieveFrames requests per the standard, 6.5.4.1

**Table 159: Retrieve Frames Options**

Options	Description
Allowable request header Accept values	multipart/related;type=application/octet-stream
	Specifies that the response can be binary DICOM pixel data for one specific frame in Little Endian uncompressed format.
	multipart/related; type={MediaType}
SOP Class Restrictions	Specifies that the response can be pixel data encoded using a {MediaType} chosen from Table 143
	SOP Classes supported in Table 12
Size Restriction	In addition, the WADOS-RS Service Provider can be configured to exclude instances of specific SOP Classes from the retrieval results.
	Restricted to size supported by McKesson Radiology™ System.

### 3.2.11.6.4 WADO-RS Retrieve Frames Response

The WADO-RS service shall provide a response for RetrieveFrames, per standard, 6.5.4.2.

#### 3.2.11.6.4.1 Response Headers

HTTP status codes include all from Table 146.

The HTTP Response contains multi-level headers. The top level HTTP response headers include standard server headers plus a Content-Type of multipart/related with a boundary parameter used to separate the attached parts.

Pixel Data

Content Type

multipart/related; type=application/octet-stream; boundary={MessageBoundary}  
multipart/related; type={MediaType}; boundary={MessageBoundary}

**Table 160: Part Response Header**

Part Response Header	Value
Content-Type	The media type (from table in section 3.2.11.1.2 or 3.2.11.1.3) representing the type of data in the content
Content-Location	The URL is the URL for BulkData to retrieve pixel data for the frame when the Media Type returned is one of in section 3.2.11.1.2 or 3.2.11.1.3

#### 3.2.11.6.4.2 Response Content



**Table 161: Response Content**

A multipart response where each part contains either
1. Pixel data for the requested frames, when the Content-Type header is a media type chosen from the table in "WADO-RS Image Transfer Syntaxes"
2. Binary pixel data in little endian format for the frame specified, when the Content-Type header is application/octet-stream. See "DICOM Little Endian Media-Type / Transfer Syntax"

NOTE1: A requested transfer syntax of 1.2.840.10008.1.2.4.50 (DICOM JPEG Baseline Process 1) only works when the stored instance is 8 bits deep.

### 3.2.11.6.5 Retrieve Frames Example

Retrieving JPEG baseline 1 compressed or lossy JPEG 2000 compressed middle 5 frames from 40 frame instance

Example URL:

<https://mckhost/DICOMRestService/Wado/studies/4.5.6/series/3.4.5/instances/1.2.3/frames/18,19,20,21,22>

**Table 162: Request Headers Sent**

Accept	multipart/related; type=image/dicom+jpeg; transfer-syntax=1.2.840.10008.1.2.4.50
Accept	multipart/related; type=image/dicom+jp2; transfer-syntax=1.2.840.10008.1.2.4.91; q=0.9

NOTE1: The frames/18,19,20,21,22 portion of the URL after the 4.5.6, 3.4.5, 1.2.3 parameters indicate the client wants the middle five frames from the DICOM instance of 40 frames which the client could know because of making a prior WADO Retrieve Metadata or QIDO instance level query (See Table 140).

For the example, the multiple Accept headers sent with the first having media type of image/dicom+jpeg and transfer syntax of DICOM JPEG Baseline process 1 and the second sent having media type image/dicom+jp2 and transfer syntax indicating lossy JPEG 2000 indicates the client prefers the 8 bit deep JPEG that would be directly displayable in a browser if the frames are 8 bits deep, otherwise is willing to accept JPEG 2000 lossy compression (if bit depth is greater than 8). Since the WADO Service Provider supports both media types, the image will be converted to the most preferred type of dicom+jpeg for output. However, if the image turns out to be deeper than 8 bits, then there will be no pixel data returned in the multipart item as the conversion will fail (See 3.2.11.11).

### 3.2.11.7 WADO-RS Retrieve BulkData

The RetrieveBulkData action causes retrieval of the bulk data for a given bulk data URL that are then used to build the response, which is a single bulk data item. The WADO-RS Clients are expected to retrieve bulk data using a bulk data URL obtained from either a WADO-RS Retrieve Metadata Request or from an includefield in the QIDO-RS query response. The WADO-RS Clients are not expected to create a bulk data URL manually.

#### 3.2.11.7.1 Command

The WADO-RS Client is expected to be getting bulk data URLs from either WADO-RS Retrieve Metadata Request or from an includefield in the QIDO-RS query response.

#### 3.2.11.7.2 WADO-RS Retrieve BulkData Options

The WADO-RS Service Provider shall support the RetrieveBulkdata action type per the standard section 6.5.5.1.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 129

**Table 163: Retrieve BulkData Options**

Options	Description
Allowable request header Accept values	multipart/related;type=application/octet-stream  Specifies that the response can be binary bulk data or DICOM pixel data for one specific frame in Little Endian uncompressed format. See Table 144
	multipart/related; type={MediaType}  Specifies that the response is pixel data encoded using a {MediaType} chosen from Table 143. The WADOS-RS clients are expected to use multipart/related; type={MediaType} if they intend to retrieve pixel data in compressed format.
SOP Class	SOP Classes supported in Table 12  In addition, the WADOS-RS Service Provider can be configured to exclude instances of specific SOP Classes from the retrieval results.
Size Restriction	Restricted to size supported by McKesson Radiology™ System.

### 3.2.11.7.3 WADO-RS Retrieve BulkData Response

The WADO-RS Service Provider shall provide a response to the RetrieveBulkdata request per the standard, section 6.5.5.2.

#### 3.2.11.7.3.1 Response Headers

HTTP status codes include all from Table 146.

The HTTP Response contains multi-level headers. The top level HTTP response headers include standard server headers plus a Content-Type of multipart/related with a boundary parameter used to separate the attached parts.

Pixel Data

Content Type

multipart/related; type=application/octet-stream; boundary={MessageBoundary}  
multipart/related; type={MediaType}; boundary={MessageBoundary}

#### 3.2.11.7.3.2 Retrieve BulkData response

**Table 164: Part Response Header**

Part Response Header	Value
Content-Type	The media type (from table in section 3.2.11.1.2 or 3.2.11.1.3) representing the type of data in the content
Content-Location	(1) When Media Type returned is one of those in section 3.2.11.1.3  URL value is for a bulk data URL for uncompressed bulk data element encoded in Little Endian binary format for the specified instance.
	(2) When Media Type returned is one of those in section 3.2.11.1.2  URL value is for a bulk data URL for compressed pixel data for each frame. In the specified SOP Instance.

### 3.2.11.7.3.3 Response Content

**Table 165: Response Content**

A multipart response where each part contains either
1. Pixel data for the specified instance if the media type is the one specified in <b>"WADO-RS Image Transfer Syntaxes"</b> .
2. Uncompressed pixel data if an instance was requested and application/octet-stream was the requested media type. See <b>"DICOM Little Endian Media-Type / Transfer Syntax"</b>
3. Binary element value if the request was for non-pixel data and application/octet-stream was requested. See <b>"DICOM Little Endian Media-Type / Transfer Syntax"</b>

NOTE1: A requested transfer syntax of 1.2.840.10008.1.2.4.50 (DICOM JPEG Baseline Process 1) only works when the stored instance is 8 bits deep.

### 3.2.11.7.4 Retrieve BulkData Example

Retrieve Frame Increment Pointer (tag 0028,0009) from a specified instance. Assume the URL is the Bulkdata URL retrieved by the WADO-RS RetrieveMetadata request.

ExampleURL:

<https://mckhost/DICOMRestService/Wado/studies/4.5.6/series/3.4.5/instances/1.2.3/attrs/00280009>

**Table 166: Request Headers Sent**

Accept	multipart/related; type=application/octet-stream
--------	--

### 3.2.11.8 WADO-RS Retrieve Metadata

The RetrieveMetadata action causes the retrieval of the DICOM instances presented as the full study metadata with the bulk data removed that are then used to build the response, which can be XML or JSON (PS 3.19 or PS 3.18 of the DICOM Standard<sup>1</sup>) encoded metadata for the DICOM attributes. The full study metadata includes all DICOM attributes under a certain size threshold which is determined by the McKesson Radiology™ System.

#### 3.2.11.8.1 Command

<https://mckhost/DICOMRestService/wado/studies/{StudyInstanceUID}/metadata>

#### 3.2.11.8.2 URL Parameters

StudyInstanceUID – the study instance UID for a single study

#### 3.2.11.8.3 WADO-RS Retrieve Metadata Options

The WADO-RS Service Provider supports the RetrieveMetadata action type per the standard section 6.5.6.1

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 131

**Table 167: Retrieve Metadata Options**

Options	Description
Allowable request header Accept values	Supported:  multipart/related; type=application/dicom+xml application/json;  See Table 145
Accept-Encoding	identity (the use of no transformation whatsoever )
SOP Class	SOP Classes supported in Table 12  In addition, the WADO-RS Service Provider can be configured to exclude instances of specific SOP Classes from the retrieval results.
Size Restriction	Restricted to size supported by McKesson Radiology™ System.

### 3.2.11.8.4 WADO-RS Retrieve Metadata Response

The response shall be per WADO-RS standard, sec 6.5.6.2.

#### 3.2.11.8.4.1 Response Headers

HTTP status codes include all from Table 146.

The HTTP Response contains multi-level headers. The top level HTTP response headers include standard server headers plus a Content-Type of multipart/related with a boundary parameter used to separate the attached parts.

Pixel Data

Content Type

multipart/related; type=application/dicom+xml;  
application/json;

#### 3.2.11.8.4.2 Retrieve Metadata response

The response shall be per WADO-RS standard, sec 6.5.6.2.

**Table 168: Part Response Header for application/dicom+xml**

Part Response Header	Value
Content-Type	application/dicom+xml; charset=utf-8

NOTE1: The "application/json" accept type will not generate a multipart response, so there is no "Part Response Header" for this content type. Multiple results returned in JSON are organized as a single top-level array of JSON objects.

#### 3.2.11.8.4.3 Response Content

**Table 169: Response Content**

<b>A multipart response where each part contains</b>
Metadata shall be provided in XML or JSON format

NOTE1: No matter the format the McKesson Radiology™ System has the data stored as; all binary valued elements are returned in the little endian format.

### 3.2.11.8.5 Retrieve Metadata Example

Retrieving metadata from study with study UID 1.2.3.4

Example URL: <https://mckhost/DICOMRestService/Wado/studies/1.2.3.4/metadata>

**Table 170: Request Headers Sent**

Accept	multipart/related; type= application/dicom+xml
Accept	application/json; q = 0.8

NOTE1: For the example, the multiple Accept headers has two entries, the media type of application/dicom+xml with no “q” parameter (equivalent to 1.0) and the media type of application/json and “q” parameter set to 0.8 means that the WADO-RS Service Provider will return a multipart response with each part containing the XML document for each instance in the study. If xml format is not accepted, the WADO-RS Service Provider can return JSON array that contains all metadata for the specified Study.

Since the McKesson Radiology™ system understands both WADO-RS Client requested formats, it will respond to the WADO-RS Client using the client’s preferred format.

### 3.2.11.9 WADO RS Multi-Context Support

The WADO-RS Service Provider supports specifying the context for both Patient ID and Accession Number in the URL for searches.

If the context for the request does not match the context of the study, the accession number returned shall be blank in the WADO-RS response.

For the study's patient, if the patient does not have a patient ID in the context for the request, the patient ID shall be returned as blank.

Example:

[https://mckhost/DICOMRestService/wado/Context/<context\\_code>/studies/1.22.333.4](https://mckhost/DICOMRestService/wado/Context/<context_code>/studies/1.22.333.4)

### 3.2.11.10 Preference Order For Multiple Accept Headers

The WADO-RS Service Provider supports returning data in a supported format chosen from one of the formats that the client sent in an Accept header.

The format chosen by the WADO-RS Service Provider will be the first format supported that is applicable for the data to be returned from the prioritized client indicated formats.

The WADO-RS Service Provider will interpret the client's priority by using the q value in the HTTPS Accept headers, and then for all formats given that have the same q value, by the order in which the client lists the formats. Note that if the format does not include a q value, this is equivalent to the client specifying a q value of 1.0."

### 3.2.11.11 WADO RS Limitations

The WADO-RS Range parameter is not supported.

Accented characters are not supported for case-insensitive searches.

For WADO-RS conversion of an image to a lower bit depth is not supported, due to loss of image fidelity.

For example, a 12-bit image may not be converted to an 8-bit image format.

On-the-fly conversion of proprietary McKesson Radiology formats to DICOM formats is not supported.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 133

For example, conversion of annotations to GSPS and flagged image information to KIN objects is not supported.

### 3.2.11.12 Connection Policies

#### 3.2.11.12.1 General

WADO-RS Service Provider supports TLS Client Certificates for its transport level security support. WADO-RS Service Provider will refuse a connection over TLS from a source that is not signed by a signing certificate the service is configured to allow.

#### 3.2.11.12.2 Security

WADO-RS supports SSL Client Certificates for its transport level security support.

WADO-RS Service Provider supports site level configuration for Cross Origin Resource Sharing (CORS) which allows the resource to be requested from browsers running web applications served from servers in another domain than the one offering the DICOM RESTful services.

## 3.3 Network Interfaces

### 3.3.1 Physical Network Interface

McKesson Radiology™ 12.2 supports a single network interface. One of the following physical network interfaces will be available depending on installed hardware options:

**Table 171: Supported Physical Network Interfaces**

Ethernet 100baseT
Ethernet 10baseT

### 3.3.2 Additional Protocols

McKesson Radiology™ 12.2 conforms to the System Management Profiles listed in the Table below. All requested transactions for the listed profiles and actors are supported. Support for optional transactions is listed in the Table below:

**Table 172: Supported System Management Profiles**

Profile Name	Actor	Protocols Used	Optional Transactions	Security Support
Network Address Management	DHCP Client	DHCP	N/A	N/A
	DNS Client	DNS	N/A	N/A
Time Synchronization	NTP Client <sup>15</sup>	NTP	N/A	N/A

#### 3.3.2.1 DHCP

DHCP can be used to obtain TCP/IP network configuration information. The network parameters obtainable via DHCP are shown in the Table below. The Default Value column of the table shows the default used if the DHCP server does not provide a value. Values for network parameters set in the Service/Installation tool take precedence over values obtained from the DHCP server. Support for DHCP can be configured via the Service/Installation Tool. The Service/Installation tool can be used to configure the machine name. If DHCP is not in use, TCP/IP network configuration information can be manually configured by McKesson MIG Service or Installation staff.

<sup>15</sup> McKesson Radiology™ 12.1.1 EXP1 uses NetTime™ 2.0 for time synchronization, which uses NTP.

**Table 173: Supported DHCP Parameters**

DHCP Parameter	Default Value
IP Address	None
Hostname	Requested machine name
List of NTP servers	Empty list
List of DNS servers	Empty list
Routers	Empty list
Static routes	None
Domain name	None
Subnet mask	Derived from IP Address (see service manual)
Broadcast address	Derived from IP Address (see service manual)
Default router	None
Time offset	Site configurable (from Time Zone)
MTU	Network Hardware Dependent
Auto-IP permission	No permission

### 3.3.2.2 DNS

DNS can be used for address resolution. If DHCP is not in use or the DHCP server does not return any DNS server addresses, the identity of a DNS server can be configured via the Service/Installation Tool. If a DNS server is not in use, local mapping between hostname and IP address can be manually configured by McKesson MIG Service or Installation staff.

## 3.4 Configuration

### 3.4.1 AE Title/Presentation Address Mapping

#### 3.4.1.1 Local AE Titles

All McKesson Radiology™ 12.2 Application Entities use configured AE Titles and TCP/IP Ports. These are assigned default values at the time of installation; However, these can be modified. The AE Title used by each individual application can be configured independently of the AE Title used by other applications on an individual McKesson Radiology™ 12.2 system.

By default, all Application Entities that only act as an Association Requestor are given the same AE Title, whereas those that can act as an Association Acceptor are all given unique AE Titles. It is possible to assign all McKesson Radiology™ 12.2 applications the same AE Title. However, this is not recommended as a single McKesson Radiology™ 12.2 system has multiple DICOM TCP/IP listening ports and associating multiple listening ports with a single AE Title can result in connectivity problems with other systems.

**Table 174: AE Title Configuration**

Application Entity	Default AE Title	Default TCP/IP Port
Sender	ALI_SCU	Not Applicable
Importer	ALI_STORE_SCP	4000
Query/Retrieve Server	ALI_QUERY_SCP	5000
Query/Retrieve Client	ALI_SCU	Not Applicable
Modality Worklist Client	ALI_SCU	Not Applicable
Print Management	ALI_SCU	Not Applicable
External Notifier	ALI_SCU	Not Applicable
Event Handler	ALI_EVENT_SCP	6000
Storage Commitment Client	ALI_EVENT_SCP	6000

### **3.4.1.2 Remote AE Title/Presentation Address Mapping**

The AE Title, host names and port numbers of remote applications can be configured in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff.

#### **3.4.1.2.1 Sender AE**

The AE Titles, TCP/IP port-numbers, and host-names for the remote Storage SCPs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. Multiple remote Storage SCPs can be defined.

#### **3.4.1.2.2 Importer AE**

The AE Titles, TCP/IP port-numbers, host-names and capabilities for the remote Storage SCUs and Storage Commitment Push Model SCUs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff.

The Importer AE can be configured to only accept Associations from systems having specific host-names. The Importer AE cannot presently be configured to check the Calling and Called AE Titles.

#### **3.4.1.2.3 Query/Retrieve Server AE**

The AE Titles, TCP/IP port-numbers, host-names and capabilities for the remote Query/Retrieve SCUs, Storage SCPs (C-MOVE Destination AEs), and Modality Worklist SCUs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. In addition, a mapping must be configured that links a possible C-MOVE Destination AE Title with a specific Presentation Address (host-name and TCP/IP port-number). Otherwise, the Query/Retrieve Server AE will not know where to send the SOP Instances in response to a C-MOVE Request.

The Query/Retrieve Server AE can be configured to only accept Associations from systems having specific host-names. The Query/Retrieve Server AE cannot presently be configured to check the Calling and Called AE Titles.

#### **3.4.1.2.4 Query/Retrieve Client AE**

The AE Titles, TCP/IP port-numbers, and host-names for the remote Query/Retrieve SCPs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. Multiple remote Query/Retrieve SCPs can be defined.

#### **3.4.1.2.5 Modality Worklist Client AE**

The AE Titles, TCP/IP port-numbers, and host-names for the remote Modality Worklist SCPs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. Only a single Modality Worklist SCP can be defined per McKesson Radiology™ 12.2 system.

#### **3.4.1.2.6 Print Management AE**

The AE Titles, TCP/IP port-numbers, and host-names for the remote Print Management SCPs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. Multiple remote Print Management SCPs can be defined.

#### **3.4.1.2.7 External Notifier AE**

The AE Titles, TCP/IP port-numbers, and host-names for the Modality Performed Procedure Step SCPs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. Multiple remote AEs for each supported SOP Class can be defined.

#### **3.4.1.2.8 Event Handler AE**



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 136

The AE Titles, TCP/IP port-numbers, host-names and capabilities for the remote Modality Performed Procedure Step SCUs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff.

### 3.4.1.2.9 Storage Commitment Client AE

The AE Titles, TCP/IP port-numbers, and host-names for the remote Storage Commitment SCPs must be defined in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff.

## 3.4.2 Configurable Parameters

A large number of parameters related to acquisition and general operation can be specified in the McKesson Radiology™ 12.2 configuration files by McKesson MIG Service or Installation staff. The Table below only shows those configuration parameters relevant to DICOM communication. Users of McKesson Radiology™ 12.2 must contact McKesson Service or Installation personnel if they wish to change any of these settings.

**Table 175: Configuration Parameters**

Parameter	Configurable (Yes/No)	Default Value
<b>General Parameters</b>		
Maximum Exported PDU Size (Larger PDUs will never be sent, even if the receiver supports a larger Max PDU Receive Size. If the receiver supports a smaller Max PDU Receive Size, then the Max PDU Send Size will be reduced accordingly for the duration of the Association. Max PDU Receive Size information is exchanged during DICOM Association Negotiation in the Maximum Length Sub-Item of the A-ASSOCIATION-RQ and A-ASSOCIATE-AC)	No	2 <sup>32</sup>
Time-out waiting for a acceptance or rejection response to an Association Request (Application Level Timeout)	No	180s
Time-out waiting for a response to an Association release request (Application Level Timeout)	No	180s
Time-out waiting for completion of a TCP/IP connect request (Low-level timeout)	No	180s
Time-out awaiting a Response to a DIMSE Request (Low-Level Timeout)	No	180s
Time-out for waiting for data between TCP/IP-packets (Low Level Timeout)	No	180s
<b>Sender AE Parameters</b>		
Supported SOP Classes	Yes	SOP Classes listed in Table 4: SOP Class Conformance of Sender AE
Supported Transfer Syntaxes	Yes	Transfer Syntaxes listed in Table 9: Sender AE Proposed Transfer Syntaxes.
Level of tracing for Service Logs (LOW, MEDIUM, HIGH). HIGH means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	HIGH
Remote Modality Worklist SCP AE to be queried by Modality Worklist Client AE. Includes AE Title, host-name, TCP/IP port number, etc.	Yes	NONE
Time-out waiting for a response to a C-STORE-RQ	No	180s
Number of Sender AE application instances that send to a single Storage SCP Remote AE.	Yes	1
Number of times a failed send job may be retried	Yes	20

Parameter	Configurable (Yes/No)	Default Value
Number of times a failed send job may be retried before demoting the send job's priority	Yes	5
CompressImage Attempt to compress all images before exporting them. If set to 'YES', and neither JPEG Lossy or Wavelet compression is enabled then the images will be JPEG Lossless compressed.	Yes	NO
ConvertLosslessToLossy If both this parameter and 'CompressImage' are configured to be 'YES', then the Sender AE will attempt to JPEG Lossy compress images before exporting them using 'CompressionRatio' and 'CineCompressionRatio'.	Yes	NO
ConvertLosslessToWavelet If both this parameter and 'CompressImage' are configured to be 'YES', then the Sender AE will attempt to Wavelet compress images before exporting them using 'CompressionRatio' and 'CineCompressionRatio'. If Wavelet compression fails and 'ConvertLosslessToLossy' is 'YES', then Sender AE will attempt to JPEG Lossy compress images before exporting them.	Yes	NO
ExcludeWaveletForModalities If 'ConvertLosslessToWavelet' is YES, then the images of modalities contained in this list will not be wavelet compressed.	Yes	US, XA
The desired lossy compression ratio for single frame images	Yes	10 : 1
The desired lossy compression ratio for cine images	Yes	30 : 1
Modify or add a configurable set of DICOM Elements in a SOP Instance before it is exported. The set of Elements and the values to assign them are also configurable.	Yes	NO
Process and send any cine files to Remote AE, including decompression if necessary.	Yes	YES
<b>Importer AE Parameters</b>		
Supported SOP Classes	Yes	SOP Classes listed in Table 12: SOP Class Conformance of Importer AE
Supported Transfer Syntaxes	Yes	Transfer Syntaxes listed in Table 22: Importer AE Accepted Transfer Syntaxes
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). HIGH means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	HIGH
Allow any Remote AE on another system to open an Association with the Importer AE. Enable only for demonstration purposes.	Yes	NO
List of host-names that are allowed to open an Association with the Importer AE.	Yes	NONE
Time-out waiting for a response to an N-ACTION-RQ or N-EVENT-RQ	No	180s
Number of Associations that can be active per Remote AE host.	Yes	10
Time to wait on an open Association for the next command (i.e. max time to wait for first C-STORE-RQ after a new Association has been opened).	Yes	3600s
Compression type to be used on received single frame images of a specific Modality Type	Yes	JPEG Lossless (US, CT, MR, CR, NM, RF) NONE (XA)
Compression type to be used on received multi-frame images of a specific Modality Type	Yes	NONE (US)
Compression type to be used if one is not defined for the type	Yes	JPEG Lossless

Parameter	Configurable (Yes/No)	Default Value
of Modality of an image.		
The desired lossy compression ratio for single frame images	Yes	10 : 1
The desired lossy compression ratio for cine images	Yes	30 : 1
List of host-names for which the original SOP Instance UID should be kept even though the images are lossy compressed.	Yes	NONE
Allow a Warning Status Code value to be returned in C-STORE-RSP.	Yes	NO
Create new SOP Instance UIDs for SOP Instances received from the specified Remote AE host-names.	Yes	NO
Receive and parse DICOM SOP Instances in memory rather than immediately writing each received PDU to a file (increases throughput performance but uses more memory resources).	Yes	YES
List of host-names that the Importer AE should always request a new Association with when sending a Storage Commitment N-EVENT-REPORT Request.	Yes	NONE
List of modalities to create a DICOMDIR for each group of SOP Instances received over an Association.	Yes	NONE
<b>Query/Retrieve Server AE</b>		
Supported SOP Classes as an SCU	Yes	SOP Classes listed in Table 12: SOP Class Conformance of Importer AE
Supported Transfer Syntaxes as an SCU	Yes	Transfer Syntaxes listed in Table 22: Importer AE Accepted Transfer Syntaxes
Supported Presentation Contexts as an SCP	Yes	Presentation Contexts listed in Table 36: Query/Retrieve Server AE Accepted Presentation Contexts
Enable IHE Image Manager compliance (full support for Image Level queries and return of additional Elements).	Yes	NO
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	HIGH
Allow any Remote AE on another system to open an Association with the Query/Retrieve Server AE. Enable only for demonstration purposes.	Yes	NO
List of host-names that are allowed to open an Association with the Query/Retrieve Server AE.	Yes	NONE
Time to wait on an open Association for the next command (i.e. max time to wait for first C-FIND-RQ after a new Association has been opened).	Yes	600s
Allow queries with no identifier Attribute values	Yes	NO
Permit Image Level queries	Yes	NO
Whether the Requestor's AE title should be matched against the C-MOVE Destination AE title. If YES, and if the AE Titles are identical, then matching images will be routed to the Requestor's host. If NO, the C-MOVE Destination AE to Host Mapping table (listed below) will be used to resolve AE titles.	Yes	YES
C-MOVE Destination AE to Host Mapping table (Provides AE Title, TCP/IP port number, and host-name for C-MOVE Destination AEs).	Yes	NONE
Number of Associations that can be active per Remote AE host.	Yes	10
List of remote C-MOVE Destination AEs for which images will be compressed before export. If compression is enabled then JPEG Lossless will be used unless some other type is enabled.	Yes	NONE

Parameter	Configurable (Yes/No)	Default Value
List of remote C-MOVE Destination AEs for which images will be JPEG Lossy compressed before export.	Yes	NONE
List of remote C-MOVE Destination AEs for which images will be Wavelet compressed before export. <sup>16</sup>	Yes	NONE
The desired lossy compression ratio for single frame images	Yes	10 : 1
The desired lossy compression ratio for cine images	Yes	30 : 1
Check for Cancel Requests from Remote AE	Yes	NO
List of remote AE Titles to which cine files should not be sent.	Yes	NONE
<b>Query/Retrieve Client AE</b>		
Supported Presentation Contexts as an SCU	Yes	Presentation Contexts listed in Table 53: Query/Retrieve Client AE Proposed Presentation Contexts
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	HIGH
Remote Query/Retrieve SCP AEs to be queried by Query/Retrieve Client AE. Includes AE Title, host-name, TCP/IP port number, etc.	Yes	NONE
Maximum number of query matches to be returned before Query/Retrieve Client AE issues a Cancel Request.	Yes	500
<b>Modality Worklist Client AE</b>		
Supported Presentation Contexts as an SCU	Yes	Presentation Contexts listed in Table 68: Modality Worklist Client AE Proposed Presentation Contexts
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	APP
Remote Modality Worklist SCP AE to be queried by Modality Worklist Client AE. Includes AE Title, host-name, TCP/IP port number, etc.	Yes	NONE
Time interval between queries of Modality Worklist SCP.	Yes	900s
Maximum number of query matches to be returned before Query/Retrieve Client AE issues a Cancel Request.	Yes	200
Time interval, in seconds, to wait for the Modality Worklist SCP to return a C-FIND-RSP.	Yes	120s
<b>Print Management AE</b>		
Supported Presentation Contexts as an SCU	Yes	Presentation Contexts listed in Table 79: Proposed Presentation Contexts
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	HIGH
Remote DICOM Printer AE (AE Title, host-name, TCP/IP port number, etc.).	Yes	NONE
Number of times to retry completing a print-job if some failure occurs.	Yes	0
<b>External Notifier AE</b>		
Supported Presentation Contexts as an SCU	Yes	Presentation Contexts listed in Table 101: External Notifier AE Proposed Presentation Contexts
Level of tracing for Service Logs (LOW, MEDIUM, HIGH,	Yes	HIGH

<sup>16</sup> If Wavelet and JPEG Lossy compression are both enabled then Wavelet compression will take precedence. If that fails then JPEG Lossy compression will be used if enabled. If that in turn fails then JPEG Lossless will be used.

Parameter	Configurable (Yes/No)	Default Value
APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.		
Remote DICOM AE to be notified (AE Title, host-name, TCP/IP port number, etc.).	Yes	NONE
Number of times to retry sending a notification after a failure.	Yes	10
Time to wait before retrying a notification after a failure occurs.	Yes	60s
<b>Event Handler AE</b>		
Supported Presentation Contexts as an SCP	Yes	Presentation Contexts listed in Table 112: Event Handler AE Accepted Presentation Contexts
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	Yes	HIGH
Time to wait on an open Association for the next command (i.e. max time to wait for first C-FIND-RQ after a new Association has been opened).	Yes	300s
Number of Associations that can be active per Remote AE host.	Yes	10
Allow any Remote AE on another system to open an Association with the Event Handler AE. Enable only for demonstration purposes.	Yes	NO
List of host-names that are allowed to open an Association with the Event Handler AE.	Yes	NONE
List of host-names that are allowed to send Messages to Event Handler AE to mark a Study as being Reported.	Yes	NONE
List of host-names that are allowed to send MPPS Messages to Event Handler AE.	Yes	NONE
<b>Storage Commitment Client AE</b>		
Supported Presentation Contexts as an SCU	NO	Presentation Contexts listed in Table 124
Supported Presentation Contexts as an SCP	YES	Presentation Contexts listed in Table 129
Level of tracing for Service Logs (LOW, MEDIUM, HIGH, APP). APP means the least amount of tracing. LOW means the most amount of tracing, including output of all DICOM Message content to the Service Logs.	YES	HIGH
Time to wait on an open Association for the next command (i.e. max time to wait for first C-FIND-RQ after a new Association has been opened).	YES	300s
Number of Associations that can be active per Remote AE host.	YES	10
Allow any Remote AE on another system to open an Association with the Storage Commitment Client AE – Listener is Event Handler AE.	YES	NO
List of host-names that are allowed to open an Association with the Storage Commitment Client AE – Listener is Event Handler AE.	YES	NONE
Determine if the Storage Commit Client AE should wait for the N-EVENT-REPORT on the N-ACTION-RQ association ( WAIT_FOR_RESULT)	YES	YES
Specifies the delay time (in second) before the agent should start processing the Storage Commitment request for a job (START_DELAY)	YES	900s
Specifies the time (in second) to wait for the N-EVENT-REPORT result (RESULT_TIMEOUT)	YES	3600s
Specifies the number of retries before expiring the job	YES	3

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 141


Parameter	Configurable (Yes/No)	Default Value
(RETRY_LIMIT)		
Specifies the delay time in minutes before a job will be re-tried (RETRY_DELAY).	YES	1800s

## 4. MEDIA INTERCHANGE

### 4.1 Implementation Model

#### 4.1.1 Application Data Flow

**Figure 10: McKesson Radiology™ DICOM Media Data Flow Diagram**



The Removable Media AE can export/import DICOM files to/from removable media. A user of McKesson Radiology™ 12.2 can choose to export all DICOM files for a specified study. When importing DICOM files from media, the user can also choose to only import those DICOM files belonging to a specific study. It is not possible to choose to import only particular SOP Instance files or all the files belonging to a particular patient or series.

#### 4.1.2 Functional Definitions of AEs

##### 4.1.2.1 Removable Media AE

The user can select access to removable media present in the system's media drive. They will then be prompted to choose which studies they wish to import into the system. Alternatively, they can choose the option to export a study to removable media. In either case, the system passes control to the Removable Media AE to actually create, read, or update the DICOM removable media.

#### 4.1.3 Sequencing of Real-World Activities

The operator can insert new media at any time before or after invocation of the Removable Media AE through the user interface tool. The Removable Media AE will wait indefinitely for a media to be inserted before starting to export the specified DICOM files. If no media is available, the export job can be canceled by the user.

#### 4.1.4 File Meta Information Options

The implementation information written to the File Meta Header in each exported DICOM file is as follows:

**Table 176: DICOM Implementation Class UID and Version for Media Export**

Implementation Class UID	1.2.840.113711.9
Implementation Version Name	V1.0

## 4.2 AE Specifications

### 4.2.1 Removable Media AE Specification

The Removable Media AE provides standard Conformance to the DICOM Interchange Option of the Media Storage Service Class. Support for a particular Application Profile and role is dependent upon the type of removable media hardware with which the system is equipped. The table below lists all the Application Profiles and roles that can possibly be supported:

**Table 177: Supported Application Profiles, Activities, and Roles**

Application Profile	Real World Activity	FSR <sup>17</sup>	FSC	FSU
STD-GEN-CD	General Purpose CD-R Interchange	YES	YES	NO
STD-US-ID-SF-CDR	Ultrasound Image Display Media Interchange, CD-R.	YES	YES	NO
STD-US-SC-SF-CDR	Ultrasound Image Spatial Calibration Media Interchange, CD-R.	YES	YES	NO
STD-US-CC-SF- CDR	Ultrasound Image Combined Calibration Media Interchange, CD-R.	YES	YES	NO
STD-US-ID-MF- CDR	Ultrasound Image and Multi-frame Image Display Media Interchange, CD-R.	YES	YES	NO
STD-US-SC-MF- CDR	Ultrasound Image and Multi-frame Image Spatial Calibration Media Interchange, CD-R.	YES	YES	NO
STD-US-CC-MF- CDR	Ultrasound Image and Multi-frame Image Combined Calibration Media Interchange, CD-R.	YES	YES	NO
STD-US-ID-SF-MOD128	Ultrasound Image Display Media Interchange, 128MB MOD.	YES	YES	NO
STD-US-SC-SF-MOD128	Ultrasound Image Spatial Calibration Media Interchange, 128MB MOD.	YES	YES	NO
STD-US-CC-SF-MOD128	Ultrasound Image Combined Calibration Media Interchange, 128MB MOD.	YES	YES	NO
STD-US-ID-MF-MOD128	Ultrasound Image and Multi-frame Image Display Media Interchange, 128MB MOD.	YES	YES	NO
STD-US-SC-MF-MOD128	Ultrasound Image and Multi-frame Image Spatial Calibration Media Interchange, 128MB MOD.	YES	YES	NO
STD-US-CC-MF-MOD128	Ultrasound Image and Multi-frame Image Combined Calibration Media Interchange, 128MB MOD.	YES	YES	NO
STD-US-ID-SF-MOD230	Ultrasound Image Display Media Interchange, 230MB MOD.	YES	YES	NO
STD-US-SC-SF-MOD230	Ultrasound Image Spatial Calibration Media Interchange, 230MB MOD.	YES	YES	NO
STD-US-CC-SF-MOD230	Ultrasound Image Combined Calibration Media Interchange, 230MB MOD.	YES	YES	NO
STD-US-ID-MF-MOD230	Ultrasound Image and Multi-frame Image Display Media Interchange, 230MB MOD.	YES	YES	NO
STD-US-SC-MF-MOD230	Ultrasound Image and Multi-frame Image Spatial Calibration Media Interchange, 230MB MOD.	YES	YES	NO
STD-US-CC-MF-MOD230	Ultrasound Image and Multi-frame Image Combined Calibration Media Interchange, 230MB MOD.	YES	YES	NO
STD-US-ID-SF-MOD540	Ultrasound Image Display Media Interchange, 540MB MOD.	YES	YES	NO
STD-US-SC-SF-MOD540	Ultrasound Image Spatial Calibration Media Interchange, 540MB MOD.	YES	YES	NO
STD-US-CC-SF-MOD540	Ultrasound Image Combined Calibration Media Interchange, 540MB MOD.	YES	YES	NO
STD-US-ID-MF-MOD540	Ultrasound Image and Multi-frame Image Display Media Interchange, 540MB MOD.	YES	YES	NO

<sup>17</sup> For the system to act as an FSR or FSC of an Application Profile it must be equipped with the necessary hardware option for writing to the specified media. This is not a standard feature of all McKesson Radiology™ systems.

STD-US-SC-MF-MOD540	Ultrasound Image and Multi-frame Image Spatial Calibration Media Interchange, 540MB MOD.	YES	YES	NO
STD-US-CC-MF-MOD540	Ultrasound Image and Multi-frame Image Combined Calibration Media Interchange, 540MB MOD.	YES	YES	NO
STD-US-ID-SF-MOD640	Ultrasound Image Display Media Interchange, 640MB MOD.	YES	YES	NO
STD-US-SC-SF-MOD640	Ultrasound Image Spatial Calibration Media Interchange, 640MB MOD.	YES	YES	NO
STD-US-CC-SF-MOD640	Ultrasound Image Combined Calibration Media Interchange, 640MB MOD.	YES	YES	NO
STD-US-ID-MF-MOD640	Ultrasound Image and Multi-frame Image Display Media Interchange, 640MB MOD.	YES	YES	NO
STD-US-SC-MF-MOD640	Ultrasound Image and Multi-frame Image Spatial Calibration Media Interchange, 640MB MOD.	YES	YES	NO
STD-US-CC-MF-MOD640	Ultrasound Image and Multi-frame Image Combined Calibration Media Interchange, 640MB MOD.	YES	YES	NO

In addition to supporting these Application Profiles, the Removable Media AE can act as an FSR, or FSC for the DICOM Interchange Option of the Media Storage Service Class for any of the Media Storage Standard SOP Classes listed in Table 178. The system can be configured to support any of the following media types: CD-R, 90mm MODs of 128MB, 230MB, 540MB, or 640MB capacity.

**Table 178: Media Storage Standard SOP Classes Supported by the Removable Media AE**

DICOM SOP Class Name	SOP Class UID	FSR	FSC
12-lead ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	No
Ambulatory ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	No
Basic Voice Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	No
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	No
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11	Yes	No
Comprehensive Structured Report	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	Yes	No
Mammography CAD Structured Report	1.2.840.10008.5.1.4.1.1.88.50	Yes	No
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Yes	No
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Yes	No
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Yes	No
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Yes	Yes
CT Image	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
Digital X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes
Digital X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes
Digital Mammography Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes
Digital Mammography Image (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes
Digital Intra-oral X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.3	Yes	Yes
Breast Tomosynthesis image	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	Yes
Digital Intra-oral X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	Yes
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	No
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1	Yes	No
Hardcopy Color Image	1.2.840.10008.5.1.1.30	Yes	Yes
Hardcopy Grayscale Image	1.2.840.10008.5.1.1.29	Yes	Yes
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	No
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	Yes	Yes
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes



## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is effective as of the last approval date

Page 144

DICOM SOP Class Name	SOP Class UID	FSR	FSC
MR Image	1.2.840.10008.5.1.4.1.1.4	Yes	Yes
Nuclear Medicine Image (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	Yes
Positron Emission Tomography Image	1.2.840.10008.5.1.4.1.1.128	Yes	Yes
Raw Data	1.2.840.10008.5.1.4.1.1.66	Yes	No
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Yes	No
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Yes	No
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Yes	No
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Yes	No
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Yes	No
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Yes	No
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Stand-alone Curve	1.2.840.10008.5.1.4.1.1.9	Yes	No
Stand-alone Modality LUT	1.2.840.10008.5.1.4.1.1.10	Yes	No
Stand-alone Overlay	1.2.840.10008.5.1.4.1.1.8	Yes	No
Stand-alone VOI LUT	1.2.840.10008.5.1.4.1.1.11	Yes	No
Standalone PET Curve	1.2.840.10008.5.1.4.1.1.129	Yes	No
Stored Print	1.2.840.10008.5.1.1.27	Yes	No
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes
Ultrasound Image (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	Yes
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes
Ultrasound Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	Yes
VL Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	Yes
VL Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	Yes
VL Slide-Coordinates Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	Yes
VL Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	Yes
VL Image (Retired)	1.2.840.10008.5.1.4.1.1.77.1	Yes	Yes
VL Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.77.2	Yes	Yes
X-Ray Angiographic Bi-Plane Image (retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	Yes
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes
X-Ray Radiation Dose Structured Report	1.2.840.10008.5.1.4.1.1.88.67	Yes	No
General Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.2	Yes	No
Arterial Pulse Waveform	1.2.840.10008.5.1.4.1.1.9.5.1	Yes	No
Respiratory Waveform	1.2.840.10008.5.1.4.1.1.9.6.1	Yes	No
Colon CAD SR Document	1.2.840.10008.5.1.4.1.1.88.69	Yes	No
Implantation Plan SR Document	1.2.840.10008.5.1.4.1.1.88.70	Yes	No
Encapsulated CDA IOD	1.2.840.10008.5.1.4.1.1.104.2	Yes	No
Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.2	Yes	No
Pseudo-Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.3	Yes	No
Blending Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.4	Yes	No
XA/XRF Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.5	Yes	No
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	No
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	Yes	Yes
Spatial Registration	1.2.840.10008.5.1.4.1.1.66.1	Yes	No
Spatial Fiducials	1.2.840.10008.5.1.4.1.1.66.2	Yes	No
Deformable Spatial Registration	1.2.840.10008.5.1.4.1.1.66.3	Yes	No
Segmentation	1.2.840.10008.5.1.4.1.1.66.4	Yes	No
Surface Segmentation	1.2.840.10008.5.1.4.1.1.66.5	Yes	No
Real World Value Mapping	1.2.840.10008.5.1.4.1.1.67	Yes	No

DICOM SOP Class Name	SOP Class UID	FSR	FSC
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	No
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	No
RT Beams Delivery Instruction	1.2.840.10008.5.1.4.34.7	Yes	No
Video Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1.1	Yes	Yes
Video Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2.1	Yes	Yes
Video Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4.1	Yes	Yes
Ophthalmic Photography 8 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.1	Yes	Yes
Ophthalmic Photography 16 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.2	Yes	Yes
Stereometric Relationship	1.2.840.10008.5.1.4.1.1.77.1.5.3	Yes	No
Lensometry Measurements	1.2.840.10008.5.1.4.1.1.78.1	Yes	No
Autorefractometry Measurements	1.2.840.10008.5.1.4.1.1.78.2	Yes	No
Keratometry Measurements	1.2.840.10008.5.1.4.1.1.78.3	Yes	No
Subjective Refraction Measurements	1.2.840.10008.5.1.4.1.1.78.4	Yes	No
Visual Acuity Measurements	1.2.840.10008.5.1.4.1.1.78.5	Yes	No
Spectacle Prescription Report	1.2.840.10008.5.1.4.1.1.78.6	Yes	No
Ophthalmic Axial Measurements	1.2.840.10008.5.1.4.1.1.78.7	Yes	No
Intraocular Lens Calculations	1.2.840.10008.5.1.4.1.1.78.8	Yes	No
Macular Grid Thickness and Volume Report	1.2.840.10008.5.1.4.1.1.79.1	Yes	No
Ophthalmic Visual Field Static Perimetry Measurements	1.2.840.10008.5.1.4.1.1.80.1	Yes	No
Basic Structured Display IOD	1.2.840.10008.5.1.4.1.1.131	Yes	No
Generic Implant Template	1.2.840.10008.5.1.4.43.1	Yes	No
Implant Assembly Template	1.2.840.10008.5.1.4.44.1	Yes	No
Implant Template Group	1.2.840.10008.5.1.4.45.1	Yes	No
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	Yes	No
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	Yes	No
Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34	Yes	No
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Yes	No
Radiopharmaceutical Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.68	Yes	No

#### 4.2.1.1 File Meta Information for the Application Entity

The Source Application Entity Title included in the File Meta Header is configurable (see section 5.4).

#### 4.2.1.2 Real-World Activities

##### 4.2.1.2.1 Activity – User Imports Files from Removable Media

The Removable Media AE can be used as a File Set Reader (FSR): The user inserts DICOM Removable Media into the system and accesses the DICOM Part 10 format files already written to it. The user will be presented with the list of studies present on the media and can then choose to transfer one or more of these to the McKesson Radiology™ database. According to the DICOM Interchange Option of the Media Storage Service Class, a DICOMDIR shall be included in the DICOM removable Media. The Removable Media AE uses the information from the DICOMDIR to determine the study information for import. But if no DICOMDIR exists, the McKesson Radiology™ Removable Media AE will create a virtual DICOMDIR file from the DICOM files in the directory.

##### 4.2.1.2.2 Activity – User Exports Files to Removable Media

The Removable Media AE can be used as a File Set Creator (FSC): The user can choose to create DICOM Removable Media for export of DICOM files already present in the McKesson Radiology™ database. The user will be prompted to insert empty media into the system and can then choose the particular studies to be written to it. A new DICOMDIR will be created for the DICOM Part 10 format files written to the media.

### 4.2.1.3 Options

In addition to the Media Storage Directory Storage SOP Class listed below, the Removable Media Application Entity supports all the SOP Classes listed in Table 178 and Transfer Syntaxes listed in Table 9: Sender AE Proposed Transfer Syntaxes. It can export or import any DICOM file having a combination of one of the SOP Classes and one of Transfer Syntaxes supported by the Sender AE.

**Table 179: Proposed Presentation Contexts**

Abstract Syntax		Transfer Syntax	
Name	UID	Name	UID
Media Storage Directory Storage	1.2.840.10008.1.3.10	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1
All combinations of SOP Classes listed in Table 178: Media Storage Standard SOP Classes Supported by the Removable Media AE and Transfer Syntaxes listed in Table 9: Sender AE Proposed Transfer Syntaxes.			

## 4.3 Augmented and Private Application Profiles

The Removable Media AE does not support any augmented or private Application Profiles.

## 4.4 Media Configuration

All local applications use the AE Titles configured via the Service/Installation Tool. The Application Entity Titles configurable for Media Services are listed in the Table below:

**Table 180: AE Title Configuration**

Parameter	Configurable (Yes/No)	Default Value
Removable Media AE	No	ALI_STORE_SCP

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 147

## 5. SUPPORT FOR EXTENDED CHARACTER SETS

McKesson Radiology™ 12.2 supports the ISO-IR 100 Latin-1 supplementary character set, and includes this value for the Specific Character Set Attribute (0008,0005).

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 148

## 6. SECURITY

McKesson Radiology™ 12.2 does not support any specific security measures.

It is assumed that McKesson Radiology™ 12.2 is used within a secured environment. It is assumed that a secured environment includes at a minimum:

- Firewall or router protections to ensure that only approved external hosts have network access to McKesson Radiology™ 12.2.
- Firewall or router protections to ensure that McKesson Radiology™ 12.2 only has network access to approved external hosts and services.
- Any communication with external hosts and services outside the locally secured environment use appropriate secure network channels (e.g. such as a Virtual Private Network (VPN))

Other network security procedures such as automated intrusion detection may be appropriate in some environments. Additional security features may be established by the local security policy and are beyond the scope of this conformance statement.

## 7. ANNEXES

### 7.1 IOD Contents

#### 7.1.1 Importer AE Standard Element Use

##### 7.1.1.1 Supported Composite SOP Classes for Display

SOP Instances conforming to the following Composite SOP Classes are fully supported for display on the McKesson Radiology™ System workstation, McKesson Radiology Station™.

**Table 181: Supported Composite Image SOP Classes for Display**

DICOM SOP Class Name	SOP Class UID
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1
CT Image	1.2.840.10008.5.1.4.1.1.2
Digital X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Mammography Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.2 See note 0
Digital Mammography Image (Processing)	1.2.840.10008.5.1.4.1.1.1.2.1
Mammography CAD Structured Report	1.2.840.10008.5.1.4.1.1.88.50
Digital Intra-oral X-Ray Image (Presentation)	1.2.840.10008.5.1.4.1.1.1.3
Breast Tomosynthesis image	1.2.840.10008.5.1.4.1.1.13.1.3 See note 4
Digital Intra-oral X-Ray Image (Processing)	1.2.840.10008.5.1.4.1.1.1.3.1
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1 See note 3
Hardcopy Color Image	1.2.840.10008.5.1.1.30
Hardcopy Grayscale Image	1.2.840.10008.5.1.1.29
Multi-frame Grayscale Byte Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.2
Multi-frame Grayscale Word Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.3
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4
MR Image	1.2.840.10008.5.1.4.1.1.4
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20 See note 5
Nuclear Medicine Image (Retired)	1.2.840.10008.5.1.4.1.1.5
Positron Emission Tomography Image	1.2.840.10008.5.1.4.1.1.128
RT Image	1.2.840.10008.5.1.4.1.1.481.1
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7
Stored Print	1.2.840.10008.5.1.1.27
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1
Ultrasound Image (Retired)	1.2.840.10008.5.1.4.1.1.6
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.3
VL Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1
VL Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2
VL Slide-Coordinates Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.3
VL Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4
VL Image (Retired)	1.2.840.10008.5.1.4.1.1.77.1
VL Multi-frame Image (Retired)	1.2.840.10008.5.1.4.1.1.77.2
X-Ray Angiographic Bi-Plane Image (Retired)	1.2.840.10008.5.1.4.1.1.12.3
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1 See note 0

DICOM SOP Class Name	SOP Class UID
Video Endoscopic Image	1.2.840.10008.5.1.4.1.1.77.1.1.1
Video Microscopic Image	1.2.840.10008.5.1.4.1.1.77.1.2.1
Video Photographic Image	1.2.840.10008.5.1.4.1.1.77.1.4.1
Ophthalmic Photography 8 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.1
Ophthalmic Photography 16 Bit Image	1.2.840.10008.5.1.4.1.1.77.1.5.2

- NOTE1: McKesson Radiology™ 12.2 supports the display Mammography images and Mammo CAD SR as an Image Display Actor for the IHE Mammography Profile.
- NOTE2: The PDF content of Encapsulated PDF SOP Instances can be displayed by the McKesson Radiology™ 12.2 RadReport reporting application.
- NOTE3: McKesson Radiology™ 12.2 includes the ability to display Text and Graphic annotations and other presentation elements (i.e. Shutter, Display Area, VOILUT etc.) in DICOM compliant GSPS objects. See Table 184
- NOTE4: McKesson Radiology™ 12.2 includes the ability to display Digital Breast Tomosynthesis (DBT) images for 64-bit McKesson Radiology Station. A few of the functions include: scroll, power scroll, window/level, zoom, pan, annotate, creation of display protocols that support hanging of both 2D and DBT images and view DBT image data at different slice thicknesses to visualize anatomical regions of interest and calcifications in greater detail (slab DBT images). Please consult with a McKesson Representative for a complete list of features that McKesson Radiology™ 12.2 supports for DBT images.
- NOTE5: McKesson Radiology™ 12.2 supports storing, querying and retrieving of DICOM nuclear medicine images from an external DICOM Application Entity. However, displaying DICOM nuclear medicine images in a format that is useful for analysis or interpretation is not supported without a 3<sup>rd</sup> party nuclear medicine viewer like Segami Oasis, Mirada Fusion XD2 or MedImage MedView. Please consult with a McKesson Representative for more information on 3<sup>rd</sup> party nuclear medicine viewers supported by McKesson Radiology™ 12.2.

### 7.1.1.2 Unsupported Composite SOP Classes for Display

SOP Instances conforming to the following Composite SOP Classes can be received, archived, and exported, but are not supported for display on McKesson Radiology Station™. When a study is opened, any SOP Instances of these particular SOP Classes will not be displayed by the user interface. The contents of some Key Object Selection and Comprehensive SR SOP Instances can be displayed. Refer to the notes below the table for specific details.

**Table 182: Unsupported Composite SOP Classes for Display**

DICOM SOP Class Name	SOP Class UID
12-lead ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.1
Ambulatory ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.3
Basic Voice Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.1
Cardiac Electrophysiology Waveform	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive Structured Report	1.2.840.10008.5.1.4.1.1.88.33
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59 See note 1
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1
Raw Data	1.2.840.10008.5.1.4.1.1.66
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6
RT Dose	1.2.840.10008.5.1.4.1.1.481.2

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 151

DICOM SOP Class Name	SOP Class UID
RT Plan	1.2.840.10008.5.1.4.1.1.481.5
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7
Stand-alone Curve	1.2.840.10008.5.1.4.1.1.9
Stand-alone Modality LUT	1.2.840.10008.5.1.4.1.1.10
Stand-alone Overlay	1.2.840.10008.5.1.4.1.1.8
Stand-alone VOI LUT	1.2.840.10008.5.1.4.1.1.11
Standalone PET Curve	1.2.840.10008.5.1.4.1.1.129
Stored Print	1.2.840.10008.5.1.1.27
X-Ray Radiation Dose Structured Report	1.2.840.10008.5.1.4.1.1.88.67 See Note 2
General Audio Waveform	1.2.840.10008.5.1.4.1.1.9.4.2
Arterial Pulse Waveform	1.2.840.10008.5.1.4.1.1.9.5.1
Respiratory Waveform	1.2.840.10008.5.1.4.1.1.9.6.1
Colon CAD SR Document	1.2.840.10008.5.1.4.1.1.88.69
Implantation Plan SR Document	1.2.840.10008.5.1.4.1.1.88.70
Encapsulated CDA IOD	1.2.840.10008.5.1.4.1.1.104.2
Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.2
Pseudo-Color Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.3
Blending Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.4
XA/XRF Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.5
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2
Spatial Registration	1.2.840.10008.5.1.4.1.1.66.1
Spatial Fiducials	1.2.840.10008.5.1.4.1.1.66.2
Deformable Spatial Registration	1.2.840.10008.5.1.4.1.1.66.3
Segmentation	1.2.840.10008.5.1.4.1.1.66.4
Surface Segmentation	1.2.840.10008.5.1.4.1.1.66.5
Real World Value Mapping	1.2.840.10008.5.1.4.1.1.67
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9
RT Beams Delivery Instruction	1.2.840.10008.5.1.4.34.7
Stereometric Relationship	1.2.840.10008.5.1.4.1.1.77.1.5.3
Lensometry Measurements	1.2.840.10008.5.1.4.1.1.78.1
Autorefractive Measurements	1.2.840.10008.5.1.4.1.1.78.2
Keratometry Measurements	1.2.840.10008.5.1.4.1.1.78.3
Subjective Refraction Measurements	1.2.840.10008.5.1.4.1.1.78.4
Visual Acuity Measurements	1.2.840.10008.5.1.4.1.1.78.5
Spectacle Prescription Report	1.2.840.10008.5.1.4.1.1.78.6
Ophthalmic Axial Measurements	1.2.840.10008.5.1.4.1.1.78.7
Intraocular Lens Calculations	1.2.840.10008.5.1.4.1.1.78.8
Macular Grid Thickness and Volume Report	1.2.840.10008.5.1.4.1.1.79.1
Ophthalmic Visual Field Static Perimetry Measurements	1.2.840.10008.5.1.4.1.1.80.1
Basic Structured Display IOD	1.2.840.10008.5.1.4.1.1.131
Generic Implant Template	1.2.840.10008.5.1.4.43.1
Implant Assembly Template	1.2.840.10008.5.1.4.44.1
Implant Template Group	1.2.840.10008.5.1.4.45.1
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2
Comprehensive 3D SR	1.2.840.10008.5.1.4.1.1.88.34
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40
Radiopharmaceutical Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.68



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 152

NOTE1: McKesson Radiology™ 12.2 includes the ability to 'flag' displayed images that are referenced by a Key Object Selection SOP Instance. This is only displayed if a KOS SOP Instance has a Document Title of "Of Interest" or roughly equivalent meaning ("Of Interest", "For Referring Provider", "For Surgery", etc.). For example, no 'flagging' will be displayed for referenced images of a "Rejected for Quality Reasons" KOS SOP Instance.

NOTE2: McKesson Radiology™ 12.2 supports receiving/storing DICOM X-Ray Radiation Dose SR objects from an external DICOM storage SCU and support sending DICOM X-Ray Radiation Dose SR objects to a remote AE SCP initiated by a DICOM C-MOVE Request for the Study. However, displaying of DICOM X-Ray Radiation Dose SR objects is not supported in McKesson Radiology™ 12.2 without a 3rd party Radiation Tracking product like Radimetrics eXposure that supports displaying the objects and DICOM Q/R for the CT X-Ray Radiation Dose SR objects from McKesson Radiology™ 12.2.

## 7.1.2 Significant Elements in Received Images

The following Elements of Composite SOP Instances received by the Importer AE are either stored to the permanent McKesson Radiology™ database or are of particular importance in the received images:

**Table 183: Significant Elements in Received Images**

Module	Attribute Name	Tag ID	Significance
Patient	Patient Name	(0010,0010)	<ul style="list-style-type: none"> <li>- Importing SCP can be configured to apply a default value if there is no value specified.</li> <li>- Value is saved to database as separate first and last names. Only first and last names are entered in the McKesson Radiology™ database.</li> <li>- Names will be parsed correctly if they are in the format of 'lname'fname' or 'lname, fname'. If space separation is used (i.e. 'lname fname'), then the entire name will be treated as the last name.</li> <li>- McKesson Radiology™ can be configured to convert all names to uppercase only.</li> </ul>
	Patient ID	(0010,0020)	<ul style="list-style-type: none"> <li>- Importing SCP can be configured to apply a default value if there is no value specified.</li> <li>- The Patient ID must be unique.</li> <li>- Verification on incoming Patient IDs is performed. If an ID already exists but the existing name does not match, then the ID is coerced to the form '&lt;original ID&gt;+1'.</li> <li>- Value is saved to database.</li> </ul>
	Issuer of Patient ID	(0010,0021)	<ul style="list-style-type: none"> <li>- For MIMA support only. Used to determine the Patient ID Context</li> <li>- Can be configured by Source.</li> </ul> <p>If the issuer Of Patient ID is not available, the McKesson Radiology™ System can use AE Title in combination with the hostname to determine the patient context. This is configurable by source.</p>
	Other Patient IDs Sequence	(0010,1002)	<ul style="list-style-type: none"> <li>- For MIMA Support only. Used to convey known patient identifiers for the patient.</li> </ul> <p>Used for Patient Matching.</p>
	>Patient ID	(0010,0020)	
	>Issuer of Patient ID	(0010,0021)	
	Patient's Birth Date	(0010,0030)	<ul style="list-style-type: none"> <li>- Importing SCP can be configured to apply a default value if there is no value specified. Value is saved to database.</li> </ul>
	Patient's Sex	(0010,0040)	<ul style="list-style-type: none"> <li>- First character must be 'M', 'm', 'F', 'f', 'O', or 'o'. If a different value or not specified then will be entered in the database as 'U', unknown.</li> <li>- Value is saved to database. (The value 'U' is for internal use only, and is updated to 'O' on export).</li> </ul>
General Study	Study Date	(0008,0020)	<ul style="list-style-type: none"> <li>- Importing SCP can be configured to apply a default value if there is no value specified.</li> <li>- Value is saved to database.</li> </ul>

Module	Attribute Name	Tag ID	Significance
	Accession Number	(0008,0050)	- Importing SCP can be configured to apply a default value if there is no value specified. - Value is saved to database.
	Issuer of Accession Number Sequence	(0008,0051)	- For MIMA Support. Used to identify the Assigning Authority that issued the Accession Number. Used to identify the Study Context in PACS. Can be configured by Source.  If the issuer Of Accession Number Sequence is not available, the McKesson Radiology™ System can use AE Title in combination with the hostname to determine the Study context. This is configurable by source.
	>Local Namespace Entity ID	(0040,0031)	
	>Universal Entity ID	(0040,0032)	
	>Universal Entity ID Type	(0040,0033)	
	Referring Physician's Name	(0008,0090)	- Value is saved to database.
	Study Description	(0008,1030)	- Importer AE can be configured to use the Study Description value for the 'exam type' of the received study. If so configured and the value matches value(s) in the McKesson Radiology™ exam type database, then it will be saved to the database as an exam type.
	Study Instance UID	(0020,000D)	- Must be provided. - Value is saved to database.
General Series	Series Description	(0008,103E)	- Importer AE can be configured to use the Series Description value for the 'exam type' of the received study. If so configured and the value matches value(s) in the McKesson Radiology™ exam type database, then it will be saved to the database as an exam type.
	Modality	(0008,0060)	- Importer AE can be configured to apply a default value if there is no value specified.
	Operator's Name	(0008,1070)	- If name matches a valid User of McKesson Radiology™, then it will be saved to the database as the sonographer of an ultrasound modality series.
	Institution Name	(0008,0080)	For MIMA Support Only. Used to convey the institution where the SOP Instance was created.
	Institution Code Sequence	(0008,0082)	For MIMA Support Only. Used to convey the institution where the SOP Instance was created.
	>Code Value	(0008,0100)	
	>Coding Scheme Designator	(0008,0102)	
	>Coding Scheme Version	(0008,0103)	Required if the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously. May be present otherwise.
	>Code Meaning	(0008,0104)	
General Image	Image Type	(0008,0008)	- Importer AE can be configured to use the Body Part Examined value for the 'exam type' of the received study. If so configured and the value matches value(s) in the McKesson Radiology™ exam type database, then it will be saved to the database as an exam type.
	Pixel Spacing	(0028,0030)	- Used for automatic scaling of measurement tool if specified in an image SOP Instance. - Also can be used for 'true size' printing if the McKesson Radiology™ system is connected to a DICOM printer that supports such functionality.
	Sequence of	(0018,6011)	- Used for automatic scaling of measurement tool if specified in an

Module	Attribute Name	Tag ID	Significance
Calibration	Ultrasound Regions		Ultrasound or Ultrasound Multiframe Image SOP Instance. - Also can be used for 'true size' printing of ultrasound images if the McKesson Radiology™ system is connected to a DICOM printer that supports such functionality.
Image Pixel	Photometric Interpretation	(0028,0004)	- The following photometric interpretations are supported for display purposes: MONOCHROME1, MONOCHROME2, RGB, PALETTE_COLOR, YBR_FULL, YBR_FULL_422, YBR_PARTIAL_422, YBR_ICT, and YBR_RCT. - YBR_FULL_422 and YBR_PARTIAL_422 are only supported for JPEG Lossy Transfer Syntaxes. - YBR_ICT and YBR_RCT are only supported for JPEG 2000 Transfer Syntaxes.
	Bits Allocated	(0028,0100)	- Must be 8 or 16 bits for display purposes. (If Bits Allocated is any other value, the image will be received and stored in the database, but cannot be displayed).
	Bits Stored	(0028,0101)	- All values of 16 or fewer are supported for display purposes
Overlay Plane Module <sup>18</sup>	Overlay Rows	(60xx,0010)	- Required in order to display an Overlay included with a DICOM image SOP Instance.
	Overlay Columns	(60xx,0011)	- Required in order to display an Overlay included with a DICOM image SOP Instance.
	Overlay Type	(60xx,0040)	- Required in order to display an Overlay included with a DICOM image SOP Instance. - Overlay data is used only if the value is "G", Graphics. If included in a DICOM image SOP Instance, then it is automatically displayed with the image. "ROI", Region Of Interest, overlay data is not displayed.
	Overlay Origin	(60xx,0050)	- Required in order to display an Overlay included with a DICOM image SOP Instance. - Value must be 1\1 or greater. If either Overlay Origin coordinate is less than 1, then the overlay is not displayed.
	Overlay Bits Allocated	(60xx,0100)	- Required in order to display an Overlay included with a DICOM image SOP Instance. - Should be 8 or 16 if the overlay data is embedded, and 1 if it is not. However, McKesson Radiology™ actually checks whether the Overlay Data is present for the Overlay Group in order to decide whether the overlay data is actually embedded or not.
	Overlay Bit Position	(60xx,0102)	Required in order to display an Overlay included with a DICOM image SOP Instance. Used if the overlay data is embedded. If the data is embedded, then this position must indicate a bit not used by each image pixel sample.
	Overlay Data	(60xx,3000)	Required in order to display a non-embedded Overlay included with a DICOM image SOP Instance. Data present in this Element or embedded in the pixel data is supported for display. If this Element is present for an Overlay Group and has the required number of values, then these values will be used even if the Overlay Bits Allocated and/or Overlay Bit Position indicate that the overlay data should be embedded.
VOI LUT	Window Center	(0028,1050)	- It is recommended that this value be defined for images that have greater than 8 bits stored per pixel sample for image display.
	Window Width	(0028,1051)	- It is recommended that this value be defined for images that have greater than 8 bits stored per pixel sample for image display.

<sup>18</sup> McKesson Radiology™ can support the display of up to 16 overlays included in an image SOP Instance. If multiple Graphic overlays are present then they are all shown in the displayed image. In addition, McKesson Radiology™ can be configured to extract the values from specific DICOM Elements and create a new overlay to display them with an image.

Module	Attribute Name	Tag ID	Significance
SOP Common	SOP Instance UID	(0008,0018)	<ul style="list-style-type: none"> <li>- Must be provided.</li> <li>- McKesson Radiology™ 12.2 can be configured to do one of two things if a received SOP Instance has the same Study Instance UID and SOP Instance UID as an existing SOP Instance. The default behavior is to not save the newly received SOP Instance. It can also be configured to save the newly received SOP Instance, but this can result in multiple SOP Instances having the same SOP Instance UID.</li> <li>- The system can also be configured to either preserve the original SOP Instance UID or assign a new UID if the received image data is lossy compressed prior to archival. The default behavior is to always assign a new SOP Instance UID.</li> <li>- In addition, McKesson Radiology™ 12.2 can be configured to always assign a new SOP Instance UID to any SOP Instances received from a specific host. This should only be enabled if the remote host is known to make errors when assigning SOP Instances (either assigning duplicates or UIDs that are not DICOM Conformant).</li> </ul>

### 7.1.3 Significant Elements in Received GSPS Instances

The following Elements of GSPS instances received by the Importer AE are supported for Display in McKesson Radiology™ 12.2.

**Table 184: Significant Elements in Received GSPS Instances**

Module	Attribute Name	Tag ID	Type	Description	Usage
Presentation State Relationship	Referenced Series Sequence	(0008,1115)	1	<ul style="list-style-type: none"> <li>- Sequence of Items where each Item includes the Attributes of one Series to which the Presentation applies.</li> <li>- One or more Items shall be present.</li> </ul>	Display supported
	>Series Instance UID	(0020,000E)	1	- Unique identifier of a Series that is part of the Study defined by the Study Instance UID (0020,000D) in the enclosing dataset.	Display supported
	>Referenced Image Sequence	(0008,1140)	1	<ul style="list-style-type: none"> <li>- Sequence of Items where each Item provides reference to a selected set of Image SOP Class/SOP Instance pairs to which the Presentation applies that are part of the Study defined by Study Instance UID (0020,000D) and the Series defined by Series Instance UID (0020,000E).</li> <li>-The referenced SOP Class shall be the same for all Images in any Item of this Referenced Series Sequence (0008,1115). Value is saved to database.</li> <li>- One or more Items shall be present.</li> </ul>	Display supported
	>> Referenced Frame Number	(0008,1160)	1C	<p>Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1.</p> <p>Note: This Attribute may be multi-valued.</p> <p>Required if the Referenced SOP Instance is a multi-frame image and</p>	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	
Presentation State Shutter	Shutter Presentation Value	(0018,1622)	1C	<p>A single grayscale unsigned value used to replace those parts of the image occluded by the shutter, when rendered on a monochrome display. The units are specified in P-Values. Required if the Display Shutter Module or Bitmap Display Shutter Module is present.</p> <p>Note: The requirement in this module is type 1C which overrides the type 3 in the Display Shutter Module.</p> <p>We do not currently support shutter colour value. Our shutters are always black.</p>	Display not supported
	Shutter Presentation Color CIELab Value	(0018,1624)	1C	<p>A color triplet value used to replace those parts of the image occluded by the shutter, when rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See C.10.7.1.1.</p> <p>Required if the Display Shutter Module or Bitmap Display Shutter Module is present and the SOP Class is other than Grayscale Softcopy Presentation State Storage.</p> <p>Note: The requirement in this module is type 1C, which overrides the type 3 in the Display Shutter and Bitmap Display Shutter Modules.</p>	Display not supported
Presentation State Mask	Mask Subtraction Sequence	(0028,6100)	1C		Display not supported
	>Mask Operation	(0028,6101)	1	<p>Type of mask operation to be performed</p> <p>Enumerated Values: AVG_SUB TID</p> <p>See C.7.6.10.1 for further explanation.</p> <p>Note: The requirement in this module is for Enumerated Values which override the requirements of the Mask Module.</p>	Display not supported
	>Contrast Frame	(0028,6112)	1C	Specified the number of contrast frames to average together before	Display not supported

Module	Attribute Name	Tag ID	Type	Description	Usage
	Averaging			performing the mask operation. Required if Mask Frame Numbers (0028,6110) specifies more than one frame (i.e. is multi-valued). Note: The requirement in this module is conditional and overrides the optional requirements of the Mask Module.	
	Recommended Viewing Mode	(0028,1090)	1C	Specifies the recommended viewing protocol(s). Enumerated Value: SUB = for subtraction with mask images Required if Mask Subtraction Sequence (0028,6100) is present. Note: The requirement in this module is type 1C and an Enumerated Value is specified which override the requirements of the Mask Module.	Display not supported
Mask	Mask Subtraction Sequence	(0028,6100)	1	- Defines a sequence that describes mask subtraction operations for a Multiframe Image.  - One or more items shall be included in this sequence.	Display not supported
	Recommended Viewing Mode	(0028,1090)	2	- Specifies the recommended viewing protocol(s). Defined terms:  SUB = for subtraction with mask images; NAT = native viewing of image as sent.  Note: If an implementation does not recognize the defined term for Recommended Viewing Mode (0028,1090), reverting to native display mode is recommended.	Display not supported
Display Shutter	Shutter Shape	(0018,1600)	1	-Shape(s) of the shutter defined for display. Enumerated Values: RECTANGULAR CIRCULAR POLYGONAL  This multi-valued Attribute shall contain at most one of each Enumerated Value. When multiple values are present, and the shutter is applied to a displayed image, then all	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				of the shapes shall be combined and applied simultaneously, that is, the least amount of image remaining shall be visible (unoccluded). See Figure C.7-4b.	
	Shutter Left Vertical Edge	(0018,1602)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the left edge of the rectangular shutter with respect to pixels in the image given as column.	Display supported
	Shutter Right Vertical Edge	(0018,1604)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the right edge of the rectangular shutter with respect to pixels in the image given as column.	Display supported
	Shutter Upper Horizontal Edge	(0018,1606)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the upper edge of the rectangular shutter with respect to pixels in the image given as row.	Display supported
	Shutter Lower Horizontal Edge	(0018,1608)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the lower edge of the rectangular shutter with respect to pixels in the image given as row.	Display supported
	Center of Circular Shutter	(0018,1610)	1C	- Required if Shutter Shape (0018,1600) is CIRCULAR. Location of the center of the circular shutter with respect to pixels in the image given as row and column.	Display supported
	Radius of Circular Shutter	(0018,1612)	1C	- Required if Shutter Shape (0018,1600) is CIRCULAR. Radius of the circular shutter with respect to pixels in the image given as a number of pixels along the row direction.	Display supported
	Vertices of the Polygonal Shutter	(0018,1620)	1C	- Required if Shutter Shape (0018,1600) is POLYGONAL. Multiple Values where the first set of two values are: row of the origin vertex column of the origin vertex Two or more pairs of values follow and are the row and column coordinates of the other vertices of the polygon	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				shutter. Polygon shutters are implicitly closed from the last vertex to the origin vertex and all edges shall be non-intersecting except at the vertices.	
	Shutter Presentation Value	(0018,1622)	3	- A single gray unsigned value used to replace those parts of the image occluded by the shutter, when rendered on a monochrome display. The units are specified in P-Values, from a minimum of 0000H (black) up to a maximum of FFFFH (white).  Note: The maximum P-Value for this Attribute may be different from the maximum P-Value from the output of the Presentation LUT, which may be less than 16 bits in depth.	Display not supported
	Shutter Presentation Color CIE Lab Value	(0018,1624)	3	- A color triplet value used to replace those parts of the image occluded by the shutter, when rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIE Lab. See C.10.7.1.1.	Display not supported
Bitmap Display Shutter	Shutter Shape	(0018,1600)	1	Shape of the shutter defined for display. Enumerated Values are: BITMAP This Attribute shall contain one Value.	Display not supported
	Shutter Overlay Group	(0018,1623)	1	Specifies the Group (60xx) of an Overlay stored within the Presentation State IOD that contains the bitmap data, as defined in the Overlay Plane Module C.9.2.	Display not supported
	Shutter Presentation Value	(0018,1622)	1	A single gray unsigned value used to replace those parts of the image occluded by the shutter, when rendered on a monochrome display. The units are specified in P-Values, from a minimum of 0000H (black) up to a maximum of FFFFH (white).  Note: The maximum P-Value for this Attribute may be different from the maximum P-Value from the output of the Presentation LUT, which may be less than 16 bits in depth.	Display not supported
	Shutter Presentation Color CIE Lab Value	(0018,1624)	3	A color triplet value used to replace those parts of the image occluded by the shutter, when rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIE Lab. See C.10.7.1.1.	Display not supported
Overlay Plane	Overlay Rows	(60xx,0010)	1	Number of Rows in Overlay.	Display not supported



Module	Attribute Name	Tag ID	Type	Description	Usage
	Overlay Columns	(60xx,0011)	1	Number of Columns in Overlay.	Display not supported
	Overlay Type	(60xx,0040)	1	Indicates whether this overlay represents a region of interest or other graphics. Enumerated Values: G = Graphics R = ROI.	Display not supported
	Overlay Origin	(60xx,0050)	1	Location of first overlay point with respect to pixels in the image, given as row\column. The upper left pixel of the image has the coordinate 1\1. Column values greater than 1 indicate the overlay plane origin is to the right of the image origin. Row values greater than 1 indicate the overlay plane origin is below the image origin. Values less than 1 indicate the overlay plane origin is above or to the left of the image origin. Note: Values of 0\0 indicate that the overlay pixels start 1 row above and one column to the left of the image pixels.	Display not supported
	Overlay Bits Allocated	(60xx,0100)	1	Number of Bits Allocated in the Overlay. The value of this Attribute shall be 1. Note: Formerly the standard described embedding the overlay data in the Image Pixel Data (7FE0,0010), in which case the value of this Attribute was required to be the same as Bits Allocated (0028,0100). This usage has been retired. See PS 3.3 2004.	Display not supported
	Overlay Bit Position	(60xx,0102)	1	The value of this Attribute shall be 0. Note: Formerly the standard described embedding the overlay data in the Image Pixel Data (7FE0,0010), in which case the value of this Attribute specified the bit in which the overlay was stored. This usage has been retired. See PS 3.3 2004.	Display not supported
	Overlay Data	(60xx,3000)	1	Overlay pixel data. The order of pixels sent for each overlay is left to right, top to bottom, i.e., the upper left pixel is sent first followed by the remainder of the first row, followed by the first pixel of the 2nd row, then the remainder of the	Display not supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				2nd row and so on. Overlay data shall be contained in this Attribute. See C.9.2.1.1 for further explanation.	
	Overlay Description	(60xx,0022)	3	User-defined comments about the overlay.	Display not supported
	Overlay Subtype	(60xx,0045)	3	Defined term which identifies the intended purpose of the Overlay Type. See C.9.2.1.3 for further explanation.	Display not supported
	Overlay Label	(60xx,1500)	3	A user defined text string which may be used to label or name this overlay.	Display not supported
	ROI Area	(60xx,1301)	3	Number of pixels in ROI area. See C.9.2.1.2 for further explanation.	Display not supported
	ROI Mean	(60xx,1302)	3	ROI Mean. See C.9.2.1.2 for further explanation.	Display not supported
	ROI Standard Deviation	(60xx,1303)	3	ROI standard deviation. See C.9.2.1.2 for further explanation.	Display not supported
Overlay Activation	Overlay Activation Layer	(60xx,1001)	2C	The layer (defined in Graphic Layer (0070,0002) of the Graphic Layer Module C.10.7) in which the Overlay described in group 60xx shall be displayed. If no layer is specified (zero length) then the overlay shall not be displayed.  Required if Group 60xx is present in the referenced image(s) or the Presentation State instance containing this Module.	Display not supported
Display Area	Displayed Area Selection Sequence	(0070,005A)	1	A sequence of Items each of which describes the displayed area selection for a group of images or frames. Sufficient Items shall be present to describe every image and frame listed in the Presentation State Relationship Module.  One or more Items shall be included in this sequence.	Display supported
	>Referenced Image Sequence	(0008,1140)	1C	The subset of images and frames listed in the Presentation State Relationship Module, to which this displayed area selection applies.  One or more Items shall be included in this sequence.  Required if the displayed area selection in this Item does not apply to all the images and frames listed in the Presentation State Relationship Module.	Display supported
	>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	Display supported
	>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	Display supported
	>> Referenced	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
	Frame Number			<p>which the reference applies. The first frame shall be denoted as frame number 1.</p> <p>Note: This Attribute may be multi-valued.</p> <p>Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.</p>	
	>> Referenced Segment Number	(0062,000B)	1C	<p>Identifies the Segment Number to which the reference applies.</p> <p>Required if the Referenced SOP Instance is a Segmentation or Surface Segmentation and the reference does not apply to all segments and Referenced Frame Number (0008,1160) is not present.</p>	Display not supported
	>Pixel Origin Interpretation	(0048,0301)	1C	<p>For a referenced multi-frame image, specifies whether the Displayed Area Top Left Hand Corner (0070,0052) and Displayed Area Bottom Right Hand Corner (0070,0053) are to be interpreted relative to the individual frame pixel origins, or relative to the Total Pixel Matrix origin (see C.8.12.4.1.4).</p> <p>Required if the value of Referenced SOP Class UID (0008,1150) within Referenced Image Sequence (0008,1140) is 1.2.840.10008.5.1.4.1.1.77.1.6 (VL Whole Slide Microscopy Image). May be present otherwise.</p> <p>Enumerated Values:</p> <p>FRAME – relative to individual frame</p> <p>VOLUME – relative to Total Image Matrix</p> <p>If not present, TLHC and BRHC are defined relative to the frame pixel origins.</p>	Display not supported
	>Displayed Area Top Left Hand Corner	(0070,0052)	1	The top left (after spatial transformation) pixel in the referenced image to be displayed, given as column\row. Column is the horizontal (before spatial transformation) offset (X) and row is the vertical (before spatial transformation) offset (Y) relative to the origin of the pixel data before spatial transformation, which is 1\1. See Figure C.10.4-1.	Display supported
	>Displayed Area Bottom Right Hand Corner	(0070,0053)	1	The bottom right (after spatial transformation) pixel in the referenced image to be displayed, given as column\row. Column is the horizontal (before spatial transformation) offset (X) and row is the vertical (before spatial transformation) offset (Y) relative to the origin of the pixel data	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				before spatial transformation, which is 1\1. See Figure C.10.4-1.	
	>Presentation Size Mode	(0070,0100)	1	Manner of selection of display size. Enumerated Values: SCALE TO FIT TRUE SIZE MAGNIFY	Display supported
	>Presentation Pixel Spacing	(0070,0101)	1C	Physical distance between the center of each pixel in the referenced image (before spatial transformation), specified by a numeric pair - adjacent row spacing (delimiter) adjacent column spacing in mm. See 10.7.1.3 for further explanation of the value order.  Notes: 1. This value may be different from Pixel Spacing (0028,0030) or Imager Pixel Spacing (0018,1164) specified in the referenced image, which are ignored, since some form of calibration may have been performed (for example by reference to an object of known size in the image). 2. If the row and column spacing are different, then the pixel aspect ratio of the image is not 1:1.  Required if Presentation Size Mode (0070,0100) is TRUE SIZE, in which case the values will correspond to the physical distance between the center of each pixel on the display device. May be present if Presentation Size Mode (0070,0100) is SCALE TO FIT or MAGNIFY, in which case the values are used to compute the aspect ratio of the image pixels.  Note: McKesson uses the value in the DICOM image header.	Display not supported
	>Presentation Pixel Aspect Ratio	(0070,0102)	1C	Ratio of the vertical size and the horizontal size of the pixels in the referenced image, to be used to display the referenced image, specified by a pair of integer values where the first value is the vertical pixel size and the second value is the horizontal pixel size. See C.7.6.3.1.7. Required if Presentation Pixel Spacing (0070,0101) is not present.	Display not supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				<p>Notes:</p> <ol style="list-style-type: none"> <li>1. This value may be different from the aspect ratio specified by Pixel Aspect Ratio (0028,0034) in the referenced image, or implied by the values of Pixel Spacing (0028,0030) or Imager Pixel Spacing (0018,1164) specified in the referenced image, which are ignored.</li> <li>2. This value must be specified even if the aspect ratio is 1:1.</li> </ol>	
	>Presentation Pixel Magnification Ratio	(0070,0103)	1C	<p>Ratio of displayed pixels to source pixels, specified in one dimension. Required if Presentation Size Mode (0070,0100) is MAGNIFY.</p> <p>Notes:</p> <ol style="list-style-type: none"> <li>1. A value of 1.0 would imply that one pixel in the referenced image would be displayed as one pixel on the display (i.e. it would not be interpolated if the aspect ratio of the image pixels is 1:1).</li> <li>2. A value of 2.0 would imply that one pixel in the referenced image would be displayed as 4 pixels on the display (i.e. up-sampled by a factor of 2 in each of the row and column directions).</li> <li>3. A value of 0.5 would imply that 4 pixels in the referenced image would be displayed as 1 pixel on the display (i.e. down-sampled by a factor of 2 in each of the row and column directions).</li> <li>4. If the source pixels have an aspect ratio of other than 1:1, then they are assumed to have been interpolated to a display pixel aspect ratio of 1:1 prior to magnification.</li> </ol>	Display supported
Graphic Annotation	Graphic Annotation Sequence	(0070,0001)	1	<ul style="list-style-type: none"> <li>- A sequence of Items each of which represents a group of annotations composed of graphics or text or both.</li> <li>- One or more Items shall be present.</li> </ul>	Display supported
	>Referenced	(0008,1140)	1C	<ul style="list-style-type: none"> <li>- Sequence of Items where each Item</li> </ul>	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
	Image Sequence			provides reference to a selected set of Image SOP Class/SOP Instance pairs that are defined in the Presentation State Relationship Module. One or more Items shall be present.  - Required if graphic annotations in this Item do not apply to all the images listed in the Presentation State Relationship Module.	
	>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	Display supported
	>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	Display supported
	>> Referenced Frame Number	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1. Note: This Attribute may be multi-valued. Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	Display supported
	>Graphic Layer	(0070,0002)	1	- The layers in which graphic and text may be Rendered	Display not supported
	>Text Object Sequence	(0070,0008)	1C	- Sequence that describes a text annotation. One or more Items may be present.  - Either one or both of Text Object Sequence (0070,0008) or Graphic Object Sequence (0070,0009) are required .	Display supported
	>>Bounding Box Annotation Units	(0070,0003)	1C	- Units of measure for the axes of the text bounding box.	Display supported
	>>Anchor Point Annotation Units	(0070,0004)	1C	- Units of measure for the axes of the text anchor point annotation.  Enumerated Values for Anchor Point Annotation Units (0070,0004) are the same as for Bounding Box Annotation Units (0070,0003).  - Required if Anchor Point (0070,0014) is present.	Display supported
	>>Unformatted Text Value	(0070,0006)	1	- Text data which is unformatted and whose manner of display within the defined bounding box or relative to the specified anchor point is implementation dependent.  The text value may contain spaces, as	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				well as multiple lines separated by either LF, CR, CR LF or LF CR, but otherwise no format control characters (such as horizontal or vertical tab and form feed) shall be present, even if permitted by the Value Representation of ST.  - In McKesson Radiology™, Text is interpreted as ISO-IR 100	
	>>Bounding Box Top Left Hand Corner	(0070,0010)	1C	- Location of the Top Left Hand Corner (TLHC) of the bounding box in which Unformatted Text Value (0070,0006) is to be displayed, in Bounding Box Annotation Units (0070,0003), given as column\row. Column is the horizontal offset and row is the vertical offset.  - Required if Anchor Point (0070,0014) is not present.	Display supported
	>>Bounding Box Bottom Right Hand Corner	(0070,0011)	1C	- Location of the Bottom Right Hand Corner (BRHC) of the bounding box in which Unformatted Text Value (0070,0006) is to be displayed, in Bounding Box Annotation Units (0070,0003), given as column\row. Column is the horizontal offset and row is the vertical offset.  - Required if Anchor Point (0070,0014) is not present.	Display supported
	>>Bounding Box Text Horizontal Justification	(0070,0012)	1C	- Location of the text relative to the vertical edges of the bounding box. Enumerated Values:  LEFT = closest to left edge RIGHT = closest to right edge CENTER = centered  - Required if Bounding Box Top Left Hand Corner (0070,0010) is present.	Display supported
	>>Anchor Point	(0070,0014)	1C	- Location of a point in the image or Specified Displayed Area to which the Unformatted Text Value (0070,0006) is related, in Anchor Point Annotation Units (0070,0004), given as column\row. Column is the horizontal offset and row is the vertical offset.  - Required if Bounding Box Top Left Hand Corner (0070,0010) and Bounding Box Bottom Right Hand Corner (0070,0011) are not present. May be present even if a bounding box is specified (i.e. Bounding Box Top Left Hand Corner (0070,0010) and Bounding Box Bottom Right Hand Corner (0070,0011) are present).	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
	>>Anchor Point Visibility	(0070,0015)	1C	<p>- Flag to indicate whether or not a visible indication (such as a line or arrow) of the relationship between the text and the anchor point is to be displayed.</p> <p>Enumerated Values:</p> <p>Y = yes N = no</p> <p>- Required if Anchor Point (0070,0014) is present.</p> <p>McKesson Radiology™ does not interpret this tag. An arrow is always present to indicate the relationship between the text and the anchor point.</p>	Display not supported
	>Graphic Object Sequence	(0070,0009)	1C	<p>- Sequence that describes a graphic annotation. One or more Items may be present.</p> <p>- Either one or both of Text Object Sequence (0070,0008) or Graphic Object Sequence (0070,0009) are required.</p>	Display supported
	>>Graphic Annotation Units	(0070,0005)	1C	<p>- Units of measure for the axes of the graphic annotation.</p> <p>Enumerated Values for Graphic Annotation Units (0070,0005) are the same as for Bounding Box Annotation Units (0070,0003).</p>	Display supported
	>>Graphic Dimensions	(0070,0020)	1	<p>Enumerated Value: 2</p> <p>McKesson Radiology™ supports Default Dimensions is 2.</p>	Display supported
	>>Number of Graphic Points	(0070,0021)	1	- Number of data points in this graphic.	Display supported
	>> Graphic Data	(0070,0022)	1	- Coordinates that specify this graphic annotation. Depending on Graphic Type (0070,0023)	Display supported
	>>Graphic Type	(0070,0023)	1	<p>The shape of graphic that is to be drawn.</p> <p>McKesson Radiology™ supports the following graphic types:</p> <p>POINT POLYLINE INTERPOLATED CIRCLE ELLIPSE</p>	Display supported
	>>Graphic Filled	(0070,0024)	1C	<p>- Whether or not the closed graphics element is displayed as filled (in some unspecified manner that shall be distinguishable from an outline) or as an outline.</p> <p>Enumerated Values:</p>	Display supported



Module	Attribute Name	Tag ID	Type	Description	Usage
				<p>Y = yes N = no</p> <p>Required if Graphic Data (0070,0022) is "closed", that is Graphic Type (0070,0023) is CIRCLE or ELLIPSE, or Graphic Type (0070,0023) is POLYLINE or INTERPOLATED and the first data point is the same as the last data point.</p>	
Spatial Transformation	Image Rotation	(0070,0042)	1	<p>How far to rotate the image clockwise in degrees, before any Image Horizontal Flip (0070,0041) is applied.</p> <p>Enumerated Values: 0, 90, 180, 270</p> <p>Notes: Negative values are not permitted since the Value Representation is unsigned.</p> <p><b>Only support rotation 90,180,270 degrees.</b></p>	Display supported
	Image Horizontal Flip	(0070,0041)	1	<p>Whether or not to flip the image horizontally after any Image Rotation has been applied such that the left side of the image becomes the right side.</p> <p>Enumerated Values: Y = yes, N = no</p> <p>Note: No vertical flip is specified since the same result can be achieved by a combination of a 180 degree rotation and a horizontal flip.</p> <p><b>Only support horizontal flip.</b></p>	Display supported
Graphic Layer	Graphic Layer Sequence	(0070,0060)	1	<p>A sequence of Items each of which represents a single layer in which overlays, curves, graphics or text may be rendered.</p> <p>One or more Items shall be included in this sequence.</p> <p>An Item is required for each layer referenced from the Graphic Annotation Module or the Overlay Activation Module.</p>	Display not supported
	>Graphic Layer	(0070,0002)	1	A string which identifies the layer.	Display not supported
	>Graphic Layer Order	(0070,0062)	1	An integer indicating the order in which it is recommended that the layer be rendered, if the display is capable of distinguishing. Lower numbered layers are to be rendered first.	Display not supported
	>Graphic Layer Recommendation	(0070,0066)	3	A default single gray unsigned value in which it is recommended that the layer be rendered on a monochrome	Display not supported

Module	Attribute Name	Tag ID	Type	Description	Usage
	d Display Grayscale Value			display. The units are specified in P-Values from a minimum of 0000H (black) up to a maximum of FFFFH (white). Note: The maximum P-Value for this Attribute may be different from the maximum P-Value from the output of the Presentation LUT, which may be <b>less</b> than 16 bits in depth.	
	>Graphic Layer Recommended Display CIELab Value	(0070,0401)	3	A default color triplet value in which it is recommended that the layer be rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See C.10.7.1.1.	Display not supported
	>Graphic Layer Description	(0070,0068)	3	A free text description of the contents of this layer.	Display not supported
Graphic Group	Graphic Group Sequence	(0070,0234)	1	Sequence that describes the combined graphic object. One or more Items shall be included in this sequence.	Display not supported
	>Graphic Group ID	(0070,0295)	1	A unique number identifying the Graphic Group, i.e. the combined graphic object.	Display not supported
	>Graphic Group Label	(0070,0207)	1	Name used to identify the Graphic Group, i.e. the combined graphic object.	Display not supported
	>Graphic Group Description	(0070,0208)	3	Description of the group.	Display not supported
Modality LUT	Modality LUT Sequence	(0028,3000)	1C	Defines a sequence of Modality LUTs. Only a single Item shall be included in this sequence. Shall not be present if Rescale Intercept (0028,1052) is present.	Display not supported
	>LUT Descriptor	(0028,3002)	1C	Specifies the format of the LUT Data in this Sequence. See C.11.1.1 for further explanation. Required if the Modality LUT Sequence (0028,3000) is sent.	Display not supported
	>LUT Explanation	(0028,3003)	3	Free form text explanation of the meaning of the LUT.	Display not supported
	>Modality LUT Type	(0028,3004)	1C	Specifies the output values of this Modality LUT. See C.11.1.1.2 for further explanation. Required if the Modality LUT Sequence (0028,3000) is sent.	Display not supported
	>LUT Data	(0028,3006)	1C	LUT Data in this Sequence. Required if the Modality LUT Sequence (0028,3000) is sent.	Display not supported
	Rescale Intercept	(0028,1052)	1C	The value b in relationship between stored values (SV) and the output	Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				units specified in Rescale Type (0028,1054). Output units = m*SV + b. Required if Modality LUT Sequence (0028,3000) is not present. Shall not be present otherwise.	
	Rescale Slope	(0028,1053)	1C	m in the equation specified by Rescale Intercept (0028,1052). Required if Rescale Intercept is present.	Display supported
	Rescale Type	(0028,1054)	1C	Specifies the output units of Rescale Slope (0028,1053) and Rescale Intercept (0028,1052). See C.11.1.1.2 for further explanation. Required if Rescale Intercept is present.	Display supported
Softcopy VOI LUT	Softcopy VOI LUT Sequence	(0028,3110)	1	Defines a sequence of VOI LUTs or Window Centers and Widths and to which images and frames they apply. No more than one VOI LUT Sequence containing a single Item or one pair of Window Center/Width values shall be specified for each image or frame. One or more Items shall be included in this sequence.	Display supported
	>Referenced Image Sequence	(0008,1140)	1C	The subset of images and frames listed in the Presentation State Relationship Module, to which this VOI LUT or Window Center and Width applies. One or more Items shall be included in this sequence. Required if the VOI LUT transformation in this Item does not apply to all the images and frames listed in the Presentation State Relationship Module.	Display supported
	>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	Display supported
	>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	Display supported
	>> Referenced Frame Number	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1.  Note: This Attribute may be multi-valued.  Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	Display supported
	>>	(0062,000B)	1C	Identifies the Segment Number to	Display not supported

Module	Attribute Name	Tag ID	Type	Description	Usage
	Referenced Segment Number	)		which the reference applies. Required if the Referenced SOP Instance is a Segmentation or Surface Segmentation and the reference does not apply to all segments and Referenced Frame Number (0008,1160) is not present.	
	> VOI LUT Sequence	(0028,3010)	1C	Defines a sequence of VOI LUTs. One or more Items shall be included in this sequence. Required if Window Center (0028,1050) is not present. May be present otherwise.	Display supported
	>> LUT Descriptor	(0028,3002)	1	Specifies the format of the LUT Data in this Sequence. See C.11.2.1.1 for further explanation.	Display supported
	>> LUT Explanation	(0028,3003)	3	Free form text explanation of the meaning of the LUT. Export as Linear DICOM VOI LUT.	
	>> LUT Data	(0028,3006)	1	LUT Data in this Sequence.	
	>> Window Center	(0028,1050)	1C	Window Center for display. See C.11.2.1.2 for further explanation. Required if VOI LUT Sequence (0028,3010) is not present. May be present otherwise.	Display supported
	>> Window Width	(0028,1051)	1C	Window Width for display. See C.11.2.1.2 for further explanation. Required if Window Center (0028,1050) is sent.	Display supported
	>> Window Center & Width Explanation	(0028,1055)	3	Free form explanation of the meaning of the Window Center and Width. Multiple values correspond to multiple Window Center and Width values.	Display supported
Softcopy Presentation LUT	Presentation LUT Sequence	(2050,0010)	1C	Defines a sequence of Presentation LUTs. Only a single item shall be included in this sequence. Required if Presentation LUT Shape (2050,0020) is absent.	Display not supported
	>LUT Descriptor	(0028,3002)	1	Specifies the format of the LUT Data in this Sequence. See C.11.6.1.1 for further explanation.	Display not supported
	>LUT Explanation	(0028,3003)	3	Free form text explanation of the meaning of the LUT.	Display not supported
	>LUT Data	(0028,3006)	1	LUT Data in this Sequence.	Display not supported
	Presentation LUT Shape	(2050,0020)	1C	Specifies predefined Presentation LUT transformation. Required if Presentation LUT Sequence (2050,0010) is absent. Enumerated Values: IDENTITY - no further translation	Partial Display supported

Module	Attribute Name	Tag ID	Type	Description	Usage
				necessary, input values are P-Values INVERSE - output values after inversion are P-Values See C.11.6.1.2  Only support value of <b>IDENTITY</b>	

### 7.1.4 McKesson Radiology™ Added Private Elements

The McKesson Radiology™ system may add some or all of the following Private Elements to the SOP Instances that it receives:

**Table 185: Private Elements Added by McKesson Radiology™**

Tag ID	Attribute Name	VR	VM	Significance
(3711,00xx)	Private Creator ID	LO	1	- The Private Creator ID for this block of added Private Elements. The value is "A.L.I. Technologies, Inc.".
(3711,xx01)	Filename	LO	1	- Holds the filename of the original SOP Instance.
(3711,xx02)	Data Blob of a Visit	OB	1	- Holds the McKesson Radiology™ system proprietary database information regarding the 'visit' for which the SOP Instance belongs.
(3711,xx03)	Revision Number	US	1	- The revision number of the extended info image.
(3711,xx04)	Unix Timestamp	UL	1	- The Unix format time-stamp of the creation of the extended info image.
(3711,xx05)	Bag ID	IS	1	- The McKesson Radiology™ Bag ID associated with an image.
(3711,xx0C)	Original Study UID	UI	1	- The original Study UID specified in the SOP Instance
(3711,xx0D)	Overlay Grayscale Value	US	1	- The MONOCHROME2 grayscale value (0 to 255) to use when displaying or printing an overlay for the SOP Instance.
(3711,xx0E)	Anonymization Status	CS	1	- Value of "ANONYMIZED" means that the confidential patient information has been removed or replaced in the DICOM header. Note that this does not guarantee that any confidential information 'burned into' the pixel data has been removed.
(3711,xx0F)	Instance Type	CS	1	- The Instance Type of images created on McKesson Radiology™. Possible values: "MOCK" = "mock" image that is added to zero-image studies "MONTAGE" = image is created by VMC Montage feature
(3711,xx30)	IP Converted Frame	LO	1	This tag will be used as a marker which will be checked when a DICOM attribute collection of NM images is being processed. It can be added with a value of "IPConvertedFrame" when McKesson Radiology™ is processing NM images that have multiple frames.
(3711,xxC3)	ALI_SIM_PRIVATE_MC_STRING	LO	1	- Medcon private Tag string that we store and return to the creator of the objects without modifying. This tag is added to MC images and DICOM objects for SIM <sup>19</sup> when McKesson Radiology is archiving these objects.

### 7.1.5 Sender AE and Query/Retrieve Server AE Element Modification

Both the Sender AE and Query/Retrieve Server AE always update SOP Instances with the latest information from the McKesson Radiology™ 12.2 database before exporting them. The following table contains a list of all Elements that can have a value modified by these AE's at the time of export using the Storage Service depending on the capabilities of the receiving remote AE:

<sup>19</sup> SIM - Shared Image Management - With SIM, customers will have one PACS system to learn and maintain instead of having a separate PACS system for both Radiology and Cardiology Studies.

**Table 186: Significant Elements in Exported Composite SOP Instances**

Module	Attribute Name	Tag ID	Significance
Patient	Patient Name	(0010,0010)	- Will be updated with value stored in database prior to export in case the Patient Name was altered after this SOP Instance was originally received.
	Patient ID	(0010,0020)	- Will be updated with value stored in database prior to export in case the Patient ID was altered after this SOP Instance was originally received.
	Patient's Birth Date	(0010,0030)	- Will be updated with value stored in database prior to export in case the Patient's Birth Date value was altered after this SOP Instance was originally received.
	Patient's Sex	(0010,0040)	- Will be updated with value stored in database prior to export in case the Patient's Sex value was altered after this SOP Instance was originally received.
General Study	Study Date	(0008,0020)	- Will be updated with value stored in database prior to export in case the Study Date value was altered after this SOP Instance was originally received.
	Accession Number	(0008,0050)	- Will be updated with value stored in database prior to export in case the Accession Number value was altered after this SOP Instance was originally received.
	Referring Physician's Name	(0008,0090)	- Will be updated with value stored in database prior to export in case the Referring Physician's Name value was altered after this SOP Instance was originally received.
	Study Description	(0008,1030)	- Will be updated with value stored in database prior to export in case the Study Description value was altered after this SOP Instance was originally received.
	Study Instance UID	(0020,000D)	- Will be updated with value stored in database prior to export in case the Study Instance UID value was altered after this SOP Instance was originally received.
General Series	Series Description	(0008,103E)	- Will be updated with value stored in database prior to export in case the Series Description value was altered after this SOP Instance was originally received.
	Modality	(0008,0060)	- Will be updated with value stored in database prior to export in case the Modality value was altered after this SOP Instance was originally received.
	Operator's Name	(0008,1070)	- Will be updated with value stored in database prior to export in case the Operator's Name value was altered after this SOP Instance was originally received.
VOI LUT	Window Center	(0028,1050)	- Default Window Center value can be configured for a specific destination AE.
	Window Width	(0028,1051)	- Default Window Width value can be configured for a specific external destination AE.
SOP Common	SOP Instance UID	(0008,0018)	<p>- The system can also be configured to either preserve the original SOP Instance UID or assign a new UID if the received image data is lossy compressed prior to archival. The default behavior is to always assign a new SOP Instance UID.</p> <p>- In addition, McKesson Radiology™ 12.2 can be configured to always assign a new SOP Instance UID to any SOP Instances received from a specific host. This should only be enabled if the remote host is known to make errors when assigning SOP Instances (either assigning duplicates or UIDs that are not DICOM Conformant).</p>

### 7.1.6 Sender AE MIMA Element Support

The Sender AE sending a SOP Instance shall provide DICOM attributes conveying the Assigning Authorities of the Patient ID and Accession Number. It shall also convey the Institution Name (0008,0080)

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 174

and Institution Code Sequence (0008,0082) so that the institution where the SOP Instance was created is identified.

If there is no patient identifier value defined for the preconfigured default Assigning Authority of the receiving Application Entity then the Patient ID value shall be left blank.

If there is no preconfigured default Assigning Authority for the receiving Application Entity then the Sending AE can specify a Patient ID value from any Assigning Authority in the images.

The Sender AE shall support sending attributes in the images as defined in the following table:

**Table 187: SOP Instance Attributes for Multiple Identity Resolution**

Attribute Name	Tag ID	Description
Patient's Name	(0010,0010)	This Name is referred to as the destination Patient's Name. Required if a Patient Name is known for the patient.
Patient ID	(0010,0020)	Used to identify the patient.  Required if a Patient ID value is known for the Assigning Authority of the destination system. May be present otherwise.  This ID is referred to as the destination Patient ID.
Issuer of Patient ID	(0010,0021)	Used to identify the Assigning Authority (system, organization, agency, or department) that issued the Patient ID.  Required if Patient ID is not empty.
Other Patient IDs Sequence	(0010,1002)	Used to convey known patient identifiers for the patient.  Required if a Patient ID is known for the patient.
>Patient ID	(0010,0020)	
>Issuer of Patient ID	(0010,0021)	
Accession Number	(0008,0050)	Used to identify the order for the Study.
Issuer of Accession Number Sequence	(0008,0051)	Used to identify the Assigning Authority that issued the Accession Number.  Required if Accession Number is not empty.
>Local Namespace Entity ID	(0040,0031)	
>Universal Entity ID	(0040,0032)	
>Universal Entity ID Type	(0040,0033)	
Institution Name	(0008,0080)	Used to convey the institution where the SOP Instance was created.
Institution Code Sequence	(0008,0082)	Used to convey the institution where the SOP Instance was created.
>Code Value	(0008,0100)	
>Coding Scheme Designator	(0008,0102)	
>Coding Scheme Version	(0008,0103)	Required if the value of Coding Scheme Designator (0008,0102) is not sufficient to identify the Code Value (0008,0100) unambiguously. May be present otherwise.
>Code Meaning	(0008,0104)	

### 7.1.7 Derived MPR Image Creation

McKesson Radiology Station™ is capable of creating derived images from CT and MR image sets using Multi-Planar Reconstruction. The created images will belong to the same SOP Class as the images from which they are derived.

### 7.1.7.1 Derived MPR Image IODs

This section describes the IODs of the derived CT and MR SOP Instances by describing the Modules that will be used for such images.

Table 188 specifies the Modules used in the derived CT SOP Instances created by Multi-Planar Reconstruction of received CT images.

**Table 188: IOD of Derived CT SOP Instances**

IE	Module	DICOM Reference (PS3.3)	Value Description Table	Presence of Module
Patient	Patient	C.7.1.1	Table 190	ALWAYS
Study	General Study	C.7.2.1	Table 191	ALWAYS
Series	General Series	C.7.3.1	Table 192	ALWAYS
Frame of Reference	Frame of Reference	C.7.4.1	Table 193	ALWAYS
Equipment	General Equipment	C.7.5.1	Table 194	ALWAYS
Image	General Image	C.7.6.1	Table 195	ALWAYS
	Image Plane	C.7.6.2	Table 196	ALWAYS
	Image Pixel	C.7.6.3	Table 197	ALWAYS
	CT Image	C.8.2.1	Table 200	ALWAYS
	VOI LUT	C.11.2	Table 198	ALWAYS
	SOP Common	C.12.1	Table 199	ALWAYS

Table 189 specifies the Modules used in the derived MR SOP Instances created by Multi-Planar Reconstruction of received MR images.

**Table 189: IOD of Derived MR SOP Instances**

IE	Module	DICOM Reference (PS3.3)	Value Description Table	Presence of Module
Patient	Patient	C.7.1.1	Table 190	ALWAYS
Study	General Study	C.7.2.1	Table 191	ALWAYS
Series	General Series	C.7.3.1	Table 192	ALWAYS
Frame of Reference	Frame of Reference	C.7.4.1	Table 193	ALWAYS
Equipment	General Equipment	C.7.5.1	Table 194	ALWAYS
Image	General Image	C.7.6.1	Table 195	ALWAYS
	Image Plane	C.7.6.2	Table 196	ALWAYS
	Image Pixel	C.7.6.3	Table 197	ALWAYS
	MR Image	C.8.3.1	Table 201	ALWAYS



	VOI LUT	C.11.2	Table 198	ALWAYS
	SOP Common	C.12.1	Table 199	ALWAYS

### 7.1.7.2 Derived MPR Image Module Attributes

This section provides information on the Elements that are part of each module present in the derived CT and MR SOP Instances created by Multi-Planar Reconstruction. For each Element, the Value Description column describes the meaning of the element, whether it must be present in the MPR image header, and what the source of the value is.

The tables use the following abbreviations:

The abbreviations in the “Presence of Value” column are:

VNAP	Value not always present (attribute is always present but may not have a value).
ANAP	Attribute not always present.
ALWAYS	Attribute always present and has a value.
EMPTY	Attribute always present but has no value.

The abbreviations in the “Source” column are:

ORIGINAL	Value is copied from an original image.
DB	Value is from the McKesson Radiology™ system database.
AUTO	Value is automatically generated by the McKesson Radiology™ system.

#### 7.1.7.2.1 Derived MPR Image Common Module Attributes

The following tables specify which Elements from Common Modules can be added to the derived MPR images:

**Table 190: Patient Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Patient's Name	(0010,0010)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Patient ID	(0010,0020)	2	Copied from original acquisition object or database.	ALWAYS	ORIGINAL/ DB
Issuer of Patient ID	(0010,0021)	3	Not present OR copied from original object.	ANAP	ORIGINAL
Patient's Birth Date	(0010,0030)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Patient's Sex	(0010,0040)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Referenced Patient Sequence	(0008,1120)	3	Not present OR copied from original object.	ANAP	ORIGINAL
>Referenced SOP Class UID	(0008,1150)	1C	Not present OR copied from original object.	ANAP	ORIGINAL
>Referenced SOP Instance UID	(0008,1155)	1C	Not present OR copied from original object.	ANAP	ORIGINAL
Patient's Birth Time	(0010,0032)	3	Not present OR copied from original object.	ANAP	ORIGINAL
Other Patient IDs	(0010,1000)	3	Not present OR copied from original object.	ANAP	ORIGINAL
Other Patient Names	(0010,1001)	3	Not present OR copied from original object.	ANAP	ORIGINAL
Ethnic Group	(0010,2160)	3	Not present OR copied from original object.	ANAP	ORIGINAL
Patient Comments	(0010,4000)	3	Not present OR copied from original object.	ANAP	ORIGINAL

**Table 191: General Study Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Study Instance UID	(0020,000D)	1	Copied from original acquisition object or database.	ALWAYS	ORIGINAL/ DB
Study Date	(0008,0020)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Study Time	(0008,0030)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Referring Physician's Name	(0008,0090)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Study ID	(0020,0010)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Accession Number	(0008,0050)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Study Description	(0008,1030)	3	Not present OR copied from original object or database	ANAP	ORIGINAL/ DB
Physician(s) of Record	(0008,1048)	3	Not present OR copied from original object.	ANAP	ORIGINAL
Name of Physician(s) Reading Study	(0008,1060)	3	Not present OR copied from original object.	ANAP	ORIGINAL

**Table 192: General Series Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	1	Copied from original acquisition object or database.	ALWAYS	ORIGINAL/ DB
Series Instance UID	(0020,000E)	1	Empty OR copied from original acquisition object or database.	ALWAYS	ORIGINAL/ DB
Series Number	(0020,0011)	2	Copied from original acquisition object or database if a value is specified. Empty otherwise.	VNAP	ORIGINAL/ DB
Laterality	(0020,0060)	2C	Not present if attribute is not present in original images. Empty if the attribute is specified in the original images.	ANAP	AUTO
Patient Position	(0018,5100)	2C	Not present if attribute is not present in original images. Empty if the attribute is specified in the original images.	ANAP	AUTO

**Table 193: Frame of Reference Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Frame of Reference UID	(0020,0052)	1	Copied from original acquisition object.	ALWAYS	ORIGINAL
Position Reference Indicator	(0020,1040)	2	Copied from original acquisition object if a value is specified. Empty otherwise.	VNAP	ORIGINAL

**Table 194: General Equipment Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Manufacturer	(0008,0070)	2	Value specified as "McKesson Medical Imaging Group"	ALWAYS	AUTO

**Table 195: General Image Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Instance Number	(0020,0013)	2	Value specified as 1 to n for each subsequent MPR image created for a series.	ALWAYS	AUTO
Image Type	(0008,0008)	3	Value specified as "DERIVED\SECONDARY\MP R".	ALWAYS	AUTO
Derivation Description	(0008,2111)	3	Value specified as "MPR" or will indicate the type of compression used and compression ratio if the pixel data has been compressed.	ALWAYS	AUTO
Image Comments	(0020,4000)	3	Value specified as "MPR Image".	ALWAYS	AUTO
Quality Control Image	(0028,0300)	3	Value specified as "NO".	ALWAYS	AUTO
Burned In Annotation	(0028,0301)	3	Value specified as "NO".	ALWAYS	AUTO
Presentation LUT Shape	(2050,0020)	3	Value specified as "INVERSE" if the Photometric Interpretation is MONOCHROME1. Otherwise, the value is "IDENTITY".	ALWAYS	AUTO

**Table 196: Image Plane Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Pixel Spacing	(0028,0030)	1	Calculated based on the values specified in the original images.	ALWAYS	AUTO
Image Orientation	(0020,0037)	1	Calculated based on the orientation of the MPR image relative to that specified for the original images.	ALWAYS	AUTO

Image Position	(0020,0032)	1	Calculated based on the position of the MPR image relative to that specified for the original images.	ALWAYS	AUTO
Slice Thickness	(0018,0050)	2	Copied from original acquisition object if a value is specified. Empty otherwise.	VNAP	ORIGINAL

**Table 197: Image Pixel Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Samples per Pixel	(0028,0002)	1	Identical to that of the original images. For CT and MR this must be 1.	ALWAYS	ORIGINAL
Photometric Interpretation	(0028,0004)	1	Identical to that of the original images. For CT and MR this must be MONOCHROME1 or MONOCHROME2.	ALWAYS	ORIGINAL
Rows	(0028,0010)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
Columns	(0028,0011)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
Bits Allocated	(0028,0100)	1	Identical to that of the original images. For CT and MR this must be 16.	ALWAYS	ORIGINAL
Bits Stored	(0028,0101)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
High Bit	(0028,0102)	1	Always specified as Bits Stored minus 1.	ALWAYS	AUTO
Pixel Representation	(0028,0103)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
Pixel Data	(7FE0,0010)	1	The derived pixel data values calculated using Multi-Planar Reconstruction.	ALWAYS	AUTO

**Table 198: VOI LUT Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Window Center	(0028,1050)	1	Calculated based on the derived MPR image data.	ALWAYS	AUTO
Window Width	(0028,1051)	1	Calculated based on the derived MPR image data.	ALWAYS	AUTO

**Table 199: SOP Common Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
SOP Class UID	(0008,0016)	1	Identical to that of the original images. "1.2.840.10008.5.1.4.1.1.2" (CT) or "1.2.840.10008.5.1.4.1.1.4" (MR).	ALWAYS	ORIGINAL

SOP Instance UID	(0008,0018)	1	New UID generated by the McKesson Radiology Station™ system.	ALWAYS	AUTO
Instance Creation Date	(0008,0012)	3	Date on which the MPR image was created.	ALWAYS	AUTO
Instance Creation Time	(0008,0013)	3	Time at which the MPR image was created.	ALWAYS	AUTO
Instance Number	(0020,0013)	3	Value specified as 1 to n for each subsequent MPR image created for a series.	ALWAYS	AUTO

### 7.1.7.2.2 Derived MPR CT Image Specific Module Attributes

The following table specifies which Elements from CT Image IOD specific Modules can be added to the MPR images derived from original CT images:

**Table 200: CT Image Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Image Type	(0008,0008)	1	Value specified as "DERIVED\SECONDARY\MP R".	ALWAYS	AUTO
Samples per Pixel	(0028,0002)	1	Identical to that of the original images. For CT this must be 1.	ALWAYS	ORIGINAL
Photometric Interpretation	(0028,0004)	1	Identical to that of the original images. For CT this must be MONOCHROME1 or MONOCHROME2.	ALWAYS	ORIGINAL
Bits Allocated	(0028,0100)	1	Identical to that of the original images. For CT this must be 16.	ALWAYS	ORIGINAL
Bits Stored	(0028,0101)	1	Identical to that of the original images. For CT this must be 12 to 16.	ALWAYS	ORIGINAL
High Bit	(0028,0102)	1	Always specified as Bits Stored minus 1.	ALWAYS	AUTO
Rescale Intercept	(0028,1052)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
Rescale Slope	(0028,1053)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
KVP	(0018,0060)	2	Copied from original acquisition object if a value is specified. Empty otherwise.	VNAP	ORIGINAL
Acquisition Number	(0020,0012)	2	No value is specified.	EMPTY	AUTO

### 7.1.7.2.3 Derived MPR MR Image Specific Module Attributes

The following table specifies which Elements from MR Image IOD specific Modules can be added to the MPR images derived from original MR images:

**Table 201: MR Image Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Image Type	(0008,0008)	1	Value specified as "DERIVED\SECONDARY\MP R".	ALWAYS	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Samples per Pixel	(0028,0002)	1	Identical to that of the original images. For MR this must be 1.	ALWAYS	ORIGINAL
Photometric Interpretation	(0028,0004)	1	Identical to that of the original images. For MR this must be MONOCHROME1 or MONOCHROME2.	ALWAYS	ORIGINAL
Bits Allocated	(0028,0100)	1	Identical to that of the original images. For MR this must be 16.	ALWAYS	ORIGINAL
Scanning Sequence	(0018,0020)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
Sequence Variant	(0018,0021)	1	Identical to that of the original images.	ALWAYS	ORIGINAL
Scan Options	(0018,0022)	2	Identical to that of the original images.	VNAP	ORIGINAL
MR Acquisition Type	(0018,0023)	2	Identical to that of the original images.	VNAP	ORIGINAL
Repetition Time	(0018,0080)	2C	Copied from original acquisition object if a value is specified. Empty if attribute is present in original object but has no value. Not present otherwise.	ANAP	ORIGINAL
Echo Time	(0018,0081)	2	Copied from original acquisition object if a value is specified. Empty otherwise.	VNAP	ORIGINAL
Echo Train Length	(0018,0091)	2	Copied from original acquisition object if a value is specified. Empty otherwise.	VNAP	ORIGINAL
Inversion Time	(0018,0082)	2C	Copied from original acquisition object if a value is specified. Empty if attribute is present in original object but has no value. Not present otherwise.	ANAP	ORIGINAL
Trigger Time	(0018,1060)	2C	Copied from original acquisition object if a value is specified. Empty if attribute is present in original object but has no value. Not present otherwise.	ANAP	ORIGINAL

### 7.1.8 Secondary Capture Image Creation for Scanned Document

McKesson Radiology™ can create DICOM Secondary Capture Image objects from documents scanned directly into McKesson Radiology™. The Secondary Capture Image objects can be exported via the Query/Retrieve or Storage Services.

#### 7.1.8.1 Secondary Capture Image IODs for Scanned Document

This section describes the IODs of the Secondary Capture SOP Instances by describing the Modules that will be used for such images.

Table 202 specifies the Modules used in the creation of Secondary Capture SOP Instances for the Scanned Documents in the Study.

**Table 202: IOD of Scanned Document SOP Instances**

IE	Module	DICOM Reference (PS3.3)	Value Description Table	Presence of Module
Patient	Patient	C.7.1.1	Table 203	ALWAYS
Study	General Study	C.7.2.1	Table 204	ALWAYS
Series	General Series	C.7.3.1	Table 205	ALWAYS
Equipment	SC Equipment	C.8.6.1	Table 206	ALWAYS
Image	General Image	C.7.6.1	Table 207	ALWAYS
	Image Pixel	C.7.6.3	Table 208	ALWAYS
	SC Image	C.8.6.2	Table 209	ALWAYS
	SOP Common	C.12.1	Table 210	ALWAYS

### 7.1.8.2 Secondary Capture Image Module Attributes for Scan Document

This section provides information on the Elements that are part of each module present in the Secondary Capture SOP Instances for scanned documents. For each Element, the Value Description column describes the meaning of the element, whether it must be present in the secondary capture image header, and what the source of the value is.

The tables use the following abbreviations:

The abbreviations in the “Presence of Value” column are:

VNAP	Value not always present (attribute is always present but may not have a value).
ANAP	Attribute not always present.
ALWAYS	Attribute always present and has a value.
EMPTY	Attribute always present but has no value.

The abbreviations in the “Source” column are:

ORIGINAL	Value is copied from an original image.
DB	Value is from the McKesson Radiology™ system database.
AUTO	Value is automatically generated by the McKesson Radiology™ system.
D	indicates a default hard-coded value is set.

**Table 203: Patient Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Patient's Name	(0010,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient ID	(0010,0020)	2	Copied from database.	ALWAYS	DB
Patient's Birth Date	(0010,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient's Sex	(0010,0040)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB



**Table 204: General Study Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Study Instance UID	(0020,000D)	1	Copied from database.	ALWAYS	DB
Study Date	(0008,0020)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Time	(0008,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Referring Physician's Name	(0008,0090)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study ID	(0020,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Accession Number	(0008,0050)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Description	(0008,1030)	3	Not present OR copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 205: General Series Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	1	Override by value in SC Equipment Module. Set to "OT"	ALWAYS	D
Series Instance UID	(0020,000E)	1	Generated on SOP Instance Creation.	ALWAYS	AUTO
Series Number	(0020,0011)	2	Set to "0"	ALWAYS	D
Series Description	(0008,103e)	3	Copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 206: SC Equipment Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	3	Set to "SC"	ALWAYS	D
Conversion Type	(0008,0064)	1	Describes the kind of image conversion. Defined Terms :  DV = Digitized Video DI = Digital Interface DF = Digitized Film WSD = Workstation <b>SD = Scanned Document</b> SI = Scanned Image DRW = Drawing SYN = Synthetic Image	ALWAYS	DB

**Table 207: General Image Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Instance Number	(0020,0013)	2	Set to "0"	ALWAYS	D
Derivation Description	(0008,2111)	3	Value will indicate the type of compression used and compression ratio if the pixel data has been compressed.	ANAP	AUTO
Lossy Image Compression	(0028,2110)	3	Specifies whether an Image has undergone lossy compression.  Enumerated Values: 00 = Image has NOT been subjected to lossy compression. 01 = Image has been subjected to lossy compression.	ANAP	AUTO

**Table 208: Image Pixel Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Samples per Pixel	(0028,0002)	1	Number of sample planes in this image  Color Images (3) Monochrome2 (1)	ALWAYS	AUTO
Photometric Interpretation	(0028,0004)	1	Specifies the intended interpretation of the pixel data  Possible values:  YBR_FULL_422 (default for JPEG lossy images)  RGB	ALWAYS	AUTO
Rows	(0028,0010)	1	Depends on Scanned Document JPEG image matrix	ALWAYS	AUTO
Columns	(0028,0011)	1	Depends on Scanned Document JPEG image matrix	ALWAYS	AUTO
Bits Allocated	(0028,0100)	1	8	ALWAYS	D
Bits Stored	(0028,0101)	1	8	ALWAYS	D
High Bit	(0028,0102)	1	7	ALWAYS	D
Pixel Representation	(0028,0103)	1	0000H (unsigned integer)	ALWAYS	D
Pixel Data	(7FE0,0010)	1	The Scanned Document JPEG image will be added as the Pixel Data.	ALWAYS	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Planar Configuration	(0028,0006)	1C	Indicates whether the pixel data are sent color-by-plane or color-by-pixel. Required if Samples per Pixel (0028,0002) has a value greater than 1.  If the image is in color, it will be added with color-by-pixel (0) as its value.	ANAP	AUTO

**Table 209: SC Image Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Pixel Spacing	(0028,0030)	1C	Physical distance in the patient between the center of each pixel, specified by a numeric pair - adjacent row spacing (delimiter) adjacent column spacing in mm. Required if the image has been calibrated. May be present otherwise	ANAP	AUTO

**Table 210: SOP Common Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
SOP Class UID	(0008,0016)	1	1.2.840.10008.5.1.4.1.1.7(OT)	ALWAYS	D
SOP Instance UID	(0008,0018)	1	Generated UID.	ALWAYS	AUTO

### 7.1.9 Grayscale SoftCopy Presentation State Object Creation

In McKesson Radiology™ 12.2, internal (proprietary format) annotations and Presentation State information that are created by the McKesson Radiology™ System can be exported using standard DICOM GSPS SOP Instances. With this feature, annotations and Presentation State information can be consistently displayed and interpreted by DICOM GSPS compliant systems.

This includes Text annotations and graphic annotations (point, polyline, interpolated, circle, eclipse) and other presentation elements (i.e. Shutter, Display Area, VOILUT etc.) described in A.33.1.2 Grayscale Softcopy Presentation State IOD Module Table in part 3 of the 2008 DICOM Standard.

McKesson Radiology™ 12.2 can create one or more DICOM GSPS SOP Instances to represent internal (proprietary format) annotations and Presentation State information in the following workflows: DICOM Archive, DICOM Send, DICOM Query/Retrieve and DICOM media Write.

#### 7.1.9.1 Grayscale SoftCopy Presentation State IODs Modules

This section describes the IODs of the GSPS SOP Instances by describing the Modules that will be used for such objects.

Table 211 specifies the Modules used in the creation of GSPS SOP Instances in the Study.

**Table 211: IOD of GSPS SOP Instances**

IE	Module	DICOM Reference (PS3.3)	Value Description Table	Presence of Module
Patient	Patient	C.7.1.1	Table 212	ALWAYS
Study	General Study	C.7.2.1	Table 213	ALWAYS
Series	General Series	C.7.3.1	Table 214	ALWAYS
	Presentation Series	C.11.9	Table 215	ALWAYS
Equipment	General Equipment	C.7.5.1	Table 216	ALWAYS
Presentation State	Presentation State Identification	C.11.10	Table 217	ALWAYS
	Presentation State Relationship	C.11.11	Table 219	ALWAYS
	Presentation State Shutter	C.11.12	Table 222	UNSUPPORTED
	Presentation State Mask	C.11.13	Table 223	UNSUPPORTED
	Mask	C.7.6.10	Table 224	UNSUPPORTED
	Display Shutter	C.7.6.11	Table 225	UNSUPPORTED
	Bitmap Display Shutter	C.7.6.15	Table 226	UNSUPPORTED
	Overlay Plane	C.9.2	Table 227	UNSUPPORTED
	Overlay Activation	C.11.7	Table 228	UNSUPPORTED
	Displayed Area	C.10.4	Table 229	ALWAYS
	Graphic Annotation	C.10.5	Table 230	ALWAYS
	Spatial Transformation	C.10.6	Table 231	UNSUPPORTED
	Graphic Layer	C.10.7	Table 232	UNSUPPORTED
	Graphic Group	C.10.11	Table 233	UNSUPPORTED
	Modality LUT	C.11.1	Table 234	UNSUPPORTED
	Softcopy VOI LUT	C.11.8	Table 235	ALWAYS
	Softcopy Presentation LUT	C.11.6	Table 236	UNSUPPORTED See Note 1
	SOP Common	C.12.1	Table 237	ALWAYS

### 7.1.9.2 Grayscale SoftCopy Presentation State Module Attributes

This section provides information on the Elements that are part of each module present in the GSPS SOP Instances. For each Element, the Value Description column describes the meaning of the element, whether it must be present in the GSPS instance header, and what the source of the value is.

The tables use the following abbreviations:

The abbreviations in the “Presence of Value” column are:

VNAP	Value not always present (attribute is always present but may not have a value).
ANAP	Attribute not always present.
ALWAYS	Attribute always present and has a value.

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 188

EMPTY Attribute always present but has no value.  
 UNSUPPORTED Attribute not supported

The abbreviations in the “Source” column are:

ORIGINAL Value is copied from an original image.  
 DB Value is from the McKesson Radiology™ system database.  
 AUTO Value is automatically generated by the McKesson Radiology™ system.  
 D indicates a default hard-coded value is set.  
 NA Value not applicable

NOTE1: Only support export IDENTITY value for Presentation LUT shape

**Table 212: Patient Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Patient's Name	(0010,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient ID	(0010,0020)	2	Copied from database.	ALWAYS	DB
Patient's Birth Date	(0010,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient's Sex	(0010,0040)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB

**Table 213: General Study Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Study Instance UID	(0020,000D)	1	Copied from database.	ALWAYS	DB
Study Date	(0008,0020)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Time	(0008,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Referring Physician's Name	(0008,0090)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study ID	(0020,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Accession Number	(0008,0050)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Description	(0008,1030)	3	Not present OR copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 214: General Series Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
----------------	-----	------	-------------------	-------------------	--------

Modality	(0008,0060)	1	Set to "PR"	ALWAYS	D
Series Instance UID	(0020,000E)	1	Generated on SOP Instance Creation. All GSPS SOP Instances in the same study has the same Series Instance UID.	ALWAYS	AUTO
Series Number	(0020,0011)	2	Set to "1"	ALWAYS	D
Series Description	(0008,103e)	3	Copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 215: Presentation Series Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	1	The Presentation Series Module specializes some Attributes of the General Series Module. Set to "PR"	ALWAYS	D

**Table 216: General Equipment Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Manufacturer	(0008,0070)	2	Value specified as "McKesson"	ALWAYS	AUTO

**Table 217: Presentation State Identification Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Presentation Creation Date	(0070,0082)	1	Date on which this presentation was created.  Note: This date may be different from the date that the DICOM SOP Instance was created, since the presentation state information contained may have been recorded earlier.  Use the last modified date of McKesson Radiology Internal/proprietary annotation or presentation files.	ALWAYS	AUTO
Presentation Creation Time	(0070,0083)	1	Time at which this presentation was created.  Note: This time may be different from the time that the DICOM SOP Instance was created, since the presentation state information contained may have been recorded earlier.  Use the last modified time of McKesson Radiology Internal/proprietary annotation or presentation files.	ALWAYS	AUTO
Include Content Identification Macro Table 10-12			Note: The Content Label value may be used by an application as a Defined Term in order to imply some grouping of different presentation states, i.e. it may have the same value for different presentation state instances that share some common concept.	ALWAYS	AUTO

**Table 218: Content Identification Macro Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Instance Number	(0020,0013)	1	Set to "1"	ALWAYS	D
Content Label	(0070,0080)	1	A label that is used to identify this SOP Instance.  Set to "MCKESSONEMI GSPS"	ALWAYS	D
Content Description	(0070,0081)	2	A description of the content of the SOP Instance.	EMPTY	D
Content Creator's Name	(0070,0084)	2	Name of operator (such as a technologist or physician) creating the content of the SOP Instance.	EMPTY	D

**Table 219: Presentation State Relationship Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Referenced Series Sequence	(0008,1115)	1	- Sequence of Items where each Item includes the Attributes of one Series to which the Presentation applies. - One or more Items shall be present.	ALWAYS	AUTO
>Series Instance UID	(0020,000E)	1	- Unique identifier of a Series that is part of the Study defined by the Study Instance UID (0020,000D) in the enclosing dataset.	ALWAYS	DB
>Referenced Image Sequence	(0008,1140)	1	- Sequence of Items where each Item provides reference to a selected set of Image SOP Class/SOP Instance pairs to which the Presentation applies that are part of the Study defined by Study Instance UID (0020,000D) and the Series defined by Series Instance UID (0020,000E).  -The referenced SOP Class shall be the same for all Images in any Item of this Referenced Series Sequence (0008,1115). Value is saved to database.  - One or more Items shall be present.	EMPTY	AUTO
>>Include Image SOP Instance Reference Macro, Table 220					

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 191

**Table 220: Image SOP Instance Macro Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Include 'SOP Instance Reference Macro' Table 221					
Referenced Frame Number	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1.  Note: This Attribute may be multi-valued.  Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	ANAP	ORIGINAL
Referenced Segment Number	(0062,000B)	1C	Identifies the Segment Number to which the reference applies. Required if the Referenced SOP Instance is a Segmentation or Surface Segmentation and the reference does not apply to all segments and Referenced Frame Number (0008,1160) is not present.	UNSUPPORTED	NA

**Table 221: SOP Instance Reference Macro Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	ALWAYS	ORIGINAL
Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	ALWAYS	ORIGINAL

**Table 222: Presentation State Shutter Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Shutter Presentation Value	(0018,1622)	1C	A single grayscale unsigned value used to replace those parts of the image occluded by the shutter, when rendered on a monochrome display. The units are specified in P-Values. Required if the Display Shutter Module or Bitmap Display Shutter Module is present. Note: The requirement in this module is type 1C which overrides the type 3 in the Display Shutter Module.  - Export not supported	UNSUPPORTED	NA
Shutter Presentation Color CIELab Value	(0018,1624)	1C	A color triplet value used to replace those parts of the image occluded by the shutter, when rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See C.10.7.1.1. Required if the Display Shutter Module or Bitmap Display Shutter Module is present and the SOP Class is other than Grayscale Softcopy Presentation State Storage.	UNSUPPORTED	DB



Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			<p>Note: The requirement in this module is type 1C, which overrides the type 3 in the Display Shutter and Bitmap Display Shutter Modules.</p> <p><b>- Export not supported</b></p>		

NOTE1: This table contains Attributes that specialize Attributes in other Modules included in a Presentation State.

**Table 223 Presentation State Mask Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Mask Subtraction Sequence	(0028,6100)	1C			NA
>Mask Operation	(0028,6101)	1	<p>Type of mask operation to be performed</p> <p>Enumerated Values: AVG_SUB TID</p> <p>See C.7.6.10.1 for further explanation.</p> <p>Note: The requirement in this module is for Enumerated Values which override the requirements of the Mask Module.</p> <p><b>- Export not supported</b></p>	<p>UNSUPPORTED</p> <p>Required if Mask Module is present. Only a single Item shall be included in this sequence. Applicable Frame Range (0028,6102) shall not be included in the Sequence Item.</p> <p>See C.7.6.10 for a complete definition of the Attributes in the Items of this Sequence other than Mask Operation(0028,6101) and Applicable Frame Range (0028,6102).</p> <p>Notes:</p> <p>1. This Sequence is replicated here in order to specify one Item, additional conditions on Mask Operation (0028,6101) and to forbid Applicable Frame Range (0028,6102).</p>	DB

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
				2. The role of Applicable Frame Range (0028,6102) is replaced by Referenced Frame Number (0008,1160).	
>Contrast Frame Averaging	(0028,6112)	1C	<p>Specified the number of contrast frames to average together before performing the mask operation.</p> <p>Required if Mask Frame Numbers (0028,6110) specifies more than one frame (i.e. is multi-valued).</p> <p>Note: The requirement in this module is conditional and overrides the optional requirements of the Mask Module.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
Recommended Viewing Mode	(0028,1090)	1C	<p>Specifies the recommended viewing protocol(s).</p> <p>Enumerated Value: SUB = for subtraction with mask images</p> <p>Required if Mask Subtraction Sequence (0028,6100) is present.</p> <p>Note: The requirement in this module is type 1C and an Enumerated Value is specified which override the requirements of the Mask Module.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA

NOTE1: This table contains Attributes that specialize the use of masks in a Presentation State

**Table 224: Mask Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Mask Subtraction Sequence	(0028,6100)	1	<p>- Defines a sequence that describes mask subtraction operations for a Multiframe Image.</p> <p>- One or more items shall be included in this sequence.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
Recommended Viewing Mode	(0028,1090)	2	<p>- Specifies the recommended viewing protocol(s). Defined terms:</p> <p>SUB = for subtraction with mask images; NAT = native viewing of image as sent.</p> <p>Note: If an implementation does not recognize the defined term for Recommended Viewing Mode (0028,1090), reverting to native display mode is recommended.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA

**Table 225: Display Shutter Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Shutter Shape	(0018,1600)	1	<p>-Shape(s) of the shutter defined for display. Enumerated Values: RECTANGULAR CIRCULAR POLYGONAL</p> <p>This multi-valued Attribute shall contain at most one of each Enumerated Value. When multiple values are present, and the shutter is applied to a displayed image, then all of the shapes shall be combined and applied simultaneously, that is, the least amount of image remaining shall be visible (unoccluded). See Figure C.7-4b.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
Shutter Left Vertical Edge	(0018,1602)	1C	<p>- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the left edge of the</p>	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			rectangular shutter with respect to pixels in the image given as column.  <b>- Export not supported</b>		
Shutter Right Vertical Edge	(0018,1604)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the right edge of the rectangular shutter with respect to pixels in the image given as column.  <b>- Export not supported</b>	UNSUPPORTED	NA
Shutter Upper Horizontal Edge	(0018,1606)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the upper edge of the rectangular shutter with respect to pixels in the image given as row.  <b>- Export not supported</b>	UNSUPPORTED	NA
Shutter Lower Horizontal Edge	(0018,1608)	1C	- Required if Shutter Shape (0018,1600) is RECTANGULAR. Location of the lower edge of the rectangular shutter with respect to pixels in the image given as row.  <b>- Export not supported</b>	UNSUPPORTED	NA
Center of Circular Shutter	(0018,1610)	1C	- Required if Shutter Shape (0018,1600) is CIRCULAR. Location of the center of the circular shutter with respect to pixels in the image given as row and column.  <b>- Export not supported</b>	UNSUPPORTED	NA
Radius of Circular Shutter	(0018,1612)	1C	- Required if Shutter Shape (0018,1600) is CIRCULAR. Radius of the circular shutter with respect to pixels in the image given as a number of pixels along the row direction.  <b>- Export not supported</b>	UNSUPPORTED	NA
Vertices of the Polygonal Shutter	(0018,1620)	1C	- Required if Shutter Shape (0018,1600) is POLYGONAL. Multiple Values where the first set of two values are: row of the origin vertex column of the origin vertex Two or more pairs of values follow and are the row and	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			column coordinates of the other vertices of the polygon shutter. Polygon shutters are implicitly closed from the last vertex to the origin vertex and all edges shall be non-intersecting except at the vertices.  <b>- Export not supported</b>		
Shutter Presentation Value	(0018,1622)	3	- A single gray unsigned value used to replace those parts of the image occluded by the shutter, when rendered on a monochrome display. The units are specified in P-Values, from a minimum of 0000H (black) up to a maximum of FFFFH (white).  Note: The maximum P-Value for this Attribute may be different from the maximum P-Value from the output of the Presentation LUT, which may be less than 16 bits in depth.  <b>- Export not supported</b>	UNSUPPORTED	NA
Shutter Presentation Color CIELab Value	(0018,1624)	3	- A color triplet value used to replace those parts of the image occluded by the shutter, when rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See C.10.7.1.1.  <b>- Export not supported</b>	UNSUPPORTED	NA

**Table 226: Bitmap Display Shutter Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Shutter Shape	(0018,1600)	1	Shape of the shutter defined for display. Enumerated Values are: BITMAP This Attribute shall contain one Value.  <b>- Export not supported</b>	UNSUPPORTED	NA
Shutter Overlay Group	(0018,1623)	1	Specifies the Group (60xx) of an Overlay stored within the Presentation State IOD that contains the bitmap data, as defined in the Overlay Plane Module C.9.2.  <b>- Export not supported</b>	UNSUPPORTED	NA
Shutter Presentation Value	(0018,1622)	1	A single gray unsigned value used to replace those parts of the image occluded by the shutter, when rendered on a monochrome display. The units are specified in P-Values, from a minimum of 0000H (black) up to a maximum of FFFFH (white). Note: The maximum P-Value for this Attribute may be different from the maximum P-Value from the output of the Presentation LUT, which may be less than 16 bits in depth.  <b>- Export not supported</b>	UNSUPPORTED	NA
Shutter Presentation Color CIELab Value	(0018,1624)	3	A color triplet value used to replace those parts of the image occluded by the shutter, when rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See C.10.7.1.1.  <b>- Export not supported</b>	UNSUPPORTED	NA

**Table 227: Overlay Plane Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Overlay Rows	(60xx,0010)	1	Number of Rows in Overlay.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Columns	(60xx,0011)	1	Number of Columns in Overlay.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Type	(60xx,0040)	1	Indicates whether this overlay represents a region of interest or other graphics. Enumerated Values:  G = Graphics R = ROI.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Origin	(60xx,0050)	1	Location of first overlay point with respect to pixels in the image, given as row\column. The upper left pixel of the image has the coordinate 1\1. Column values greater than 1 indicate the overlay plane origin is to the right of the image origin. Row values greater than 1 indicate the overlay plane origin is below the image origin. Values less than 1 indicate the overlay plane origin is above or to the left of the image origin. Note: Values of 0\0 indicate that the overlay pixels start 1 row above and one column to the left of the image pixels.	UNSUPPORTED	NA
Overlay Bits Allocated	(60xx,0100)	1	Number of Bits Allocated in the Overlay. The value of this Attribute shall be 1. Note: Formerly the standard described embedding the overlay data in the Image Pixel Data (7FE0,0010), in which case the value of this Attribute was required to be the same as Bits Allocated (0028,0100). This usage has been retired. See PS 3.3 2004.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Bit Position	(60xx,0102)	1	The value of this Attribute shall be	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			0. Note: Formerly the standard described embedding the overlay data in the Image Pixel Data (7FE0,0010), in which case the value of this Attribute specified the bit in which the overlay was stored. This usage has been retired. See PS 3.3 2004.  <b>- Export not supported</b>	D	
Overlay Data	(60xx,3000)	1	Overlay pixel data. The order of pixels sent for each overlay is left to right, top to bottom, i.e., the upper left pixel is sent first followed by the remainder of the first row , followed by the first pixel of the 2nd row, then the remainder of the 2nd row and so on. Overlay data shall be contained in this Attribute. See C.9.2.1.1 for further explanation.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Description	(60xx,0022)	3	User-defined comments about the overlay.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Subtype	(60xx,0045)	3	Defined term which identifies the intended purpose of the Overlay Type. See C.9.2.1.3 for further explanation.  <b>- Export not supported</b>	UNSUPPORTED	NA
Overlay Label	(60xx,1500)	3	A user defined text string which may be used to label or name this overlay.  <b>- Export not supported</b>	UNSUPPORTED	NA
ROI Area	(60xx,1301)	3	Number of pixels in ROI area. See C.9.2.1.2 for further explanation.  <b>- Export not supported</b>	UNSUPPORTED	NA
ROI Mean	(60xx,1302)	3	ROI Mean. See C.9.2.1.2 for further explanation.	UNSUPPORTED	NA



Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			- Export not supported		
ROI Standard Deviation	(60xx,1303)	3	ROI standard deviation. See C.9.2.1.2 for further explanation.	UNSUPPORTED	NA
			- Export not supported		

Table 228: Overlay Activation Module Attributes

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Overlay Activation Layer	(60xx,1001)	2C	The layer (defined in Graphic Layer (0070,0002) of the Graphic Layer Module C.10.7) in which the Overlay described in group 60xx shall be displayed. If no layer is specified (zero length) then the overlay shall not be displayed.  Required if Group 60xx is present in the referenced image(s) or the Presentation State instance containing this Module.	UNSUPPORTED	NA
			- Export not supported		

Table 229: Display Area Module Attributes

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Displayed Area Selection Sequence	(0070,005A)	1	A sequence of Items each of which describes the displayed area selection for a group of images or frames. Sufficient Items shall be present to describe every image and frame listed in the Presentation State Relationship Module.  One or more Items shall be included in this sequence.	ALWAYS	AUTO
>Referenced Image Sequence	(0008,1140)	1C	The subset of images and frames listed in the Presentation State Relationship Module, to which this displayed area selection applies.  One or more Items shall be included in this sequence.  Required if the displayed area selection in this Item does not apply to all the images and frames listed in the Presentation State	ANAP	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			Relationship Module.		
>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	ALWAYS	ORIGINAL
>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	ALWAYS	ORIGINAL
>> Referenced Frame Number	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1.  Note: This Attribute may be multi-valued.  Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	ANAP	AUTO
>> Referenced Segment Number	(0062,000B)	1C	Identifies the Segment Number to which the reference applies.  Required if the Referenced SOP Instance is a Segmentation or Surface Segmentation and the reference does not apply to all segments and Referenced Frame Number (0008,1160) is not present.  <b>- Export not supported</b>	UNSUPPORTED	NA
>Pixel Origin Interpretation	(0048,0301)	1C	For a referenced multi-frame image, specifies whether the Displayed Area Top Left Hand Corner (0070,0052) and Displayed Area Bottom Right Hand Corner (0070,0053) are to be interpreted relative to the individual frame pixel origins, or relative to the Total Pixel Matrix origin (see C.8.12.4.1.4).  Required if the value of Referenced SOP Class UID (0008,1150) within Referenced Image Sequence (0008,1140) is 1.2.840.10008.5.1.4.1.1.77.1.6 (VL Whole Slide Microscopy Image). May be present otherwise.  Enumerated Values: FRAME – relative to individual frame VOLUME – relative to Total Image Matrix If not present, TLHC and	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			BRHC are defined relative to the frame pixel origins.		
>Displayed Area Top Left Hand Corner	(0070,0052)	1	The top left (after spatial transformation) pixel in the referenced image to be displayed, given as column\row. Column is the horizontal (before spatial transformation) offset (X) and row is the vertical (before spatial transformation) offset (Y) relative to the origin of the pixel data before spatial transformation, which is 1\1. See Figure C.10.4-1.	ALWAYS	AUTO
>Displayed Area Bottom Right Hand Corner	(0070,0053)	1	The bottom right (after spatial transformation) pixel in the referenced image to be displayed, given as column\row. Column is the horizontal (before spatial transformation) offset (X) and row is the vertical (before spatial transformation) offset (Y) relative to the origin of the pixel data before spatial transformation, which is 1\1. See Figure C.10.4-1.	ALWAYS	AUTO
>Presentation Size Mode	(0070,0100)	1	Manner of selection of display size. Enumerated Values: SCALE TO FIT TRUE SIZE MAGNIFY	ALWAYS	AUTO
>Presentation Pixel Spacing	(0070,0101)	1C	Physical distance between the center of each pixel in the referenced image (before spatial transformation), specified by a numeric pair - adjacent row spacing (delimiter) adjacent column spacing in mm. See 10.7.1.3 for further explanation of the value order. Notes: 1. This value may be different from Pixel Spacing (0028,0030) or Imager Pixel Spacing (0018,1164) specified in the referenced image, which are ignored, since some form of calibration may	ANAP	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			<p>have been performed (for example by reference to an object of known size in the image).</p> <p>2. If the row and column spacing are different, then the pixel aspect ratio of the image is not 1:1.</p> <p>Required if Presentation Size Mode (0070,0100) is TRUE SIZE, in which case the values will correspond to the physical distance between the center of each pixel on the display device.</p> <p>May be present if Presentation Size Mode (0070,0100) is SCALE TO FIT or MAGNIFY, in which case the values are used to compute the aspect ratio of the image pixels.</p>		
>Presentation Pixel Aspect Ratio	(0070,0102)	1C	<p>Ratio of the vertical size and the horizontal size of the pixels in the referenced image, to be used to display the referenced image, specified by a pair of integer values where the first value is the vertical pixel size and the second value is the horizontal pixel size. See C.7.6.3.1.7.</p> <p>Required if Presentation Pixel Spacing (0070,0101) is not present.</p> <p>Notes:</p> <ol style="list-style-type: none"> <li>1. This value may be different from the aspect ratio specified by Pixel Aspect Ratio (0028,0034) in the referenced image, or implied by the values of Pixel Spacing (0028,0030) or Imager Pixel Spacing (0018,1164) specified in the referenced image, which</li> </ol>	ANAP	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			are ignored. 2. This value must be specified even if the aspect ratio is 1:1.		
>Presentation Pixel Magnification Ratio	(0070,0103)	1C	<p>Ratio of displayed pixels to source pixels, specified in one dimension.</p> <p>Required if Presentation Size Mode (0070,0100) is MAGNIFY.</p> <p>Notes:</p> <ol style="list-style-type: none"> <li>1. A value of 1.0 would imply that one pixel in the referenced image would be displayed as one pixel on the display (i.e. it would not be interpolated if the aspect ratio of the image pixels is 1:1).</li> <li>2. A value of 2.0 would imply that one pixel in the referenced image would be displayed as 4 pixels on the display (i.e. up-sampled by a factor of 2 in each of the row and column directions).</li> <li>3. A value of 0.5 would imply that 4 pixels in the referenced image would be displayed as 1 pixel on the display (i.e. down-sampled by a factor of 2 in each of the row and column directions).</li> <li>4. If the source pixels have an aspect ratio of other than 1:1, then they are assumed to have been interpolated to a display pixel aspect ratio of</li> </ol>	SUPPORTED	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			1:1 prior to magnification.		

**Table 230: Graphic Annotation Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Graphic Annotation Sequence	(0070,0001)	1	A sequence of Items each of which represents a group of annotations composed of graphics or text or both. One or more Items shall be included in this sequence.	ALWAYS	AUTO
>Referenced Image Sequence	(0008,1140)	1C	The subset of images and frames listed in the Presentation State Relationship Module, to which this graphic annotation applies. One or more Items shall be included in this sequence. Required if graphic annotations in this Item do not apply to all the images and frames listed in the Presentation State Relationship Module.	ANAP	AUTO
>> Referenced Frame Number	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1. Note: This Attribute may be multi-valued. Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	ANAP	AUTO
>Graphic Layer	(0070,0002)	1	- The layers in which graphic and text may be Rendered  <b>- Export not supported</b>	UNSUPPORT ED	NA
>Text Object Sequence	(0070,0008)	1C	- Sequence that describes a text annotation. One or more Items may be present.  - Either one or both of Text Object Sequence (0070,0008) or Graphic Object Sequence (0070,0009) are required .	ANAP	AUTO
>>Bounding Box Annotation Units	(0070,0003)	1C	- Units of measure for the axes of the text bounding box.  <b>- Export not supported</b>	UNSUPPORT ED	NA
>>Anchor Point Annotation Units	(0070,0004)	1C	- Units of measure for the axes of the text anchor point annotation.  Enumerated Values for Anchor Point Annotation Units	ALWAYS	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			<p>(0070,0004) are the same as for Bounding Box Annotation Units (0070,0003).</p> <p>PIXEL = Image relative position specified with sub-pixel resolution such that the origin, which is at the Top Left Hand Corner (TLHC) of the TLHC pixel is 0.0\0.0, the Bottom Right Hand Corner (BRHC) of the TLHC pixel is 1.0\1.0, and the BRHC of the BRHC pixel is Columns\Rows (see figure C.10.5-1). The values must be within the range 0\0 to Columns\Rows.</p> <p>DISPLAY = Fraction of Specified Displayed Area where 0.0\0.0 is the TLHC and 1.0\1.0 is the BRHC. The values must be within the range 0.0 to 1.0.</p> <p>MATRIX = Image relative position specified with sub-pixel resolution such that the origin, which is at the Top Left Hand Corner (TLHC) of the TLHC pixel of the Total Pixel Matrix, is 0.0\0.0, the Bottom Right Hand Corner (BRHC) of the TLHC pixel is 1.0\1.0, and the BRHC of the BRHC pixel of the Total Pixel Matrix is Total Pixel Matrix Columns\Total Pixel Matrix Rows (see C.8.12.4.1.3). The values must be within the range 0.0\0.0 to Total Pixel Matrix Columns\Total Pixel Matrix Rows. MATRIX may be used only if the value of Referenced SOP Class UID (0008,1150) within Referenced Image Sequence (0008,1140) is 1.2.840.10008.5.1.4.1.1.77.1.6 (VL Whole Slide Microscopy Image).</p> <p>- Required if Anchor Point (0070,0014) is present.</p>		
>>Unformatted Text Value	(0070,0006)	1	<p>- Text data which is unformatted and whose manner of display within the defined bounding box or relative to the specified anchor point is implementation dependent.</p> <p>The text value may contain spaces, as well as multiple lines separated by either LF, CR, CR LF or LF CR, but otherwise no format control characters (such as horizontal or vertical tab and</p>	ALWAYS	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			form feed) shall be present, even if permitted by the Value Representation of ST.  - In HMI, Text is interpreted as ISO-IR 100		
>>Bounding Box Top Left Hand Corner	(0070,0010)	1C	- Location of the Top Left Hand Corner (TLHC) of the bounding box in which Unformatted Text Value (0070,0006) is to be displayed, in Bounding Box Annotation Units (0070,0003), given as column\row. Column is the horizontal offset and row is the vertical offset.  - Required if Anchor Point (0070,0014) is not present.  <b>- Export not supported</b>	UNSUPPORTED	NA
>>Bounding Box Bottom Right Hand Corner	(0070,0011)	1C	- Location of the Bottom Right Hand Corner (BRHC) of the bounding box in which Unformatted Text Value (0070,0006) is to be displayed, in Bounding Box Annotation Units (0070,0003), given as column\row. Column is the horizontal offset and row is the vertical offset.  - Required if Anchor Point (0070,0014) is not present.  <b>- Export not supported</b>	UNSUPPORTED	NA
>>Bounding Box Text Horizontal Justification	(0070,0012)	1C	- Location of the text relative to the vertical edges of the bounding box. Enumerated Values:  LEFT = closest to left edge RIGHT = closest to right edge CENTER = centered  - Required if Bounding Box Top Left Hand Corner (0070,0010) is present.  <b>- Export not supported</b>	UNSUPPORTED	NA
>>Anchor Point	(0070,0014)	1C	- Location of a point in the image or Specified Displayed Area to which the Unformatted Text Value (0070,0006) is related, in Anchor Point Annotation Units (0070,0004), given as column\row. Column is the horizontal offset and row is the vertical offset.  - Required if Bounding Box Top	ALWAYS	AUTO



Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			Left Hand Corner (0070,0010) and Bounding Box Bottom Right Hand Corner (0070,0011) are not present. May be present even if a bounding box is specified (i.e. Bounding Box Top Left Hand Corner (0070,0010) and Bounding Box Bottom Right Hand Corner (0070,0011) are present).		
>>Anchor Point Visibility	(0070,0015)	1C	<p>- Flag to indicate whether or not a visible indication (such as a line or arrow) of the relationship between the text and the anchor point is to be displayed.</p> <p>Enumerated Values:</p> <p>Y = yes N = no</p> <p>- Required if Anchor Point (0070,0014) is present.</p> <p>HMI does not interpret this tag. An arrow is always present to indicate the relationship between the text and the anchor point.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
>Graphic Object Sequence	(0070,0009)	1C	<p>- Sequence that describes a graphic annotation. One or more items may be present.</p> <p>- Either one or both of Text Object Sequence (0070,0008) or Graphic Object Sequence (0070,0009) are required.</p>	ANAP	AUTO
>>Graphic Annotation Units	(0070,0005)	1C	<p>- Units of measure for the axes of the graphic annotation.</p> <p>Enumerated Values for Graphic Annotation Units (0070,0005) are the same as for Bounding Box Annotation Units (0070,0003).</p>	ALWAYS	AUTO
>>Graphic Dimensions	(0070,0020)	1	<p>Enumerated Value: 2</p> <p>McKesson Radiology exports a default Dimensions with a value of 2.</p> <p><b>- Export supported</b></p>	ALWAYS	D
>>Number of Graphic Points	(0070,0021)	1	- Number of data points in this graphic.	ALWAYS	AUTO
>> Graphic Data	(0070,0022)	1	- Coordinates that specify this graphic annotation. Depending on Graphic Type (0070,0023)	ALWAYS	AUTO
>>Graphic Type	(0070,0023)	1	<p>The shape of graphic that is to be drawn.</p> <p>McKesson Radiology supports</p>	ALWAYS	AUTO

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			the following graphic types:  POINT POLYLINE INTERPOLATED CIRCLE ELLIPSE		
>>Graphic Filled	(0070,0024)	1C	<p>- Whether or not the closed graphics element is displayed as filled (in some unspecified manner that shall be distinguishable from an outline) or as an outline.</p> <p>Enumerated Values: Y = yes N = no</p> <p>Required if Graphic Data (0070,0022) is “closed”, that is Graphic Type (0070,0023) is CIRCLE or ELLIPSE, or Graphic Type (0070,0023) is POLYLINE or INTERPOLATED and the first data point is the same as the last data point.</p> <p>McKesson Radiology export a default value of “N”</p> <p><b>- Export not supported</b></p>	ALWAYS	D

**Table 231: Spatial Transformation Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Image Rotation	(0070,0042)	1	<p>How far to rotate the image clockwise in degrees, before any Image Horizontal Flip (0070,0041) is applied.</p> <p>Enumerated Values: 0, 90, 180, 270</p> <p>Notes: Negative values are not permitted since the Value Representation is unsigned.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
Image Horizontal Flip	(0070,0041)	1	<p>Whether or not to flip the image horizontally after any Image Rotation has been applied such that the left side of the image becomes</p>	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			<p>the right side.</p> <p>Enumerated Values:</p> <p>Y = yes, N = no</p> <p>Note: No vertical flip is specified since the same result can be achieved by a combination of a 180 degree rotation and a horizontal flip.</p> <p><b>- Export not supported</b></p>		

Table 232: Graphic Layer Module Attributes

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Graphic Layer Sequence	(0070,0060)	1	<p>A sequence of Items each of which represents a single layer in which overlays, curves, graphics or text may be rendered.</p> <p>One or more Items shall be included in this sequence.</p> <p>An Item is required for each layer referenced from the Graphic Annotation Module or the Overlay Activation Module.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
>Graphic Layer	(0070,0002)	1	<p>A string which identifies the layer.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
>Graphic Layer Order	(0070,0062)	1	<p>An integer indicating the order in which it is recommended that the layer be rendered, if the display is capable of distinguishing. Lower numbered layers are to be rendered first.</p> <p><b>- Export not supported</b></p>	UNSUPPORTED	NA
>Graphic Layer Recommended Display Grayscale Value	(0070,0066)	3	<p>A default single gray unsigned value in which it is recommended that the layer be rendered on a monochrome display. The units are specified in P-Values from a minimum of 0000H (black) up to a maximum of FFFFH (white).</p> <p>Note: The maximum P-Value for this Attribute may be different from the</p>	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			maximum P-Value from the output of the Presentation LUT, which may be less than 16 bits in depth.		
>Graphic Layer Recommended Display CIELab Value	(0070,0401)	3	A default color triplet value in which it is recommended that the layer be rendered on a color display. The units are specified in PCS-Values, and the value is encoded as CIELab. See C.10.7.1.1.  <b>- Export not supported</b>	UNSUPPORTED	NA
>Graphic Layer Description	(0070,0068)	3	A free text description of the contents of this layer.  <b>- Export not supported</b>	UNSUPPORTED	NA

**Table 233: Graphic Group Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Graphic Group Sequence	(0070,0234)	1	Sequence that describes the combined graphic object. One or more Items shall be included in this sequence.  <b>- Export not supported</b>	UNSUPPORTED	NA
>Graphic Group ID	(0070,0295)	1	A unique number identifying the Graphic Group, i.e. the combined graphic object.  <b>- Export not supported</b>	UNSUPPORTED	NA
>Graphic Group Label	(0070,0207)	1	Name used to identify the Graphic Group, i.e. the combined graphic object.  <b>- Export not supported</b>	UNSUPPORTED	NA
>Graphic Group Description	(0070,0208)	3	Description of the group <b>- Export not supported.</b>	UNSUPPORTED	NA

**Table 234: Modality LUT Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality LUT Sequence	(0028,3000)	1C	Defines a sequence of Modality LUTs. Only a single Item shall be included in this sequence. Shall not be present if Rescale Intercept (0028,1052) is present.  <b>- Export not supported</b>	UNSUPPORTED	NA
>LUT Descriptor	(0028,3002)	1C	Specifies the format of the LUT Data in this Sequence. See C.11.1.1 for further explanation. Required if the Modality LUT Sequence (0028,3000) is sent.  <b>- Export not supported</b>	UNSUPPORTED	NA
>LUT Explanation	(0028,3003)	3	Free form text explanation of the meaning of the LUT.	UNSUPPORTED	NA
>Modality LUT Type	(0028,3004)	1C	Specifies the output values of this Modality LUT. See C.11.1.1.2 for further explanation. Required if the Modality LUT Sequence (0028,3000) is sent.  <b>- Export not supported</b>	UNSUPPORTED	NA
>LUT Data	(0028,3006)	1C	LUT Data in this Sequence. Required if the Modality LUT Sequence (0028,3000) is sent.  <b>- Export not supported</b>	UNSUPPORTED	NA
Rescale Intercept	(0028,1052)	1C	The value b in relationship between stored values (SV) and the output units specified in Rescale Type (0028,1054). Output units = m*SV + b. Required if Modality LUT Sequence (0028,3000) is not present. Shall not be present otherwise.  <b>- Export not supported</b>	UNSUPPORTED	NA
Rescale Slope	(0028,1053)	1C	m in the equation specified by Rescale Intercept (0028,1052). Required if Rescale Intercept is present.  <b>- Export not supported</b>	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Rescale Type	(0028,1054)	1C	Specifies the output units of Rescale Slope (0028,1053) and Rescale Intercept (0028,1052). See C.11.1.1.2 for further explanation. Required if Rescale Intercept is present.  - Export not supported	UNSUPPORTED	NA

Table 235: Softcopy VOI LUT Module Attributes

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Softcopy VOI LUT Sequence	(0028,3110)	1	Defines a sequence of VOI LUTs or Window Centers and Widths and to which images and frames they apply. No more than one VOI LUT Sequence containing a single Item or one pair of Window Center/Width values shall be specified for each image or frame. One or more Items shall be included in this sequence.	ANAP	AUTO
>Referenced Image Sequence	(0008,1140)	1C	The subset of images and frames listed in the Presentation State Relationship Module, to which this VOI LUT or Window Center and Width applies. One or more Items shall be included in this sequence. Required if the VOI LUT transformation in this Item does not apply to all the images and frames listed in the Presentation State Relationship Module.	ANAP	AUTO
>> Referenced SOP Class UID	(0008,1150)	1	Uniquely identifies the referenced SOP Class.	ALWAYS	AUTO
>> Referenced SOP Instance UID	(0008,1155)	1	Uniquely identifies the referenced SOP Instance.	ALWAYS	AUTO
>> Referenced Frame Number	(0008,1160)	1C	Identifies the frame numbers within the Referenced SOP Instance to which the reference applies. The first frame shall be denoted as frame number 1. Note: This Attribute may be multi-valued. Required if the Referenced SOP Instance is a multi-frame image and the reference does not apply to all frames, and Referenced Segment Number (0062,000B) is not present.	ANAP	AUTO
>> Referenced Segment Number	(0062,000B)	1C	Identifies the Segment Number to which the reference applies. Required if the Referenced SOP Instance is a Segmentation or Surface Segmentation and the reference does not apply to all segments and Referenced Frame Number (0008,1160) is not present.	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			<b>- Export not supported</b>		
> VOI LUT Sequence	(0028,3010)	1C	Defines a sequence of VOI LUTs. One or more Items shall be included in this sequence. Required if Window Center (0028,1050) is not present. May be present otherwise.	ANAP	AUTO
>> LUT Descriptor	(0028,3002)	1	Specifies the format of the LUT Data in this Sequence. See C.11.2.1.1 for further explanation.	ALWAYS	AUTO
>> LUT Explanation	(0028,3003)	3	Free form text explanation of the meaning of the LUT. Export as Linear DICOM VOI LUT.	ANAP	AUTO
>> LUT Data	(0028,3006)	1	LUT Data in this Sequence.	ALWAYS	AUTO
>> Window Center	(0028,1050)	1C	Window Center for display. See C.11.2.1.2 for further explanation. Required if VOI LUT Sequence (0028,3010) is not present. May be present otherwise.  Will be exported as linear VOILUT  <b>- Export not supported</b>	UNSUPPORTED	NA
>> Window Width	(0028,1051)	1C	Window Width for display. See C.11.2.1.2 for further explanation. Required if Window Center (0028,1050) is sent.  Will be exported as linear VOILUT  <b>- Export not supported</b>	UNSUPPORTED	NA
>> Window Center & Width Explanation	(0028,1055)	3	Free form explanation of the meaning of the Window Center and Width. Multiple values correspond to multiple Window Center and Width values.  <b>- Export not supported</b>	UNSUPPORTED	NA

**Table 236: Softcopy Presentation LUT Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Presentation LUT Sequence	(2050,0010)	1C	Defines a sequence of Presentation LUTs. Only a single item shall be included in this sequence. Required if Presentation LUT Shape (2050,0020) is absent.  <b>- Export not supported</b>	UNSUPPORTED	NA
>LUT Descriptor	(0028,3002)	1	Specifies the format of the LUT Data in this Sequence. See C.11.6.1.1 for further explanation.  <b>- Export not supported</b>	UNSUPPORTED	NA

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
>LUT Explanation	(0028,3003)	3	Free form text explanation of the meaning of the LUT.  - Export not supported	UNSUPPORTED	NA
>LUT Data	(0028,3006)	1	LUT Data in this Sequence.  - Export not supported	UNSUPPORTED	NA
Presentation LUT Shape	(2050,0020)	1C	Specifies predefined Presentation LUT transformation. Required if Presentation LUT Sequence (2050,0010) is absent. Enumerated Values: IDENTITY - no further translation necessary, input values are P-Values INVERSE - output values after inversion are P-Values See C.11.6.1.2  Export default value <b>IDENTITY</b>	ALWAYS	D

**Table 237: SOP Common Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
SOP Class UID	(0008,0016)	1	1.2.840.10008.5.1.4.1.1.11.1 (PR)	ALWAYS	D
SOP Instance UID	(0008,0018)	1	Generated UID. Reuse existing UID if there is one already generated for the annotation file in the study.	ALWAYS	AUTO

**Table 238: McKesson Private Attributes in GSPS Objects**

Tag ID	Attribute Name	VR	VM	Significance
(3711,00xx)	Private Creator ID	LO	1	- The Private Creator ID for this block of added Private Elements. The value is "A.L.I. Technologies, Inc.".
(3711,xxB0)	ALI_SERIALIZED_ANNOTATIONS	OB	1	-Serialized Internal annotations in proprietary format
(3711,xxB1)	ALI_SERIALIZED_GSPS_DATE	DA	1	- Serialization Date
(3711,xxB2)	ALI_SERIALIZED_GSPS_TIME	TM	1	- Serialization Time
(3711,xxB3)	ALI_SERIALIZED_PRESENTATION	OB	1	-Serialized Internal presentation elements in proprietary format

NOTE1: McKesson Radiology™ User created annotations (e.g. distance, ellipse etc.) and presentation elements (zoom, w/l etc.) are serialized in the above private attributes in the GSPS object. This allows the McKesson Radiology application to deserialize our own richer representation than what can be represented by DICOM standard GSPS attributes.



McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 216

## 7.1.10 Raw Data Instance Creation for MC Study Data Files

McKesson Radiology™ 12.2 can create DICOM Raw Data instances from Non-DICOM data files<sup>20</sup> in McKesson Cardiology studies that McKesson Radiology 12.2 has a reference to for SIM<sup>21</sup> customers. This allows the encapsulated files to be DICOM archived to a DICOM archive SCP and Query/Retrieved back from a DICOM archive SCP.

### 7.1.10.1 Raw Data IOD for MC Study Data Files

This section describes the IOD of the Raw Data SOP Instances by describing the Modules that will be used for such objects.

Table 239 specifies the Modules used in the creation of Raw Data SOP Instances for HC Non-DICOM data files in the Study.

**Table 239: IOD of Raw Data SOP Instances**

IE	Module	DICOM Reference (PS3.3)	Value Description Table	Presence of Module
Patient	Patient	C.7.1.1	Table 240	ALWAYS
Study	General Study	C.7.2.1	Table 241	ALWAYS
Series	General Series	C.7.3.1	Table 242	ALWAYS
Equipment	General Equipment	C.7.5.1	Table 243	ALWAYS
Raw Data	Acquisition Context	C.7.6.14	Table 244	VNAP
	Raw Data	C.19.1	Table 245	ALWAYS
	SOP Common	C.12.1	Table 246	ALWAYS

### 7.1.10.2 RAW Data Object Module Attributes for MC Data files

This section provides information on the Elements that are part of each module present in the Raw Data SOP Instances for McKesson Cardiology Non-DICOM data files<sup>20</sup>. For each Element, the Value Description column describes the meaning of the element, whether it must be present in the Raw Data header, and what the source of the value is.

The tables use the following abbreviations:

The abbreviations in the “Presence of Value” column are:

VNAP	Value not always present (attribute is always present but may not have a value).
ANAP	Attribute not always present.
ALWAYS	Attribute always present and has a value.
EMPTY	Attribute always present but has no value.

The abbreviations in the “Source” column are:

ORIGINAL	Value is copied from an original image.
DB	Value is from the McKesson Radiology™ system database.
AUTO	Value is automatically generated by the McKesson Radiology™ system.
D	indicates a default hard-coded value is set.

<sup>20</sup> Some examples of Non-DICOM file types that SIM needs to wrap as DICOM Raw Data instances (.ant, .wav, .txt, .doc, .htm, and jpg, fds etc.).

<sup>21</sup> SIM - Shared Image Management - With SIM, customers will have one PACS system to learn and maintain instead of having a separate PACS system for both Radiology and Cardiology Studies.

**Table 240: Patient Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Patient's Name	(0010,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient ID	(0010,0020)	2	Copied from database.	ALWAYS	DB
Patient's Birth Date	(0010,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient's Sex	(0010,0040)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB

**Table 241: General Study Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Study Instance UID	(0020,000D)	1	Copied from database.	ALWAYS	DB
Study Date	(0008,0020)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Time	(0008,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Referring Physician's Name	(0008,0090)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study ID	(0020,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Accession Number	(0008,0050)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Description	(0008,1030)	3	Not present OR copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 242: General Series Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	1	Type of equipment that originally acquired the data used to create the images in this Series. Set to appropriate modality etc "OT"	ALWAYS	D

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Series Instance UID	(0020,000E)	1	Generated on SOP Instance Creation.  A single series instance uid will be used for all raw data files in a study when archived.  If a new raw data file is added to a study after it has been archived a new series instance uid will be created when the raw data file is added to the dicom archive.	ALWAYS	AUTO
Series Number	(0020,0011)	2	Set to empty value	ALWAYS	D
Series Description	(0008,103e)	3	Copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 243: General Equipment Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Manufacturer	(0008,0070)	2	Value specified as "McKesson Medical Imaging Group"	ALWAYS	AUTO

**Table 244: Acquisition Context Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Acquisition Context Sequence	(0040,0555)	2	A sequence of Items that describes the conditions present during the acquisition of the data of the SOP Instance.  Zero items shall be included in this sequence.	EMPTY	D

**Table 245: Raw Data Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Instance Number	(0020,0013)	2	A number that identifies this raw data. The value shall be unique within a series.  Set to empty value.	ALWAYS	D

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Content Date	(0008,0023)	1	The date the raw data creation was started.  Content Date will use the same date as General Study Module Attributes, Study Date	ALWAYS	AUTO
Content Time	(0008,0033)	1	The time the raw data creation was started.  Content Time will use the same time as General Study Module Attributes, Study time	ALWAYS	AUTO
Creator-Version UID	(0008,9123)	1	Unique identification of the equipment and version of the software that has created the Raw Data information. The UID allows one to avoid attempting to interpret raw data with an unknown format.  Use: 1.2.840.113711.25.<version> so use 1.2.840.113711.25.1	ALWAYS	D
Private attributes that contain Raw Data Information See Table 247: Private Elements Added To Raw Data Object					

Table 246: SOP Common Module Attributes

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
SOP Class UID	(0008,0016)	1	1.2.840.10008.5.1.4.1.1.66	ALWAYS	D
SOP Instance UID	(0008,0018)	1	Generated UID.	ALWAYS	AUTO

Table 247: Private Elements Added To Raw Data Object

Tag ID	Attribute Name	VR	VM	Significance
(3711,00xx)	Private Creator ID	LO	1	- The Private Creator ID for this block of added Private Elements. The value is "A.L.I. Technologies, Inc."
(3711,xxC4)	ALI_SIM_DATA_SEQUENCE	SQ	1	- A sequence of Items each of which represents a section of the McKesson Radiology™ HC proprietary data and size of data blob for Horizon Cardiology Study objects types. - 10 Items shall be included in this sequence.
> (3711,00xx)	Private Creator ID	LO	1	- The Private Creator ID for this block of added Private Elements. The value is "A.L.I. Technologies, Inc."
> (3711,xxC0)	ALI_SIM_DATA_BLOB	OB	1	- Holds the McKesson Radiology™ HC proprietary data for McKesson Cardiology Study objects types20.
> (3711,xxC2)	ALI_SIM_DATA_BLOB_SIZE	UL	1	- Size of the data blob
(3711,xxC1)	ALI_SIM_WRAP_FILE_CREATOR_ID	LO	1	- Unique Identifier to indicate this is a HMI wrapped DICOM file; "HMI SIM"

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 220

Tag ID	Attribute Name	VR	VM	Significance
(3711,xxC3)	ALI_SIM_PRIVATE_MC_STRING	LO	1	- Medcon private Tag string that we store and return to them without modifying
(3711,xx01)	ALI_FILENAME_TAG	LO	1	- Original filename
(3711,xx05)	ALI_BAG_ID_TAG	IS	1	- bag ID that the file belongs to

### 7.1.11 Encapsulated PDF Instance Creation for MC Study PDF Files

McKesson Radiology™ 12.2 can create DICOM encapsulated PDF instances from Non-DICOM .pdf data files in McKesson Cardiology studies that McKesson Radiology™ 12.2 has a reference to for SIM<sup>22</sup> customers. This allows the encapsulated files to be DICOM archived to a DICOM archive SCP and Query/Retrieved back from a DICOM archive SCP.

#### 7.1.11.1 EPDF IOD for MC Study PDF Files

This section describes the IOD of the EPDF SOP Instances by describing the Modules that will be used for such objects.

Table 248 specifies the Modules used in the creation of EPDF SOP Instances for MC .pdf data files in the Study.

**Table 248: IOD of EPDF SOP Instances**

IE	Module	DICOM Reference (PS3.3)	Value Description Table	Presence of Module
Patient	Patient	C.7.1.1	Table 249	ALWAYS
Study	General Study	C.7.2.1	Table 250	ALWAYS
Series	Encapsulated Document Series	C.24.1	Table 251	ALWAYS
Equipment	General Equipment	C.7.5.1	Table 252	ALWAYS
	SC Equipment	C.8.6.1	Table 253	ALWAYS
Raw Data	Encapsulated Document	C.7.6.14	Table 254	ALWAYS
	SOP Common	C.12.1	Table 255	ALWAYS

#### 7.1.11.2 EPDF Object Module Attributes for MC PDF files

This section provides information on the Elements that are part of each module present in the encapsulated PDF SOP Instances for McKesson Cardiology .pdf data files. For each Element, the Value Description column describes the meaning of the element, whether it must be present in the EPDF header, and what the source of the value is.

The tables use the following abbreviations:

The abbreviations in the “Presence of Value” column are:

VNAP	Value not always present (attribute is always present but may not have a value).
ANAP	Attribute not always present.
ALWAYS	Attribute always present and has a value.
EMPTY	Attribute always present but has no value.
NA	Not applicable

The abbreviations in the “Source” column are:

<sup>22</sup> SIM - Shared Image Management - With SIM, customers will have one PACS system to learn and maintain instead of having a separate PACS system for both Radiology and Cardiology Studies.

ORIGINAL	Value is copied from an original image.
DB	Value is from the McKesson Radiology™ system database.
AUTO	Value is automatically generated by the McKesson Radiology™ system.
D	indicates a default hard-coded value is set.
NA	Not applicable

**Table 249: Patient Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Patient's Name	(0010,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient ID	(0010,0020)	2	Copied from database.	ALWAYS	DB
Patient's Birth Date	(0010,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Patient's Sex	(0010,0040)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB

**Table 250: General Study Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Study Instance UID	(0020,000D)	1	Copied from database.	ALWAYS	DB
Study Date	(0008,0020)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Time	(0008,0030)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Referring Physician's Name	(0008,0090)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study ID	(0020,0010)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Accession Number	(0008,0050)	2	Copied from database if a value is specified. Empty otherwise.	VNAP	DB
Study Description	(0008,1030)	3	Not present OR copied from database if a value is specified. Empty otherwise.	ANAP	DB

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 222

**Table 251: Encapsulated Document Series Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	1	The modality appropriate for the encapsulated document. This Type definition shall override the definition in the SC Equipment Module. See section C.7.3.1.1.1 for Defined Terms.  Use "DOC"	ALWAYS	D
Series Instance UID	(0020,000E)	1	Generated on SOP Instance Creation.  A single series instance uid will be used for all PDF files in a bag when a study is archived  If a new PDF file is added to a study after it has been archived a new series instance uid will be created when that PDF file is added to the dicom archive	ALWAYS	AUTO
Series Number	(0020,0011)	2	Series Number will be an empty value	ALWAYS	D
Series Description	(0008,103e)	3	Copied from database if a value is specified. Empty otherwise.	ANAP	DB

**Table 252: General Equipment Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Manufacturer	(0008,0070)	2	Value specified as "McKesson Medical Imaging Group"	ALWAYS	AUTO

**Table 253: SC Equipment Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Modality	(0008,0060)	3	Set to "DOC"	ALWAYS	D
Conversion Type	(0008,0064)	1	Describes the kind of image conversion. Defined Term used:  <b>SI = Scanned Image</b>	ALWAYS	DB

**Table 254: Encapsulated Document Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
Instance Number	(0020,0013)	1	A number that identifies this SOP Instance. The value shall be unique within a series.  Instance Number will be an empty value	ALWAYS	D
Content Date	(0008,0023)	2	The date the document content creation was started.  Content Date will use the same date as General Study Module Attributes, Study Date.	ALWAYS	AUTO
Content Time	(0008,0033)	2	The time the document creation was started.  Content Time will use the same time as General Study Module Attributes, Study time.	ALWAYS	AUTO
Acquisition DateTime	(0008,002A)	2	The date and time that the original generation of the data in the document started.	EMPTY	D
Burned In Annotation	(0028,0301)	1	Indicates whether or not the encapsulated document contains sufficient burned in annotation to identify the patient and date the data was acquired. Enumerated Values: YES NO  Identification of patient and date as text in an encapsulated document (e.g., in an XML attribute or element) is equivalent to "burned in annotation". A de-identified document may use the value NO.  Burned In Annotation. We will use "YES".  Our understanding is that the PDF files will contain reports so we expect them to include enough information to identify the patient. If this understanding is incorrect and some PDF files contain patient information and some do not contain patient information, since we have no way of determining which is which it is safest to use "YES" for all PDF files.	ALWAYS	D
Source Instance Sequence	(0042,0013)	1C	A sequence that identifies the	NA	NA



Attribute Name	Tag	Type	Value Description	Presence of Value	Source
			set of Instances that were used to derive the encapsulated document.		
Document Title	(0042,0010)	2	The title of the document.	VNAP	ORIGINAL
Verification Flag	(0040,A493)	3	Indicates whether the Encapsulated Document is Verified. Enumerated Values: UNVERIFIED = Not attested by a legally accountable person. VERIFIED = Attested to (signed) by a Verifying Observer or Legal Authenticator named in the document, who is accountable for its content.	NA	NA
HL7 Instance Identifier	(0040,E001)	1C	Instance Identifier of the encapsulated HL7 Structured Document, encoded as a UID (OID or UUID), concatenated with a caret ("^") and Extension value (if Extension is present in Instance Identifier). Required if encapsulated document is a CDA document.	NA	NA
MIME Type of Encapsulated Document	(0042,0012)	1	The type of the encapsulated document stream described using the MIME Media Type (see RFC 2046).  Set to "application/pdf"	ALWAYS	D
List of MIME Types	(0042,0014)	1C	MIME Types of subcomponents of the encapsulated document. Required if the encapsulated document incorporates subcomponents with MIME types different than the primary MIME Type of the encapsulated document. Note: An Encapsulated CDA that includes an embedded JPEG image and an embedded PDF would list "image/jpeg\application/pdf".	NA	NA
Encapsulated Document	(0042,0011)	1	Encapsulated Document stream, containing a document encoded according to the MIME Type.  - Contains the pdf data	ALWAYS	ORIGINAL

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 225

**Table 255: SOP Common Module Attributes**

Attribute Name	Tag	Type	Value Description	Presence of Value	Source
SOP Class UID	(0008,0016)	1	1.2.840.10008.5.1.4.1.1.104.1	ALWAYS	D
SOP Instance UID	(0008,0018)	1	Generated UID.	ALWAYS	AUTO

**Table 256: Private Elements Added To PDF Data Object**

Tag ID	Attribute Name	VR	VM	Significance
(3711,00xx)	Private Creator ID	LO	1	- The Private Creator ID for this block of added Private Elements. The value is "A.L.I. Technologies, Inc.".
(3711,xxC1)	ALI_SIM_WRAP_FILE_CREATOR_ID	LO	1	- Unique Identifier to indicate this is a HMI wrapped DICOM file; "HMI SIM"
(3711,xxC2)	ALI_SIM_DATA_BLOB_SIZE	UL	1	- Size of the pdf file blob
(3711,xxC3)	ALI_SIM_PRIVATE_MC_STRING	LO	1	- Medcon private Tag string that we store and return to them without modifying
(3711,xx01)	ALI_FILENAME_TAG	LO	1	- Original filename
(3711,xx05)	ALI_BAG_ID_TAG	IS	1	- bag ID that the file belongs to

### 7.1.12 Significant Elements in Received Mammography CAD SR

McKesson Radiology™ 12.2 supports displaying information about CAD findings encoded in R2 and iCAD DICOM Mammography SR objects. This information can be graphical marks on related Digital Mammography images or textual information (e.g. Algorithm Name, Algorithm Version, and Number of Calcifications) about the findings. The types of CAD findings supported for display includes Density mass, Calcification Cluster and Mass with Calcifications. CAD Processing status indicates whether the CAD detection algorithms succeeded and if there are any findings is also supported for display. McKesson Radiology™ 12.2 can display the Mammography Breast Density data such as Volume of fibroglandular tissue, Volume of Breast, and percentage of fibroglandular tissue encoded in R2, iCAD, VuCOMP and Volpara DICOM Mammography SR objects. In addition, McKesson Radiology™ 12.2 can also display a BI-RADS Breast Density Score to categorize the breast as almost entirely fat, having scattered fibroglandular tissue, being heterogeneously dense, or as extremely dense. Support for CAD SR is available only for Digital Mammography images and other types of CAD SR, such as CAD SR for Chest X-Rays, are not supported.

Table 257 lists the templates and their content items in the Mammography CAD SR instances that are supported by McKesson Radiology™ 12.2.

**Table 257: Supported Content Items in Mammography CAD SR Instances**

Template	Rows	Expected Value
TID 4000, Mammography CAD Document Root	1,3,4,5,6,8	See Table 258 TID 4000
TID 4001, Mammography CAD Overall Impression/Recommendation	1,2,3	See Table 259 TID 4001
TID 4003, Mammography CAD Individual Impression/Recommendation	1,2,3,4,5	See Table 261 TID 4003
TID 4004, Mammography CAD Composite Feature	1,2,5,6	See Table 262 TID 4004

Template	Rows	Expected Value
TID 4005 Mammography CAD Composite Feature Body	1,2	See Table 263 TID 4005
TID 4006, Mammography CAD Single Image Finding	1,2,5,6,7,8,12-14	See Table 264 TID 4006
TID 4007 Mammography CAD Breast Composition Template	1,2	See Table 265 TID 4007
TID 4015, CAD Detections Performed	1	See Table 266 TID 4015
TID 4016, CAD Analyses Performed	1	See Table 267 TID 4016
TID 4020, CAD Image Library Entry	1	See Table 268 TID 4020
TID 4021, Mammography CAD Geometry	1-4	See Table 269 TID 4021
Volpara Private Elements for Volpara BI-RADS Density Score	1-2	See Table 270

**Table 258 TID 4000 Mammography CAD Document Root**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CONTAINER	EV(111036, DCM, "Mammography CAD Report")	1	M			<b>Supported</b>
2	>	HAS CONCEPT MOD	INCLUDE	DTID (1204) Language of Content Item and Descendants	1	M			<b>Not Supported</b> Hard code for English.
3	>	CONTAINS	CONTAINER	EV(111028, DCM, "Image Library")	1	M			<b>Supported</b>
4	>>	CONTAINS	INCLUDE	DTID (4020) CAD Image Library Entry	1-n	M		\$ImageLaterality = DCID (6022) Side, \$ImageView = DCID (4014) View for Mammography, \$ImageViewModifier = DCID (4015) View Modifier for Mammography	<b>Supported</b> Support the Referenced SOP Sequence containing the Referenced SOP Class UID and Referenced SOP Instance UID for display.  Other observations related to the image are parsed but not used for display.  E.g. Image Laterality, Patient Orientation.
5	>	CONTAINS	INCLUDE	DTID (4001) Mammography CAD Overall Impression / Recommendation	1	M			<b>Supported</b>
6	>	CONTAINS	CODE	EV(111064, DCM, "Summary of Detections")	1	M		DCID (6042) Status of Results	<b>Supported</b>

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
7	>>	INFERRED FROM	INCLUDE	DTID (4015) CAD Detections Performed	1	MC	Shall be present unless the value of (111064, DCM, "Summary of Detections") is (111225, DCM, "Not Attempted")	\$DetectionCode = DCID (6014) Mammography Single Image Finding	<b>Not Supported</b>  McKesson Radiology 12.2 does not use this information.
8	>	CONTAINS	CODE	EV(111065, DCM, "Summary of Analyses")	1	M		DCID (6042) "Status of Results"	<b>Supported</b>
9	>>	INFERRED FROM	INCLUDE	DTID (4016) CAD Analyses Performed	1	MC	Shall be present unless the value of (111065, DCM, "Summary of Analyses") is (111225, DCM, "Not Attempted")	\$AnalysisCode = DCID (6043) Types of Mammography CAD Analysis	<b>Not Supported</b>  McKesson Radiology 12.2 does not use this information

**Table 259 TID 4001 Mammography CAD Overall Impression/Recommendation**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CODE	EV (111017, DCM, "CAD Processing and Findings Summary")	1	M		DCID (6047) CAD Processing and Findings Summary	<b>Supported</b>
2	>	HAS PROPERTIES	INCLUDE	DTID (4002) Mammography CAD Impression/Recommendation Body"	1	U			<b>Supported</b>  Only for McKesson Radiology 12.2, rows 12-13 of TID 4002
3	>	INFERRED FROM	INCLUDE	DTID (4003) Mammography CAD Individual Impression/Recommendation	1-n	MC	Shall be present if 1 or more (111059, DCM, "Single Image Finding") or (111015, DCM, "Composite Feature") content items are reported.		<b>Supported</b>

**Table 260 TID 4002 Mammography CAD Impression/Recommendation Body**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
12			NUM	DCID (6142) Calculated Value	1-n	U			<b>Supported</b>  Some breast density measurements from R2 uses their own 99R2TECH coding scheme.  <b>iCAD and Volpara, VuCOMP</b>  - 112191, DCM, 'Breast tissue density

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
								<ul style="list-style-type: none"> <li>- 112192, DCM, 'Volume of parenchymal tissue'</li> <li>- 112193, DCM, 'Volume of breast'</li> </ul> <p><b>R2 5.x:</b></p> <ul style="list-style-type: none"> <li>- 112193, DCM, 'Volume of breast'</li> <li>- R2cn015, 99R2TECH, 'Volume of fibroglandular tissue = 112192, DCM, 'Volume of parenchymal tissue'</li> <li>- R2cn016, 99R2TECH, 'Percentage of fibroglandular tissue') = 112191, DCM, 'Breast tissue density'</li> </ul> <p><b>R2 Quantra:</b></p> <ul style="list-style-type: none"> <li>- R2cn018, 99R2TECH, 'VFG Volume of fibroglandular tissue = 112192, DCM, 'Volume of parenchymal tissue'</li> <li>- R2cn019, 99R2TECH, 'Vbd: Volumetric breast density tissue') = 112191, DCM, 'Breast tissue density'</li> <li>- R2cn020, 99R2TECH, 'Vbd: Volumetric breast density tissue') = 112193, DCM, 'Volume of breast'</li> <li>- R2cn027, 99R2TECH, 'Q_abd: Quartile area breast density (integral)')</li> </ul>	
13	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT, "Laterality")	1	U		DCID (6022) Side	

**Table 261 TID 4003 Mammography CAD Individual Impression/Recommendation**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	
1			CONTAINER	EV (111034, DCM, "Individual Impression/Recommendation")	1	M			<b>Supported</b>
2	>	HAS CONCEPT MOD	CODE	EV (111056, DCM, "Rendering Intent")	1	M		DCID (6034) Intended Use of CAD Output	<b>Supported</b>  Only display as tooltips information about CAD marks not interpreted for intended use of CAD Output.
3	>	CONTAINS	INCLUDE	DTID (4002) Mammography CAD Impression / Recommendation Body	1	U			<b>Not Supported</b>
4	>	CONTAINS	INCLUDE	DTID (4004) Mammography CAD Composite Feature	1-n	MC	At least one of rows 4, 5 shall be present.		<b>Supported</b>
5	>	CONTAINS	INCLUDE	DTID (4006) Mammography CAD Single Image Finding	1-n	MC	At least one of rows 4, 5 shall be present.		<b>Supported</b>

**Table 262 TID 4004 Mammography CAD Composite Feature**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CODE	EV (111015, DCM, "Composite Feature")	1	M		DCID (6016) Mammography Composite Feature	<b>Supported</b>  Only (DCM 111459 Mass with calcifications)
2	>	HAS CONCEPT MOD	CODE	EV (111056, DCM, "Rendering Intent")	1	M		DCID (6034) Intended Use of CAD Output	<b>Supported</b>  Only display as tooltips information about CAD marks. Not interpreted for intended use of CAD Output
3	>	HAS OBS CONTEXT	INCLUDE	DTID (4108) Tracking Identifier	1	U			<b>Not Supported</b>
4	>	HAS PROPERTIES	INCLUDE	DTID (4005) Mammography CAD Composite Feature Body	1	M			<b>Supported</b>  McKesson can display the Marks that are spatially related and on only one of the images from R2
5	>	INFERRED FROM	INCLUDE	DTID (4004) Mammography CAD Composite Feature	1-n	MC	At least two items shall be present: two of row 5, two of row 6, or one of each.		<b>Not Supported</b>
6	>	INFERRED FROM	INCLUDE	DTID (4006) Mammography CAD Single Image Finding	1-n	MC	At least two items shall be present: two of		<b>Supported</b>

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
							row 5, two of row 6, or one of each.		
7	>	HAS OBS CONTEXT	INCLUDE	DTID (4022) CAD Observation Context	1	MC	Shall be present only if this feature is incorporated from a different report than its parent.		<b>Not Supported</b>

**Table 263 TID 4005 Mammography CAD Composite Feature Body**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CODE	EV (111016, DCM, "Composite type")	1	M		DCID (6035) Composite Feature Relations. The value shall be (111154, DCM, "Target content items are related spatially")	<b>Supported</b>  From R2:  (111154, DCM, 'Target content items are related spatially')
2			CODE	EV (111057, DCM, "Scope of Feature")	1	M		DCID (6036) Scope of Feature	<b>Supported</b>  From R2:  (111157, DCM, 'Feature detected on only one of the images')

**Table 264 TID 4006 Mammography CAD Single Image Finding**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CODE	EV (111059, DCM, "Single Image Finding")	1	M		DCID (6014) Mammography Single Image Finding	<b>Supported</b>  SRT F-01796 Mammographic breast density  SRT F-01776 Individual Calcification  SRT F-01775 Calcification Cluster
2	>	HAS CONCEPT MOD	CODE	EV (111056, DCM, "Rendering Intent")	1	M		DCID (6034) Intended Use of CAD Output	<b>Supported</b>  Only display as tooltips information about

## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is  
effective as of the last approval  
date

Page 231

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
									CAD marks. Not interpreted for intended use of CAD Output.
3	>>	HAS PROPERTIES	NUM	EV (111071, DCM, "CAD Operating Point")	1	UC	IFF value of row 2 is (111151, DCM, "Presentation Optional") and row 9 of TID 4017 is present	UNITS = DT ({1:n}, UCUM, "range: 1:n"), where n is the maximum specified in Row 9 of TID 4017. Value is restricted to being an integer	<b>Not Supported</b>
4	>	HAS OBS CONTEXT	INCLUDE	DTID (4108) Tracking Identifier	1	U			<b>Not Support</b>
5	>	HAS PROPERTIES	INCLUDE	DTID (4019) CAD Algorithm Identification	1	M			<b>Supported</b>  Display as tooltips information about CAD marks
6	>	HAS PROPERTIES	NUM	EV(111012, DCM, "Certainty of Finding")	1	U		UNITS = EV(%, UCUM, "Percent") Value = 0 – 100	<b>Supported</b>  Display as tooltips information about CAD marks if available
7	>	HAS PROPERTIES	NUM	EV (111047, DCM, "Probability of cancer")	1	UC	May be present unless value of parent is (F-01710,SRT, "Breast composition"), (111100, DCM, "Breast geometry"), (T-04100, SRT, "Nipple"), (111099, DCM, "Selected region"), (111101, DCM, "Image quality") or (111102, DCM, "Non-lesion")	UNITS = EV(%, UCUM, "Percent") Value = 0 – 100	<b>Not Supported</b>
8	>	HAS PROPERTIES	INCLUDE	DTID (4021) Mammography CAD Geometry	1	MC	Shall be present unless value of parent is (F-01710,SRT, "Breast composition"), (111100, DCM, "Breast geometry") or (111101, DCM, "Image quality")		<b>Supported</b>  Rows 1-4 of DTID (4021)
9	>	HAS PROPERTIES	INCLUDE	DTID (4007) Mammography CAD Breast Composition	1	MC	Shall be present only if value of parent is (F-01710,SRT, "Breast composition")		<b>Support</b>
10	>	R-INFERRED FROM	CODE		1-n	UC	May be present only if value of parent is (F-01710,SRT, "Breast composition")	Shall reference a (111059, DCM, "Single Image Finding") of value: EV (111100, DCM, "Breast geometry")	<b>Not Supported</b>



## McKesson Radiology™ 12.2 – DICOM Conformance Statement

Document ID: 2015-30991

Rev #1.0

Released This document is effective as of the last approval date

Page 232

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
11	>	HAS PROPERTIES	INCLUDE	DTID (4008) Mammography CAD Breast Geometry	1	MC	Shall be present only if value of parent is (11100, DCM, "Breast geometry")		Not Supported
12	>	HAS PROPERTIES	INCLUDE	DTID (4009) Mammography CAD Individual Calcification	1	UC	May be present only if value of parent is (F-01776, SRT, "Individual Calcification")		Supported
13	>	HAS PROPERTIES	INCLUDE	DTID (4010) Mammography CAD Calcification Cluster	1	UC	May be present only if value of parent is (F-01775, SRT, "Calcification Cluster")		Supported
14	>	HAS PROPERTIES	INCLUDE	DTID (4011) Mammography CAD Density	1	UC	May be present only if value of parent is (F-01796, SRT, "Mammography breast density")		Supported
15	>	HAS PROPERTIES	CODE	EV (111297, DCM, "Nipple Characteristic")	1	UC	May be present only if value of parent is (T-04100, SRT, "Nipple")	DCID (6039) Nipple Characteristic	Not Supported
16	>	HAS PROPERTIES	INCLUDE	DTID (4012) Mammography CAD Non-Lesion	1	MC	Shall be present only if value of parent is (11102, DCM, "Non-lesion")		Not Supported
17	>	HAS PROPERTIES	INCLUDE	DTID (4013) Mammography CAD Selected Region	1	MC	Shall be present only if value of parent is (111099, DCM, "Selected Region")		Not Supported
18	>	R-INFERRED FROM	IMAGE		1	MC	IF value of parent is (11101, DCM, "Image quality") and IFF row 19 is not present	Shall reference an IMAGE content item in the (111028, DCM, "Image Library")	Not Supported
19	>	HAS PROPERTIES	SCoord	EV (111030, DCM, "Image Region")	1-n	MC	IF value of parent is (11101, DCM, "Image quality") and IFF row 18 is not present		Not Supported
20	>>	R-SELECTED FROM	IMAGE		1	M		All the (111030, DCM, "Image Region") content items in a single invocation of this template shall reference the same IMAGE content item in the (111028, DCM, "Image Library")	Not Supported
21	>	HAS PROPERTIES	INCLUDE	DTID (4014) CAD Image Quality	1-n	MC	Shall be present only if value of parent is (11101, DCM, "Image quality")	\$QualityFinding = DCID (6041) "Mammography Image Quality Finding", \$QualityStandard = DCID (6045) "Mammography Types of Quality Control Standard"	Not Supported

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
22	>	HAS PROPERTIES	NUM	DCID (6142) Calculated Value	1-n	U			Not Supported
23	>>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")	1	M		DCID (6140) Calculation Methods	Not Supported
24	>>	INFERRED FROM	TEXT	EV (112034, DCM, "Calculation Description")	1	U			Not Supported
25	>	INFERRED FROM	INCLUDE	DTID (4006) Mammography CAD Single Image Finding	1-n	UC	May be present only if value of parent is (F-01775,SRT, "Calcification Cluster")	EV (F-01776,SRT, "Individual Calcification")	Supported
26	>	HAS OBS CONTEXT	INCLUDE	DTID (4022) CAD Observation Context	1	MC	Shall be present only if this finding is incorporated from a different report than its parent.		Not Supported

Table 265 TID 4007 Mammography CAD Breast Composition Template

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CODE	EV (F-01710,SRT, "Breast composition")	1	MC	At least one of row 1 or 2 shall be present	DCID (6000) Overall Breast Composition	Supported  For R2, iCAD and VuCOMP  For Volpara, the vendor will send the BI-RADS Grade in private attribute in Table 270
2			NUM	EV (111046, DCM, "Percent Fibroglandular Tissue")	1	MC	At least one of row 1 or 2 shall be present	UNITS = EV (%), UCUM, "Percent") Value = 0 – 100	Supported

Table 266 TID 4015 CAD Detections Performed

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CONTAINER	EV(111063, DCM, "Successful Detections")	1	MC	Shall be present only if value of parent is (111222, DCM, "Succeeded") or (111223, DCM, "Partially Succeeded")		Supported
2	>	CONTAINS	INCLUDE	DTID (4017) CAD Detection Performed	1-n	M		\$DetectionCode = \$DetectionCode	Not Supported
3			CONTAINER	EV(111025, DCM, "Failed Detections")	1	MC	Shall be present only if value of parent is (111224, DCM, "Failed") or (111223, DCM, "Partially		Not Supported

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
							Succeeded")		
4	>	CONTAINS	INCLUDE	DTID (4017) CAD Detection Performed	1-n	M		\$DetectionCode = \$DetectionCode	<b>Not Supported</b>

**Table 267 TID 4016 CAD Analyses Performed**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			CONTAINER	EV(111062, DCM, "Successful Analyses")	1	MC	Shall be present only if value of parent is (111222, DCM, "Succeeded") or (111223, DCM, "Partially Succeeded")		<b>Supported</b>
2	>	CONTAINS	INCLUDE	DTID (4018) CAD Analysis Performed	1-n	M		\$AnalysisCode=\$AnalysisCode	<b>Not Supported</b>
3			CONTAINER	EV(111024, DCM, "Failed Analyses")	1	MC	Shall be present only if value of parent is (111224, DCM, "Failed") or (111223, DCM, "Partially Succeeded")		<b>Not Supported</b>
4	>	CONTAINS	INCLUDE	DTID (4018) CAD Analysis Performed	1-n	M		\$AnalysisCode=\$AnalysisCode	<b>Not Supported</b>

**Table 268 TID 4020 CAD Image Library Entry**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			IMAGE		1	M			<b>Supported</b>  Used the Referenced SOP Sequence containing the Referenced SOP Class UID and Referenced SOP Instance UID for display.  Other observations related to the image are parsed but not used for display.  E.g. Image Laterality, Patient Orientation.
2	>	HAS ACQ CONTEXT	CODE	EV(111027, DCM, "Image Laterality")	1	MC	Shall be present if (0020,0062) is in the Image Instance	\$ImageLaterality	<b>Not Supported</b>
3	>	HAS ACQ CONTEXT	CODE	EV (111031, DCM, "Image View")	1	MC	Shall be present if (0054,0220) is in the Image Instance	\$ImageView	<b>Not Supported</b>

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
4	>>	HAS CONCEPT MOD	CODE	EV (111032, DCM, "Image View Modifier")	1-n	MC	Shall be present if (0054,0222) is in the Image Instance	\$ImageViewMod	Not Supported
5	>	HAS ACQ CONTEXT	TEXT	EV (111044, DCM, "Patient Orientation Row")	1	MC	Shall be present if (0020,0020) is in the Image Instance		Not Supported
6	>	HAS ACQ CONTEXT	TEXT	EV (111043, DCM, "Patient Orientation Column")	1	MC	Shall be present if (0020,0020) is in the Image Instance		Not Supported
7	>	HAS ACQ CONTEXT	DATE	EV (111060, DCM, "Study Date")	1	MC	Shall be present if (0008,0020) is in the Image Instance		Not Supported
8	>	HAS ACQ CONTEXT	TIME	EV (111061, DCM, "Study Time")	1	MC	Shall be present if (0008,0030) is in the Image Instance		Not Supported
9	>	HAS ACQ CONTEXT	DATE	EV (111018, DCM, "Content Date")	1	MC	Shall be present if (0008,0023) is in the Image Instance		Not Supported
10	>	HAS ACQ CONTEXT	TIME	EV (111019, DCM, "Content Time")	1	MC	Shall be present if (0008,0033) is in the Image Instance		Not Supported
11	>	HAS ACQ CONTEXT	NUM	EV (111026, DCM, "Horizontal Pixel Spacing")	1	MC	Shall be present if (0018,1164) or (0028,0030) is in the Image Instance	UNITS = EV (um, UCUM, "micrometer")	Not Supported
12	>	HAS ACQ CONTEXT	NUM	EV (111066, DCM, "Vertical Pixel Spacing")	1	MC	Shall be present if (0018,1164) or (0028,0030) is in the Image Instance	UNITS = EV (um, UCUM, "micrometer")	Not Supported
13	>	HAS ACQ CONTEXT	NUM	EV (112011, DCM, "Positioner Primary Angle")	1	UC	May be present if (0018,1510) is in the Image Instance		Not Supported
14	>	HAS ACQ CONTEXT	NUM	EV (112012, DCM, "Positioner Secondary Angle")	1	UC	May be present if (0018,1511) is in the Image Instance		Not Supported

Table 269 TID 4021 Mammography CAD Geometry

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
1			SCCOORD	EV(111010, DCM, "Center")	1	M		GRAPHIC TYPE = {POINT}	Supported
2	>	R-SELECTED FROM	IMAGE		1	M		Shall reference an IMAGE content item in the (111028, DCM, "Image Library")	Supported
3			SCCOORD	EV(111041, DCM, "Outline")	1	U			Supported

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint	Usage
4	>	R-SELECTED FROM	IMAGE		1	M		Shall reference the same content item as row 2	Supported
5			SCoord	DCID (6166) CAD Geometry Secondary Graphical Representation	1-n	U			Not Supported
6	>	R-SELECTED FROM	IMAGE		1	M		Shall reference the same content item as row 2	Not Supported

**Table 270: Private Elements for Volpara BI-RADS Density Score**

Tag ID	Attribute Name	VR	VM	Significance	Usage
(0015,0010)	Private Creator ID	LO	1	- The Private Creator ID "MATAKINA_10" for Volpara BI-RADS score".	Supported
(0015,1028)	Volpara Density Grade	LO	1	- BI-RADS score (Volpara Density Grade; VDG) from Volpara automated volumetric breast density assessment system.	Supported

**Table 271: Context ID 6000**

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
Include CID 6001		

**Table 272: Context ID 6001**

From BI-RADS® Third Edition (National Mammography Database, E77)

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
SRT	F-01711	Almost entirely fat
SRT	F-01712	Scattered fibroglandular densities
SRT	F-01713	Heterogeneously dense
SRT	F-01714	Extremely dense

## 8. REVIEWERS

	Rusty Boguslavsky	Director, Software Architecture
	Wilfred Rosenbaum	Senior Project Manager
	Elliot Silver	Standards Analyst
	Howard Fung	Senior Project Manager
	Edwood Yiu	Senior Software Engineer
	Ivy Kwok	Senior Software Engineer
	Glen Scott	Software Development Lead
	Shirley Ma	Senior Software Engineer
	Gary Tsang	Support Product Analyst
	Kyle Batty	Support Representative
	Nina Nesic	Technical Writer
	Indra Lalari	Product Manager
	Nadia Marchant	Quality Assurance Analyst, Quality Assurance & Regulatory Affairs Analyst

McKesson Radiology™ 12.2 – DICOM Conformance Statement			
Document ID: 2015-30991	Rev #1.0	Released This document is effective as of the last approval date	Page 238

## 9. APPROVERS

_____ Rostislav Boguslavsky Director, Software Architecture	_____ Date
_____ Nadia Marchant Quality Assurance Analyst, Quality Assurance & Regulatory Affairs Analyst	_____ Date
_____ Elliot Silver Standards Analyst	_____ Date
_____ Indra Lalari Product Manager	_____ Date



### McKesson Technology Solutions

130-10711 Cambie Road, Richmond, BC Canada V6X 3G5