



# **DICOM Conformance Statement**

## **Change Healthcare Cardiology**

**DICOM Conformance Statement 14.1**

Document ID: DCM-10029  
Revision 3.0 | Release Number 14.1  
Effective Date August 2018

**Rx Only**

## **Copyright and trademarks**

Copyright 2018 Change Healthcare LLC and/or one of its subsidiaries. Change Healthcare and the Change Healthcare logos, are trademarks of Change Healthcare LLC. All other product or company names mentioned may be trademarks, service marks or registered trademarks of their respective companies. All Rights Reserved.

Produced in Cork, Ireland

# 1. Conformance Statement Overview

This document contains DICOM conformance statements for Change Healthcare Cardiology 14.1.

Change Healthcare Cardiology includes a selection of DICOM-related functionality. The customer may choose which functionality is to be installed.

Change Healthcare Cardiology provides the following network services:

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
<b>Transfer</b>		
Computed Radiography Image Storage	Yes	Yes
CT Image Storage	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
Ultrasound Multi-frame Image Storage (Retired)	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Ultrasound Image Storage (Retired)	Yes	Yes
MR Image Storage	Yes	Yes
Enhanced MR Image Storage	Yes	Yes
Secondary Capture Image Storage	Yes	Yes
Multi-Frame Single bit Secondary Capture Image Storage	Yes	Yes
Multi-Frame Grayscale Byte Secondary Capture Image Storage	Yes	Yes
Multi-Frame Grayscale Word Secondary Capture Image Storage	Yes	Yes
Multi-Frame True Color Secondary Capture Image Storage	Yes	Yes
X-Ray Angiographic Image Storage	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	Yes	Yes
X-Ray Bi-Plane Angiographic Image Storage (Retired)	Yes	Yes
Nuclear Medicine Image Storage	Yes	Yes

<b>SOP Classes</b>	<b>User of Service (SCU)</b>	<b>Provider of Service (SCP)</b>
Nuclear Medicine Image Storage (Retired)	Yes	Yes
Grayscale Softcopy Presentation State Storage	Yes	Yes
Positron Emission Tomography Image Storage	Yes	Yes
RT Image	Yes	Yes
Digital X-Ray Image Storage – For Presentation	Yes	Yes
Digital X-Ray Image Storage – For Processing	Yes	Yes
Digital Mammography Image Storage – For Presentation	Yes	Yes
Digital Mammography Image Storage – For Processing	Yes	Yes
Digital Intra-oral X-Ray Image Storage – For Presentation	Yes	Yes
Digital Intra-oral X-Ray Image Storage – For Processing	Yes	Yes
VL Endoscopic Image Storage	Yes	Yes
VL Microscopic Image Storage	Yes	Yes
VL Slide-Coordinates Microscopic Image Storage	Yes	Yes
VL Photographic Image Storage	Yes	Yes
12-lead ECG Waveform Storage	Yes	Yes
General ECG Waveform Storage	Yes	Yes
Ambulatory ECG Waveform Storage	Yes	Yes
Hemodynamic Waveform Storage	Yes	Yes
Cardiac Electrophysiology Waveform Storage	Yes	Yes
Basic Voice Audio Waveform Storage	Yes	Yes
Waveform Storage – Trial (Retired)	Yes	Yes
Intravascular Optical Coherence Tomography Image Storage – for Presentation	Yes	Yes

<b>SOP Classes</b>	<b>User of Service (SCU)</b>	<b>Provider of Service (SCP)</b>
Intravascular Optical Coherence Tomography Image Storage – for Processing	Yes	Yes
Key Object Selection Document Storage	Yes	Yes
Storage Commitment Push Model	Yes	Yes
Basic Text SR Storage	Yes	Yes
Enhanced SR Storage	Yes	Yes
Comprehensive SR Storage	Yes	Yes
Procedure Log Storage	Yes	Yes
Encapsulated PDF Storage	Yes	Yes
Raw Data Storage	No	Yes
<b>Query/Retrieve</b>		
Patient Root Query/Retrieve Info Model – FIND	Yes	Yes
Study Root Query/Retrieve Info Model – FIND	Yes	Yes
Patient Root Query/Retrieve Info Model – MOVE	Yes	Yes
Study Root Query/Retrieve Info Model – MOVE	Yes	Yes
<b>Workflow Management</b>		
Modality Worklist Information Model - FIND	Yes	Yes
Modality Performed Procedure Step	Yes	Yes
<b>Print Management</b>		
Basic Grayscale Print Management Meta	Yes	No
Basic Color Print Management Meta	Yes	No

## 2. Table of Contents

1. Conformance Statement Overview .....	1
2. Table of Contents .....	4
3. Introduction .....	7
3.1 Revision History .....	7
3.2 Audience.....	7
3.3 Remarks.....	7
3.4 Basics of DICOM Communication .....	8
3.5 Abbreviations .....	9
3.6 References.....	10
4. Implementation Model .....	11
4.1 Application Data Flow Diagram .....	12
4.2 Functional Definition of Application Entities.....	18
4.2.1 Functional Definition of Client Application Entity .....	18
4.2.2 Functional Definition of Query/Retrieve Server Application Entity .....	19
4.2.3 Functional Definition of Gateway Application Entity .....	19
4.2.4 Functional Definition of Storage Manager Committer Application Entity.....	19
4.2.5 Functional Definition of Modality Worklist Server Application Entity .....	19
4.2.6 Functional Definiton of MPPS Server Application Entity .....	19
4.2.7 Functional Definition of Sync Storer Application Entity .....	20
4.2.8 Functional Definition of Sync Comitter Application Entity .....	20
4.3 Sequencing of Real-World Activities.....	20
5. AE Specifications.....	21
5.1 Client AE Specification .....	21
5.1.1 SOP Classes .....	21
5.1.2 Association Policies.....	24
5.1.3 Association Initiation Policy .....	24
5.1.4 Association Acceptance Policy .....	34
5.2 Query/Retrieve AE Server Specification.....	34
5.2.1 SOP Classes .....	34
5.2.2 Association Policies.....	37
5.2.3 Association Initiation Policy .....	38
5.2.4 Association Acceptance Policy .....	42

5.3	Gateway AE Specification.....	55
5.3.1	SOP Classes .....	55
5.3.2	Association Policies.....	57
5.3.3	Association Initiation Policy .....	58
5.3.4	Association Acceptance Policy .....	59
5.4	Storage Manager Committer AE Specification .....	65
5.4.1	SOP Classes .....	65
5.4.2	Association Policies.....	65
5.4.3	Association Initiation Policy .....	66
5.4.4	Association Acceptance Policy .....	67
5.5	Modality Worklist Server AE Specification .....	68
5.5.1	SOP Classes .....	68
5.5.2	Association Policies.....	68
5.5.3	Association Initiation Policy .....	69
5.5.4	Association Acceptance Policy .....	69
5.6	MPPS Server AE Specification.....	73
5.6.1	SOP Classes .....	73
5.6.2	Association Policies.....	73
5.6.3	Association Initiation Policy .....	74
5.6.4	Association Acceptance Policy .....	75
5.7	Sync Storer AE Specification.....	81
5.7.1	SOP Classes .....	81
5.7.2	Association Policies.....	84
5.7.3	Association Initiation Policy .....	84
5.7.4	Association Acceptance Policy .....	88
5.8	Sync Committer AE Specification.....	89
5.8.1	SOP Classes .....	89
5.8.2	Association Policies.....	89
5.8.3	Association Initiation Policy .....	90
5.8.4	Association Acceptance Policy .....	91
6.	Communication Profiles.....	93
6.1	TCP/IP Stack.....	93
6.1.1	TCP/IP API .....	93
7.	Extensions/Specializations/Privatization .....	94

8.	Configuration.....	97
9.	Annexes.....	98
9.1	IOD Contents .....	98
9.1.1	Rejection Note Key Object Selection (KOS) Object Contents.....	98
10.	Contact and Support Information.....	101
10.1	Support information .....	101



## 3. Introduction

### 3.1 Revision History

Revision	Revision Date	Summary of Changes
Rev. 1.0	February 2018	Initial release
Rev. 2.0	August 2018	Rebranded for Change Healthcare.
Rev. 3.0	August 2018	Added “Produced in Cork, Ireland”

### 3.2 Audience

This document is intended for people that need to understand how Change Healthcare Cardiology will integrate into their healthcare facility in the aspect of DICOM communication. This includes those responsible for overall imaging network policy and architecture, as well as integrators who require a detailed understanding of the DICOM features. This document contains basic DICOM definitions so that any reader may understand how this product implements DICOM features. However, integrators are expected to fully understand all the DICOM terminology, how the tables in this document relate to the product's functionality, and how that functionality integrates with other devices that support compatible DICOM features.

### 3.3 Remarks

The scope of this DICOM Conformance Statement is to facilitate integration between Change Healthcare Cardiology and other products using the DICOM standard. The Conformance Statement should be read and understood in conjunction with the DICOM Standard. DICOM by itself does not guarantee interoperability. The Conformance Statement does, however, facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of intended information. In fact, the user should be aware of the following important issues:

- The comparison of different Conformance Statements is just the first step towards assessing interconnectivity and interoperability between the product and other DICOM conformant equipment.
- Test procedures should be defined and executed to validate the required level of interoperability.

---

**Note:** The Digital Imaging and Communications in Medicine (DICOM) Standard is constantly evolving. This DICOM Conformance Statement describes Change Healthcare Cardiology's conformance thereto at the time of writing. As the DICOM Standard evolves according to users' request, Change Healthcare modifies its product accordingly. Revised versions of the DICOM Conformance Statement are issued periodically. The currently published version may not reflect all the latest modifications. Please contact Change Healthcare Support for more information. Change Healthcare reserves the right to make changes in its products to comply with evolving DICOM Standards and to update the DICOM Conformance Statement at reasonable intervals.

---

### 3.4 Basics of DICOM Communication

Note: The contents of this section are based on NEMA's [DICOM conformance statement template](#).

This section describes terminology used in this Conformance Statement for the non-specialist. The key terms used in the Conformance Statement are highlighted in *italics* below. This section is not a substitute for training about DICOM, and it makes many simplifications about the meanings of DICOM terms.

Two *Application Entities* (devices) that want to communicate with each other over a network using DICOM protocol must first agree on several things during an initial network "handshake". One of the two devices must initiate an *Association* (a connection to the other device), and ask if specific services, information, and encoding can be supported by the other device (*Negotiation*).

DICOM specifies a number of network services and types of information objects, each of which is called an *Abstract Syntax* for the Negotiation. DICOM also specifies a variety of methods for encoding data, denoted *Transfer Syntaxes*. The Negotiation allows the initiating Application Entity to propose combinations of Abstract Syntax and Transfer Syntax to be used on the Association whose combinations are called *Presentation Contexts*. The receiving Application Entity accepts the Presentation Contexts it supports.

For each Presentation Context, the Association Negotiation also allows the devices to agree on *Roles* - which one is the *Service Class User* (SCU - client) and which is the *Service Class Provider* (SCP - server). Normally the device initiating the connection is the SCU, i.e., the client system calls the server, but not always.

The Association Negotiation finally enables exchange of maximum network packet (*PDU*) size, security information, and network service options (called *Extended Negotiation* information).

The Application Entities, having negotiated the Association parameters, may now commence exchanging data. Common data exchanges include queries for

worklists and lists of stored images, transfer of image objects and analyses (structured reports), and sending images to film printers. Each exchangeable unit of data is formatted by the sender in accordance with the appropriate *Information Object Definition*, and sent using the negotiated Transfer Syntax. There is a Default Transfer Syntax that all systems must accept, but it may not be the most efficient for some use cases. Each transfer is explicitly acknowledged by the receiver with a *Response Status* indicating success, failure, or that query or retrieve operations are still in process.

### 3.5 Abbreviations

AE	Application Entity
CT	Computed Tomography
DICOM	Digital Imaging and Communications in Medicine
IHE	Integrating the Healthcare Enterprise
IOCM	Imaging Object Change Management
IOD	Information Object Definition
JPEG	Joint Photographic Experts Group
KOS	Key Object Selection
MPPS	Modality Performed Procedure Step
MR	Magnetic Resonance Imaging
MWL	Modality Worklist
NM	Nuclear Medicine
O	Optional (Key Attribute)
PACS	Picture Archiving and Communication System
PET	Positron Emission Tomography
PDU	Protocol Data Unit
R	Required (Key Attribute)
SC	Secondary Capture
SCP	Service Class Provider
SCU	Service Class User
SOP	Service-Object Pair
SR	Structured Reporting
U	Unique (Key Attribute)
US	Ultrasound
VL	Visible Light
VR	Value Representation
XA	X-ray Angiography

### 3.6 References

- NEMA PS3 Digital Imaging and Communications in Medicine (DICOM) Standard, available free at <http://medical.nema.org/>
- IHE Radiology Technical Framework IOCM Extention - [https://www.ihe.net/uploadedFiles/Documents/Radiology/IHE\\_RAD\\_Suppl\\_IOC\\_M.pdf](https://www.ihe.net/uploadedFiles/Documents/Radiology/IHE_RAD_Suppl_IOC_M.pdf)
- NEMA DICOM Conformance Statement Template (Normative) - [http://dicom.nema.org/medical/dicom/current/output/html/part02.html#chapter\\_A](http://dicom.nema.org/medical/dicom/current/output/html/part02.html#chapter_A)

## 4. Implementation Model


Change Healthcare Cardiology provides the following DICOM capabilities:

- Image storage (SCU/SCP)
- Queries on image database (SCU/SCP)
- Retrieving images (SCU/SCP)
- Commitment for the storage of data (SCU/SCP)
- Printing images (SCU)
- Getting Worklist (SCU)
- Providing Worklist (SCP)
- Managing Modality-performed procedure steps (SCP/SCU)


## 4.1 Application Data Flow Diagram

Figure 1 – Change Healthcare Cardiology 14.1 DICOM Network Data Flow Diagram


**Figure 1-1 Send Instances to External System**

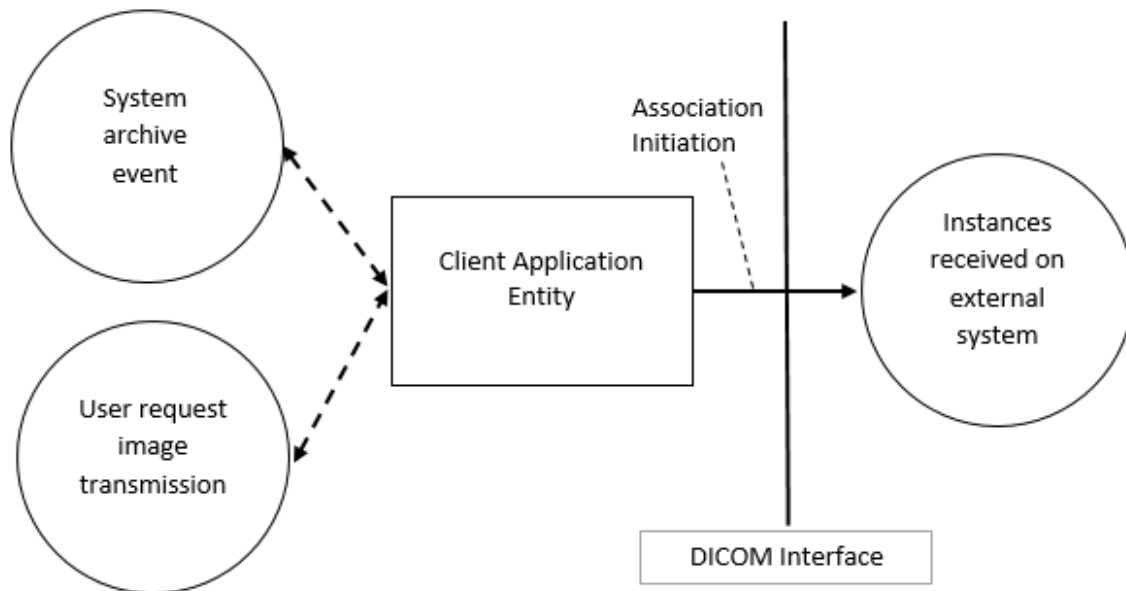


**Figure 1-2 Receive Instances from External System**

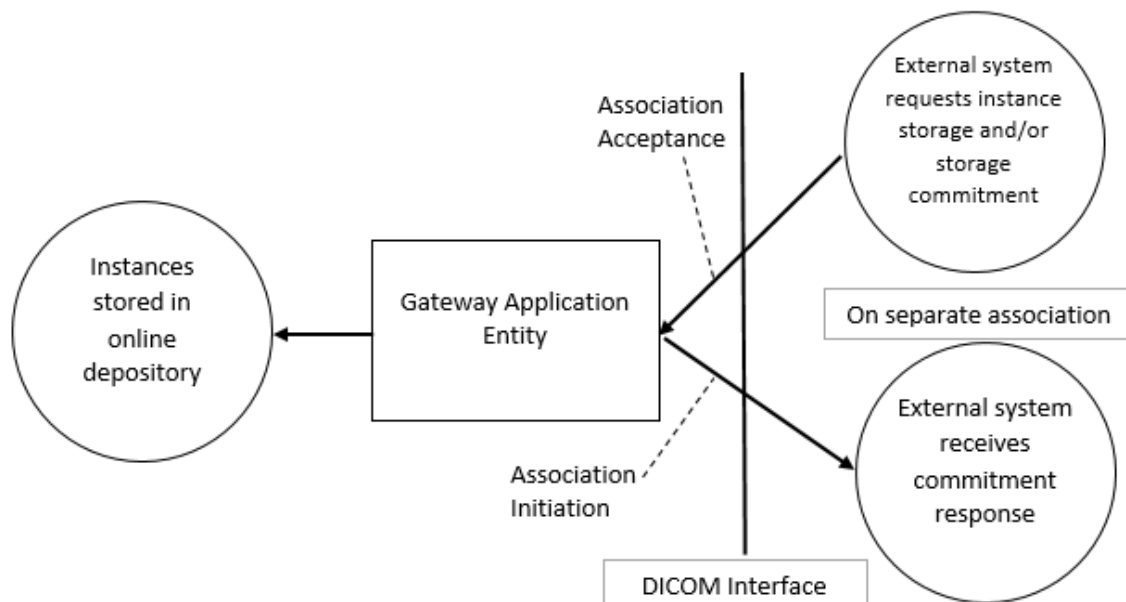


**Figure 1-3 Issue Query/Retrieve Request**


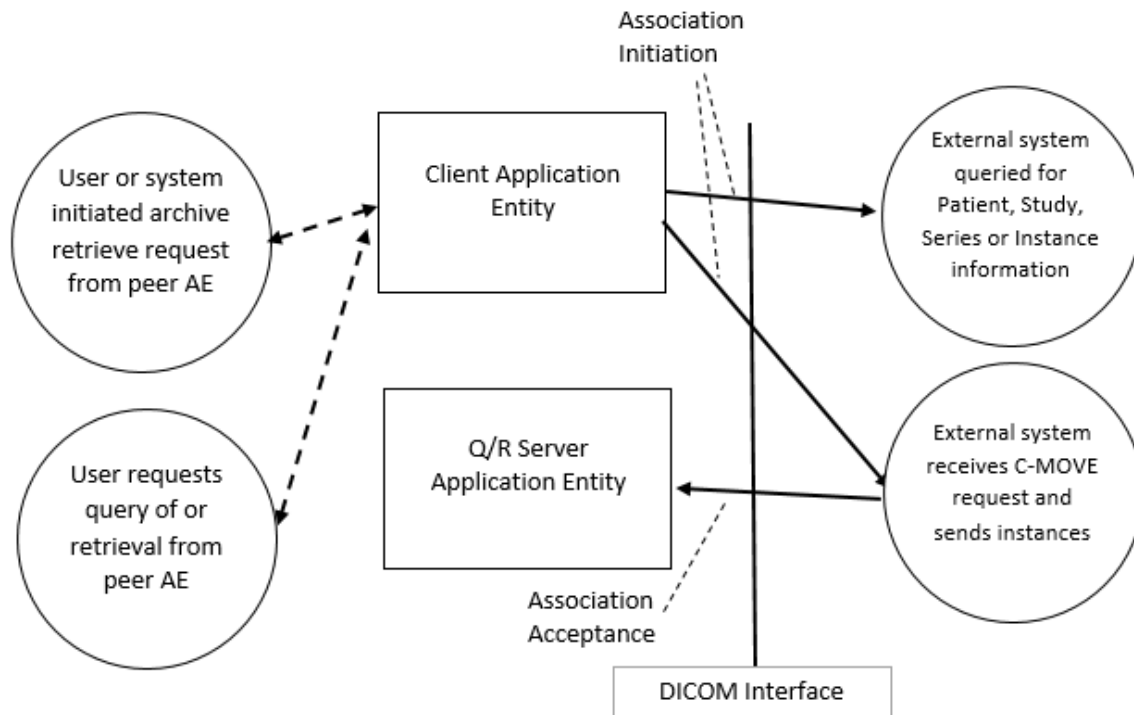



**Figure 1-4 Get Modality Worklist**

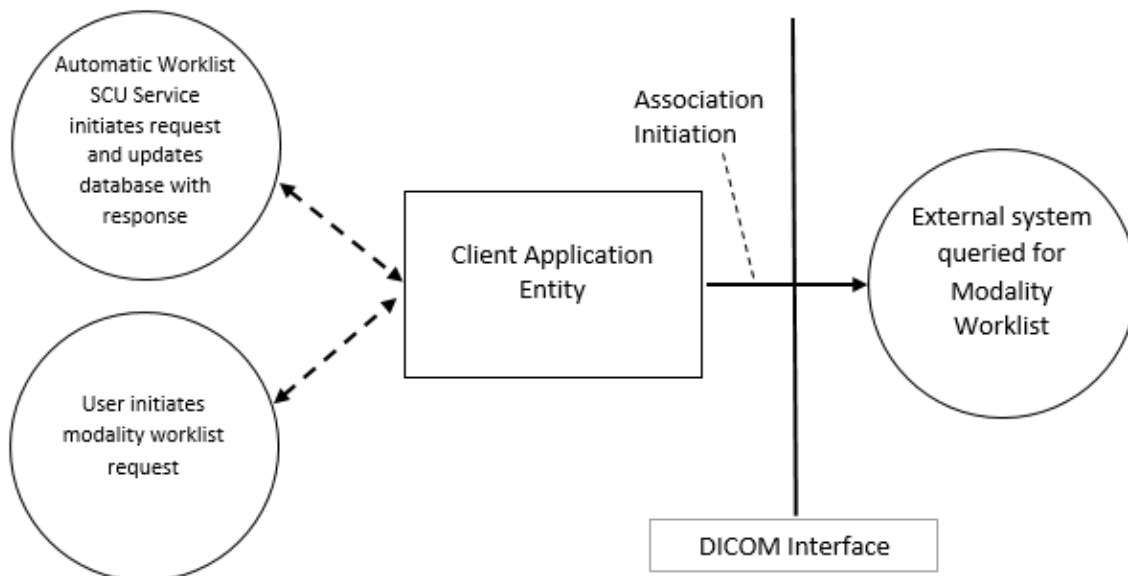

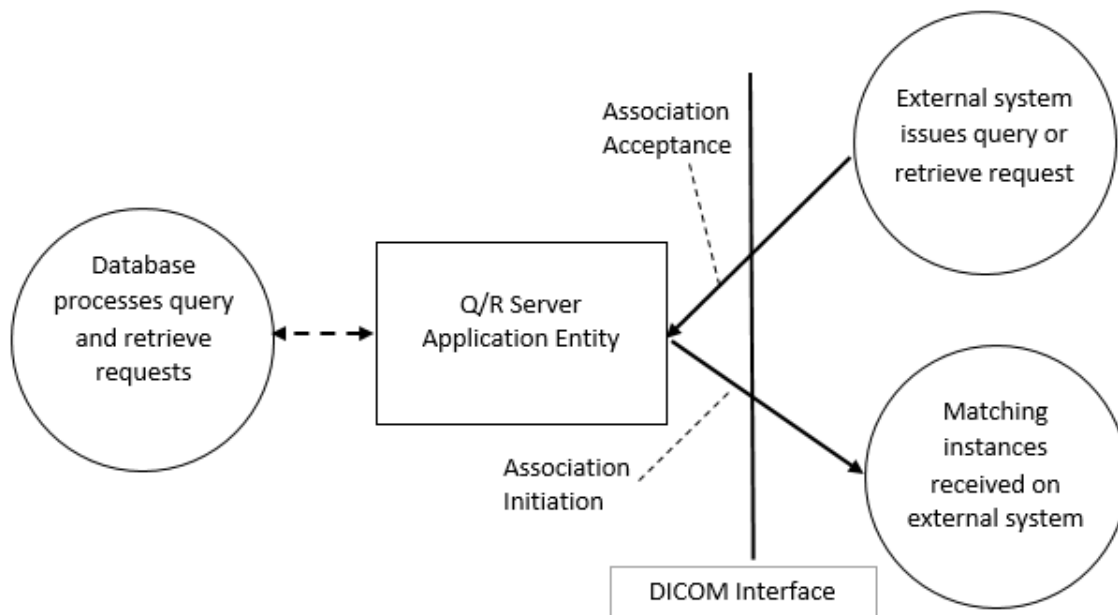
**Figure 1-5 Respond to Query/Retrieve Requests**

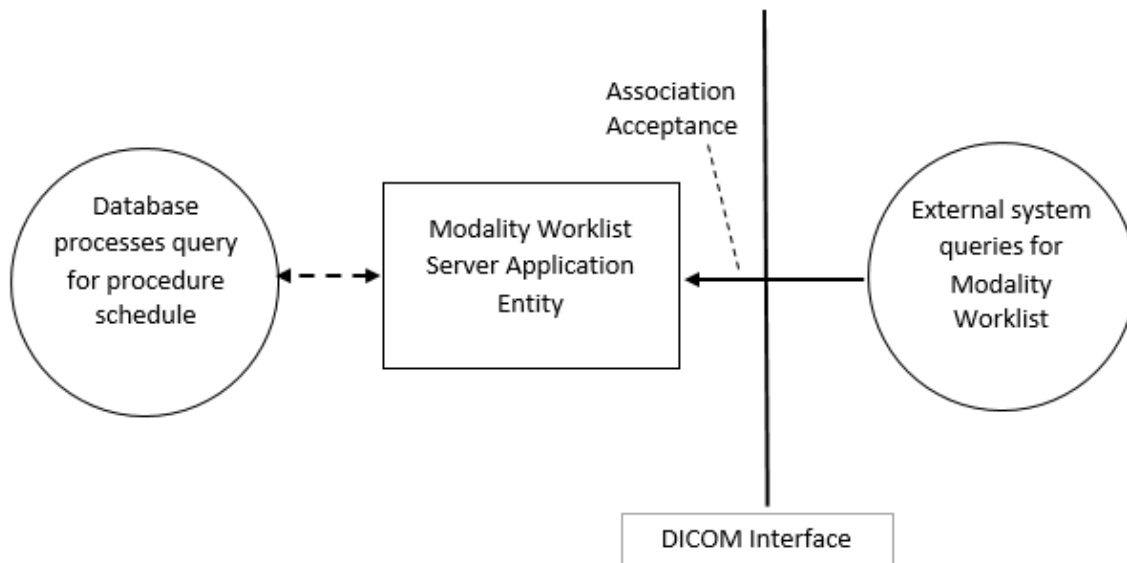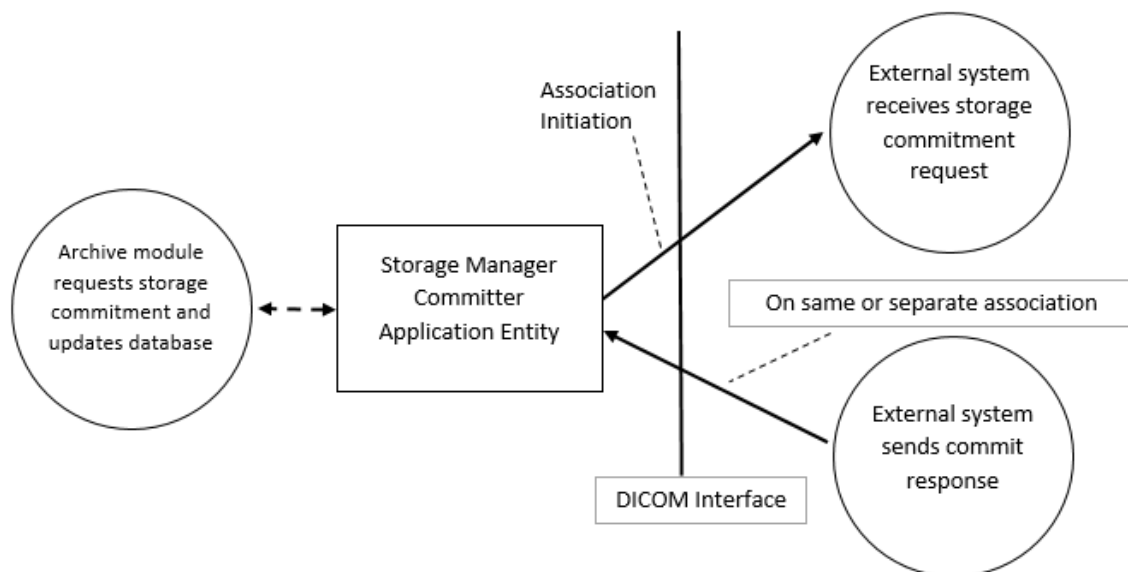


**Figure 1-6 Respond to Modality Worklist Requests****Figure 1-7 Get Storage Commitment – DICOM Archive Module**

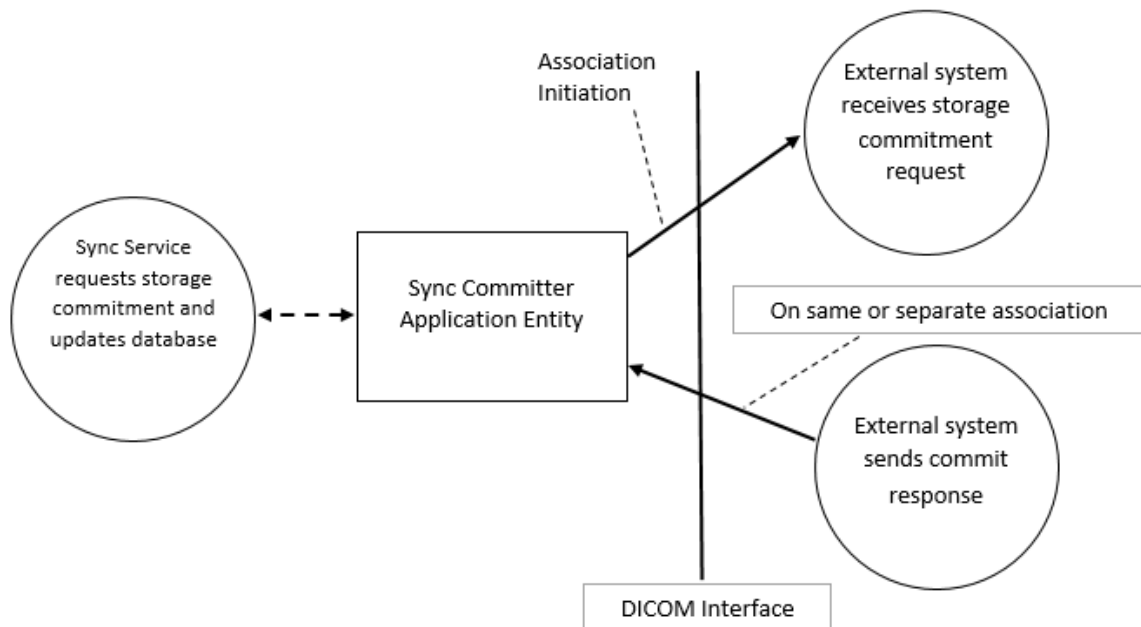
**Figure 1-8 Get Storage Commitment – Synchronization Service**

**Figure 1-9 Receive Modality Performed Procedure Step (MPPS)**

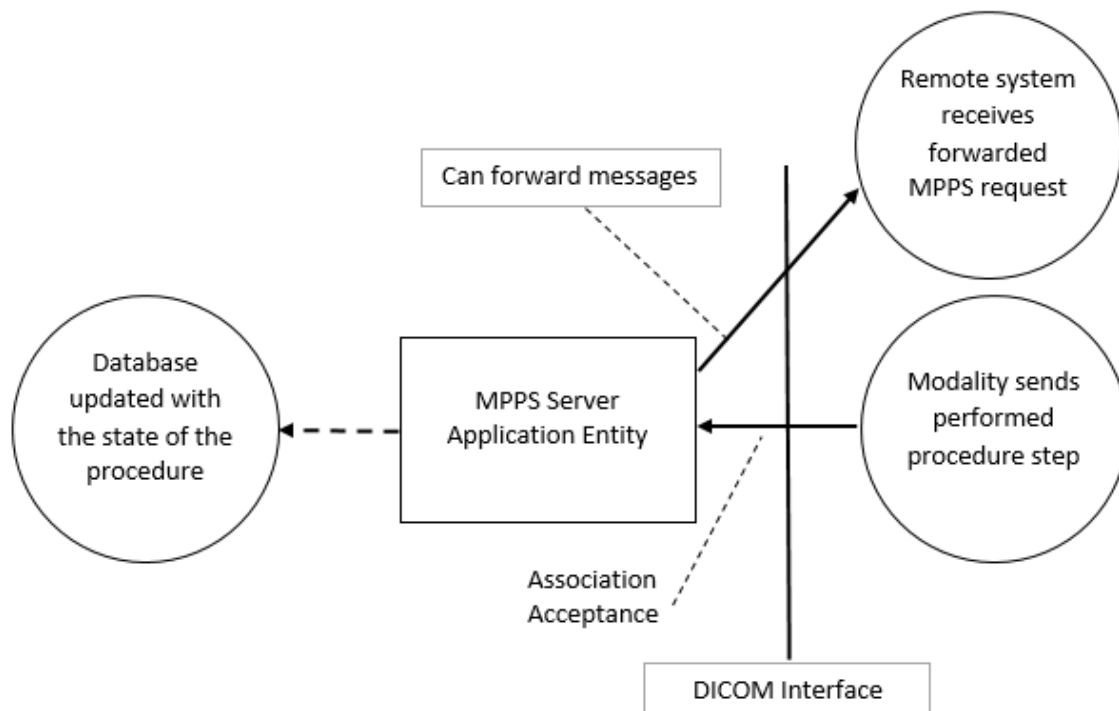

**Figure 1-10 Send rejection notes and updates instances to external system (IOCM profile operations)**

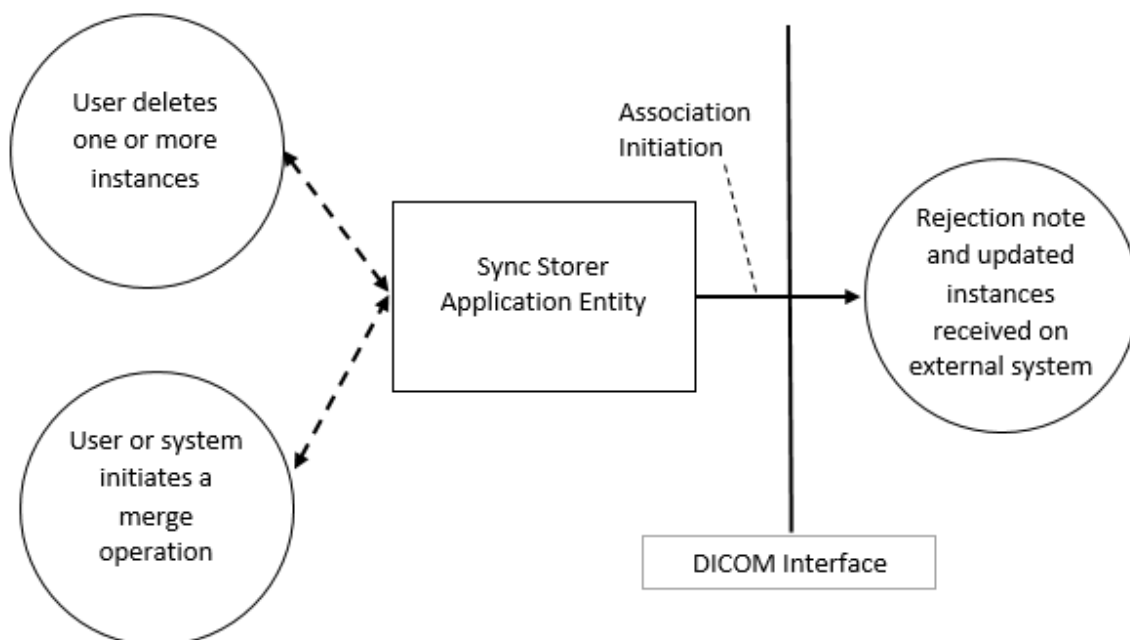

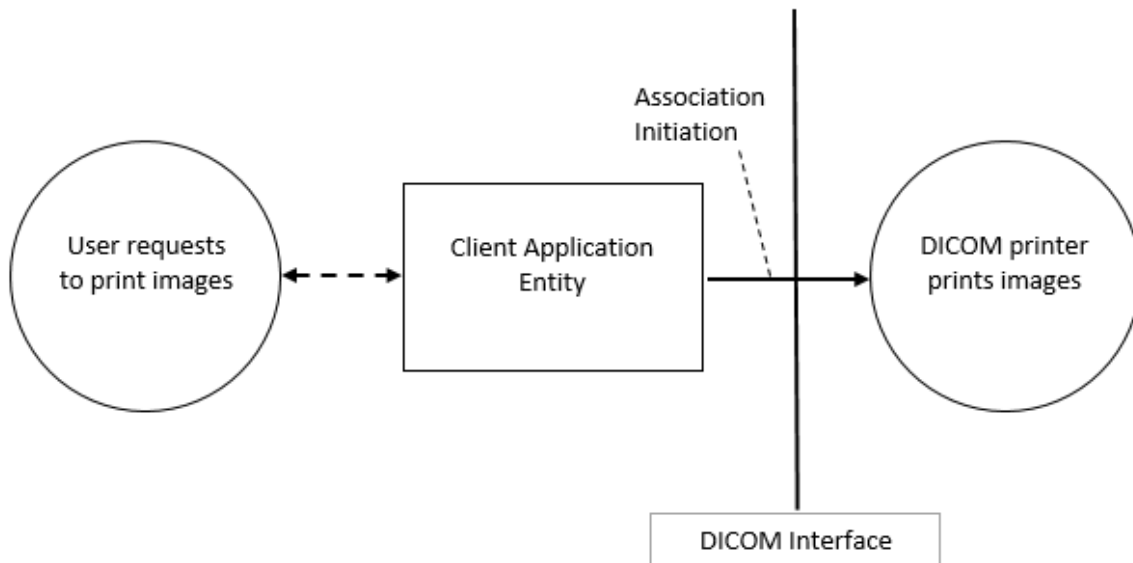**Figure 1-11 Send images to printer**

## 4.2 Functional Definition of Application Entities

### 4.2.1 Functional Definition of Client Application Entity

The Client AE acts as a multi-purpose SCU and implements the following Service Classes as SCU:

- Storage
- Query/Retrieve
- Print Management
- Modality Worklist

The Client AE can perform the following tasks:

- Send instances to a remote storage SCP AE, initiated by the archive storage manager service or the Change Healthcare Cardiology application.
- Query patient, study, series or instance level information, initiated by the Change Healthcare Cardiology application.
- Send a retrieve (C-MOVE) request to remote Query/Retrieve SCP AE, initiated by the archive storage manager service or the Change Healthcare Cardiology application.
- Query for Modality Worklist from a remote MWL SCP AE, initiated by the Automatic Worklist SCU service or the Change Healthcare Cardiology application.

- Send a request to print instances, initiated by Change Healthcare Cardiology application.

#### **4.2.2 Functional Definition of Query/Retrieve Server Application Entity**

The Query/Retrieve Server AE implements the Query/Retrieve Service Class as an SCP. The Query/Retrieve Server AE handles requests from external devices to query the database for patient, study, series and instance level information. It can also handle C-MOVE Requests from remote AEs for the retrieval of Composite SOP Instances. The Query/Retrieve Server AE can act as an SCU of the Storage Service to transfer the requested Composite SOP Instances to the requested destination.

The Query/Retrieve Server AE can act as an SCP of the Storage Service Class to serve as a C-MOVE destination and receive Composite SOP Instances that were requested by the Client AE.

#### **4.2.3 Functional Definition of Gateway Application Entity**

The Gateway AE acts as an SCP and implements the Storage Service Class operation. It can receive unsolicited instance storage requests from external DICOM storage SCUs. It also acts as an SCP for the Storage Commitment Push Model SOP Class.

#### **4.2.4 Functional Definition of Storage Manager Committer Application Entity**

The Storage Manager Committer AE implements the Storage Commitment Service Class as an SCU. When acting as an SCU, it issues a Storage Commitment Push Model N-ACTION request to a remote storage commitment SCP AE to explicitly request the remote storage commitment SCP AE to make the commitment for the safekeeping of the SOP instances mentioned in the N-ACTION request. The Storage Manager Committer AE can receive Storage Commitment Confirmation for composite SOP Instances from the Storage Commitment SCP AE on the same association or on a separate association.

#### **4.2.5 Functional Definition of Modality Worklist Server Application Entity**

The Modality Worklist Server AE implements the Modality Worklist SOP Class as an SCP. The Modality Worklist Server AE handles requests from external devices to query the database for procedure schedule.

#### **4.2.6 Functional Definition of MPPS Server Application Entity**

The MPPS Server AE implements the Modality Performed Procedure Step SOP Class as an SCP. The MPPS Server AE handles requests from external devices to update the database on a procedure state.

The Change Healthcare Cardiology MPPS SCP can also serve as MPPS SCU in order to forward an entire data set, as is, to another MPPS SCP, if configured to do so.

#### 4.2.7 Functional Definition of Sync Storer Application Entity

The Sync Storer AE acts as an SCU and implements the Storage Service Class operation. It can transmit rejection notification objects and corrected instances as part of the IHE IOCM profile.


#### 4.2.8 Functional Definition of Sync Comitter Application Entity

The Sync Comitter AE implements the Storage Commitment Service Class as an SCU. When acting as an SCU, it issues a Storage Commitment request to a remote storage commitment AE to make the commitment for the safekeeping of the SOP instances mentioned in the request. The Sync Comitter AE can receive storage commitment confirmation for composite SOP Instances from the Storage Commitment SCP AE on the same association or on a separate association.

### 4.3 Sequencing of Real-World Activities

The below figure demonstrates Change Healthcare Cardiology sequencing constraints.

**Figure 2 – Change Healthcare Cardiology Sequencing Constraints**

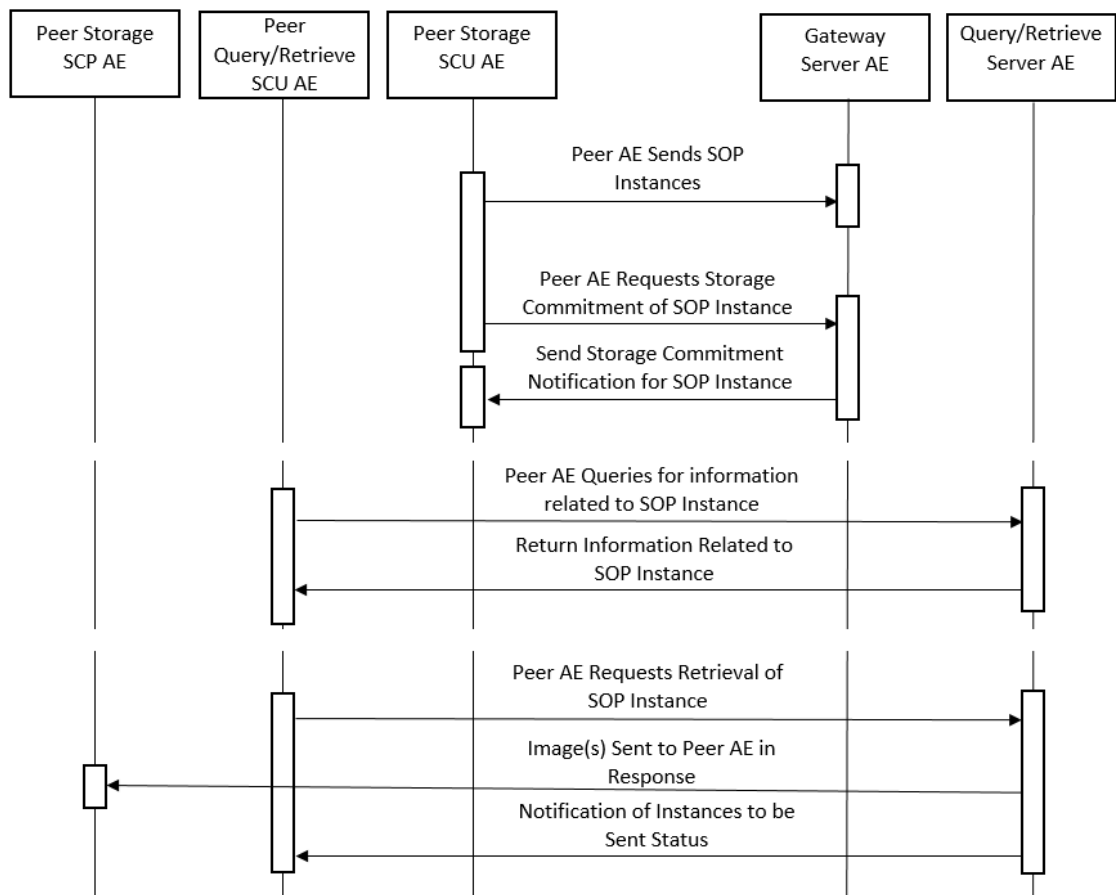

## 5. AE Specifications

### 5.1 Client AE Specification

#### 5.1.1 SOP Classes

Client AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	No
<b>Transfer</b>			
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	No
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	No
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	No
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	No
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	No
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	No
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	No
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Yes	No
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	No
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Yes	No
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	No
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Yes	No
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	No

SOP Class Name	SOP Class UID	SCU	SCP
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	No
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	No
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	No
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	No
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	No
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Yes	No
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	No
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	No
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	No
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	No
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	No
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	No
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	No
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	No
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	No
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	No
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	No
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	No
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	No
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	No
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	No
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	No



SOP Class Name	SOP Class UID	SCU	SCP
Storage			
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	No
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	No
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1	Yes	No
Intravascular Optical Coherence Tomography Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.14.1	Yes	No
Intravascular Optical Coherence Tomography Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.14.2	Yes	No
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59	Yes	No
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Yes	No
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Yes	No
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Yes	No
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	No
<b>Query/Retrieve</b>			
Patient Root Query/Retrieve Info Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	No
Study Root Query/Retrieve Info Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	No
Patient Root Query/Retrieve Info Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	No
Study Root Query/Retrieve Info Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No
<b>Workflow Management</b>			
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Yes	No
<b>Print Management</b>			
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management	1.2.840.10008.5.1.1.18	Yes	No

SOP Class Name	SOP Class UID	SCU	SCP
Meta			

## 5.1.2 Association Policies

### 5.1.2.1 General

DICOM application context for Client AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes).

### 5.1.2.2 Number of Associations

Number of Association as Association Initiator:

Maximum number of simultaneous associations	Configurable
---	--------------

### 5.1.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

### 5.1.2.4 Implementation Identifying Information

#### DICOM Implementation Class and Version for Client AE

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

## 5.1.3 Association Initiation Policy

Client AE attempts to initiate a new association in the following cases:

- To check the connection to the remote system
- To transfer (store) a series of images on the remote system
- To find several instances in the remote system
- To retrieve several instances from the remote system
- To print several images
- To get worklist modality worklist

### Real-World Activity – Verification

#### Associated Real-World Activity

The associated Real-World Activity is an attempt to check whether remote AE is ready for DICOM dialog.

### Proposed Presentation Contexts

For this Real-World Activity, the client AE will propose one of the Presentation Contexts listed in Table 1.

**Table 1 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

#### 5.1.3.1 Real-World Activity – Storing instances

##### Associated Real-World Activity

The associated Real-World Activity is an attempt to store a series of instances on a remote system.

The Client AE initiates an association for C-STORE in the following cases:

- The Change Healthcare Cardiology user has requested to send images to a specific modality/workstation
- Change Healthcare Cardiology storage manager service has requested to send instances to a specific DICOM archive destination.

### Proposed Presentation Contexts

Each time an association is initiated, the Client AE proposes one or more Presentation Contexts to be used on that association, as shown in Table 2 on page 25.

**Table 2 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Note		Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
See Note		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
See Note		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
See Note		JPEG Lossless, Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCU	None
See Note		JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCU	None
See Note		RLE Lossless	1.2.840.10008.1.2.5	SCU	None

---

**Note:** The Abstract Syntax corresponds to the SOP Class UID for Series modality. The selection of these syntaxes can be found in [Table 3:](#)

---

**Table 3 - Abstract Syntaxes**

<b>Abstract Syntax</b>	
<b>Name</b>	<b>UID</b>
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Radiotherapy Image	1.2.840.10008.5.1.4.1.1.481.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2

Abstract Syntax	
Name	UID
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Visible Light Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1
Visible Light Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2
Visible Light Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3
Visible Light Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59
Basic Text Structure Report	1.2.840.10008.5.1.4.1.1.88.11
Enhanced Structure Report	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive Structure Report	1.2.840.10008.5.1.4.1.1.88.33
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

### 5.1.3.2 Real-World Activity – Finding Instances

#### Associated Real-World Activity

The associated Real-World Activity is an attempt to find instances in a remote system. The user of the Change Healthcare Cardiology application selects the query operation button on the user interface. The user can specify wild card or specific information for Patient Name, Patient ID, Patient Sex, Patient Birthdate, Study ID, Study UID, Study Accession Number, Study Date Range, Study Time Range, Referring Physician, Modalities in Study.

Wild card queries can result in an excessive number of responses. The user interface is able to restrict the number of patients displayed.

The user can cancel the current query operation by clicking the cancel button.

Client AE defaults to using Study Root Query Model when initiating query request. The query model used can be changed to Patient Root Query Model by changing a configuration parameter.

### Multiple Sources Option

Change Healthcare Cardiology can be configured to access multiple sources with a single user request.

In the event an information source becomes unavailable, , the Change Healthcare Cardiology application provides the information it received from other sources. In addition, the Change Healthcare Cardiology informs the users that they are viewing potentially incomplete results. When a study-level or series-level query to multiple sources finds the study/series referenced in multiple places, the study/series is either duplicated or split across the systems. When the user queries of the study/series, the Change Healthcare Cardiology application collates the information, determines if the information is duplicated or split, and presents a consolidated view of the results.

### Proposed Presentation Contexts

For this Real-World Activity, Client AE will propose one of the Presentation Contexts listed in Table 4.

**Table 4- Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Patient Root	1.2.840.10008.5.1.4.1.2.1.1	Explicit VR	1.2.840.10008.1.2.2	SCU	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Query/Retrieve Information Model – FIND		Big Endian			
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

### 5.1.3.3 Real-World Activity – Retrieving Instances

#### Associated Real-World Activity

The associated Real-World Activity is an attempt to retrieve instances from a remote system.

The user selects one or more instance, series or study within studies from a list presented as a result of a previous query operation. Clicking Retrieve initiates the move operation.

The user can cancel the current Retrieve operation by clicking Cancel.

Another associated activity is an attempt to retrieve instances referenced in Change Healthcare Cardiology Database from archive without a preceding query operation.

#### Multiple Sources Option

Change Healthcare Cardiology can be configured to access multiple sources with a single user retrieval request.

When Change Healthcare Cardiology performs a study-level or series-level query to multiple sources and finds the study/series referenced in multiple places, the study/series is either duplicated or the study/series is split across the systems.

When the user requests a retrieval of the study/series, Change Healthcare Cardiology collates the information, determines whether the information is actually duplicated or split, and presents a consolidated view of results to the user.

Avoiding redundant retrieval is managed by checking whether a definite IOD has already been retrieved in the current session.

#### Proposed Presentation Contexts

For this Real-World Activity, Client AE will propose one of the Presentation Contexts listed in [Table 5](#).



**Table 5 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

**5.1.3.4 Real-World Activity – Printing Images****Associated Real-World Activity**

The associated Real-World Activity is a request to print one or more images.

The Print Module represents a single Application Entity. It acts independently of other DICOM applications that may be running on the same system. The Print Module can support printing to multiple DICOM printers at the same time, each printer being uniquely identified by an Application Entity Title and port.

**Proposed Presentation Contexts**

Client AE will propose one of the Presentation Contexts listed in Table 6.

**Table 6 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	JPEG Lossless Hierarchical First-Order Predictions	1.2.840.10008.1.2.4.70	SCU	None
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCU	None
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	RLE Lossless	1.2.840.10008.1.2.4.5	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	JPEG Lossless Hierarchical First-Order Predictions	1.2.840.10008.1.2.4.70	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	RLE Lossless	1.2.840.10008.1.2.4.5	SCU	None

### 5.1.3.5 Real-World Activity – Automatically Getting Modality Worklist from Remote System

#### Associated Real World Activity

Change Healthcare Cardiology Automatic Worklist Service requests for Modality Worklist from the remote information system. The associated Real-World activity is a request to perform a worklist query based on pre-defined criteria. The association is closed when all data have been received from the remote

DICOM network node. The client is also able to abort the association when an error occurs.

### Proposed Presentation Contexts

**Table 7 - Proposed Presentation Contexts**

<b>Presentation Context Table</b>				
<b>Abstract Syntax</b>		<b>Transfer Syntax</b>		<b>Role</b>
<b>Name</b>	<b>UID</b>	<b>Name</b>	<b>UID</b>	
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

### SOP Specific Conformance – Modality Worklist

Dependent on user requested search type and worklist configuration, C-FIND request will contain elements of the following sets of matching key attributes:

#### Find by Scheduled Date, Station and Physician

<b>Matching Key Attribute</b>
(0040,0002) Scheduled Procedure Step Start Date
(0040,0006) Scheduled Performing Physician's Name
(0040,0010) Scheduled Station Name
(0040,0001) Scheduled Station AE Title

#### Find by Modality

<b>Matching Key Attribute</b>
(0008,0060) Modality

### 5.1.3.6 Real-World Activity – Manually Getting Modality Worklist from Remote System

#### Associated Real Work Activity

User initiates requests for Modality Worklist from the remote information system using the Change Healthcare Cardiology application. The associated Real-World activity is a request to perform a worklist query based on pre-defined criteria. The association is closed when all data has been received from

the remote DICOM network node. The client is also able to abort the association when an error occurs.

### Proposed Presentation Contexts

**Table 8 - Proposed Presentation Contexts**

<b>Presentation Context Table</b>				
<b>Abstract Syntax</b>		<b>Transfer Syntax</b>		<b>Role</b>
<b>Name</b>	<b>UID</b>	<b>Name</b>	<b>UID</b>	
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

### SOP Specific Conformance – Modality Worklist

Depending on the user requested search type, the C-FIND request will contain elements of the following sets of matching key attributes:

#### Find by Patient ID and Name

<b>Matching Key Attribute</b>
(0010,0020) Patient ID
(0010,0010) Patient's Name

#### 5.1.4 Association Acceptance Policy

The Client AE does not accept associations.

## 5.2 Query/Retrieve AE Server Specification

### 5.2.1 SOP Classes

Query/Retrieve Server AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

<b>SOP Class Name</b>	<b>SOP Class UID</b>	<b>SCU</b>	<b>SCP</b>
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	Yes
<b>Transfer</b>			

SOP Class Name	SOP Class UID	SCU	SCP
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	Yes
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	Yes
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Yes	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Yes	Yes
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Yes	Yes
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	Yes
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	Yes
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	Yes
Grayscale Softcopy	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes

SOP Class Name	SOP Class UID	SCU	SCP
Presentation State Storage			
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	Yes
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	Yes
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	Yes
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	Yes
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	Yes
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	Yes
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	Yes
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	Yes
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	Yes
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	Yes
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	Yes
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	Yes
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	Yes
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1	Yes	Yes

SOP Class Name	SOP Class UID	SCU	SCP
Intravascular Optical Coherence Tomography Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.14.1	Yes	Yes
Intravascular Optical Coherence Tomography Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.14.2	Yes	Yes
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59	Yes	Yes
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Yes	Yes
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Yes	Yes
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	Yes
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Yes	Yes
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes
<b>Query/Retrieve</b>			
Patient Root Query/Retrieve Info Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	No	Yes
Study Root Query/Retrieve Info Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	No	Yes
Patient Root Query/Retrieve Info Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	No	Yes
Study Root Query/Retrieve Info Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	No	Yes
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	No	Yes

## 5.2.2 Association Policies

### 5.2.2.1 General

DICOM application context for Query/Retrieve Server AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable for both SCU/SCP (default is 16,384 bytes).

### 5.2.2.2 Number of Associations

Number of Association as Association Initiator:

Maximum number of simultaneous	3 by default (Configurable)
--------------------------------	-----------------------------

associations	
--------------	--

Number of Associations as an Association Acceptor:

Maximum number of simultaneous associations	3 by default (Configurable)
---	-----------------------------

### 5.2.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

### 5.2.2.4 Implementation Identifying Information

#### DICOM Implementation Class and Version for Query/Retrieve Server AE

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

### 5.2.3 Association Initiation Policy

Query/Retrieve Server AE attempts to initiate a new association in the following cases:

- To check the connection to the remote system
- To transfer (store) a series of instances to a remote system

#### 5.2.3.1 Real-World Activity – Verification

##### Associated Real-World Activity

The associated Real-World Activity is an attempt to check whether remote AE is ready for DICOM dialog.

##### Proposed Presentation Contexts

For this Real-World Activity, the Query/Retrieve Server AE will propose one of the Presentation Contexts listed in Table 9.

**Table 9 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None



### 5.2.3.2 Real-World Activity – Storing Instances

#### Associated Real-World Activity

The associated Real-World Activity is a retrieve (C-MOVE) request from a remote system.

#### Proposed Presentation Contexts

Each time an association is initiated, the Client AE proposes one or more Presentation Contexts to be used on that association, as shown in Table 10 on page 39.

**Table 10 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Note		Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
See Note		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
See Note		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
See Note		JPEG Lossless, Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCU	None
See Note		JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCU	None
See Note		RLE Lossless	1.2.840.10008.1.2.5	SCU	None

---

**Note:** The Abstract Syntax corresponds to the SOP Class UID for Series modality. The selection of these syntaxes can be found in [Table 11](#).

---

**Table 11 - Abstract Syntaxes**

<b>Abstract Syntax</b>	
<b>Name</b>	<b>UID</b>
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Radiotherapy Image	1.2.840.10008.5.1.4.1.1.481.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2

Abstract Syntax	
Name	UID
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Visible Light Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1
Visible Light Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2
Visible Light Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3
Visible Light Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59
Basic Text Structure Report	1.2.840.10008.5.1.4.1.1.88.11
Enhanced Structure Report	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive Structure Report	1.2.840.10008.5.1.4.1.1.88.33
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

### 5.2.3.3 Real-World Activity – Providing Storage Commitment response

The associated Real-World Activity is an attempt to make the commitment for the safekeeping of the SOP instances. Query/Retrieve Server AE uses Storage Commitment SOP Class Push Model implementation in order to guarantee the safe storage of SOP instances.

Query/Retrieve Server AE always returns the N-EVENT-REPORT on a separate association. This association is opened with reverse role negotiation, that is, the Calling AE is the SCP and the Called AE is the SCU.

After an N-ACTION request containing the Study Component Sequence has been received, the Storage Commitment N-EVENT-REPORT is built and returned.

#### Proposed Presentation Contexts

For this Real-World Activity, Query/Retrieve Server AE will propose the Presentation Contexts listed in Table 12.

**Table 12- Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

#### 5.2.4 Association Acceptance Policy

Query/Retrieve Server AE accepts an association for finding and retrieving instances.

##### 5.2.4.1 Real World Activity – Verification

Query/Retrieve Server AE accepts associations from nodes that wish to perform a verification operation on Change Healthcare Cardiology.

#### Associated Real World Activity – Verification

The Real World Activity associated with the C-ECHO request is that an external node wishes to verify network or server operation without initiating any actual work.

#### Accepted Presentation Contexts

Table 13 shows the Presentation Contexts that may be accepted by Change Healthcare Cardiology for verification operations.

**Table 13 - Acceptable Presentation Contexts for Query/Retrieve Server AE for Verification**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM	1.2.840.10008.1.2	SCP	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
		Implicit VR Little Endian			
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### SOP Specific Conformance for SOP Class Verification

Not Applicable.

#### Presentation Context Acceptance Criterion

Query/Retrieve Server AE will accept the verification SOP classes listed in [Table 13](#) above. Query/Retrieve Server AE defines no limit on the number of presentation contexts accepted. If Query/Retrieve Server AE runs out of resources when trying to accept multiple presentation contexts, it will reject the association request.

#### Transfer Syntax Selection Policies

Query/Retrieve Server AE prefers Explicit Little Endian Transfer Syntax.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priority to the choice of Transfer Syntax:

1. Explicit Little Endian Transfer Syntax
2. Implicit Little Endian Transfer Syntax
3. Explicit Big Endian Transfer Syntax

#### 5.2.4.2 Real-World Activity – Storing Instances

The Real-World Activity associated with the C-STORE operation is the storage of instances as a C-MOVE destination for the Client AE. Query/Retrieve Server AE will issue a failure status response if it is unable to store the instance.

The instances received by Query/Retrieve Server AE are stored in a temporary cache for viewing by the local Change Healthcare Cardiology application or to be copied into the online depository.

When Query/Retrieve Server AE receives the association request, it will allow the following activities to be performed during that association:

- Verification - Allow a remote DICOM device to verify that Query/Retrieve Server AE is active on the DICOM network.
- Storage Commitment - Receive the request for storage commitment.

### Associated Real-World Activity

The Real-World activity associated with the C-STORE operation is the storage of the instance on the disk of the system upon which Query/Retrieve Server AE is running. Instances are stored by writing the data set of the C-STORE command to disk and adding the PS 3.10 header.

Query/Retrieve Server AE will issue a failure status response if it is unable to store the instance on disk or if the instance does not conform to the IOD of the SOP class under which it was transmitted.

### Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 14 are acceptable to Query/Retrieve Server AE for receiving instances.

**Table 14 - Acceptable Presentation Contexts for Query/Retrieve Server AE**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Note	See Note	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
See Note	See Note	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
See Note	See Note	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
See Note	See Note	JPEG Lossless Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCP	None
See Note	See Note	JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCP	None
See Note	See Note	RLE Lossless	1.2.840.10008.1.2.4.5	SCP	None

---

**Note:** The Abstract Syntax corresponds to the SOP Class UID for Series modality and can be one of the syntaxes in Table 15.

---

**Table 15 - Abstract Syntaxes**

Abstract Syntax	
Name	UID
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1

Abstract Syntax	
Name	UID
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Radiotherapy Image	1.2.840.10008.5.1.4.1.1.481.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1

Abstract Syntax	
Name	UID
Visible Light Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1
Visible Light Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2
Visible Light Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3
Visible Light Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59
Basic Text Structure Report	1.2.840.10008.5.1.4.1.1.88.11
Enhanced Structure Report	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive Structure Report	1.2.840.10008.5.1.4.1.1.88.33
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

## SOP Specific Conformance

### 5.2.4.2.1.1 SOP Specific Conformance to Storage SOP Classes

Query/Retrieve Server AE conforms to the SOPs of the Storage Service Class at Level 2 (Full). No elements are discarded or coerced by Query/Retrieve Server AE. In the event of a successful C-STORE operation, the instances have successfully been written to Change Healthcare Cardiology system. They may be accessed by Change Healthcare Cardiology applications or through DICOM Query/Retrieve Model.

If Query/Retrieve Server AE returns one of the following status codes, then the C-STORE was unsuccessful.

Status	Action	Status	Description
A700	Refused	Out of resources	Indicates that there is not enough space to store the instance.
A800		SOP Class not	Indicates that the SOP Class



Status	Action	Status	Description
		supported	of the instance in the C-Store operation did not match the Abstract Syntax negotiated for the Presentation Context. This indicates a problem with the SCU of the Service Class.
A900	Failed	Data Set does not match SOP Class	Indicates that the Data Set does not encode an instance of the SOP Class specified. This indicates a problem with SCU of the Service Class.
C000	Unable to Process	Unable to understand	Indicates that Query/Retrieve Server AE cannot parse the Data Set into elements. This indicates a problem with the SCU.

#### 5.2.4.2.1.2 *Presentation Context Acceptance Criterion*

Query/Retrieve Server AE defines no limit on the number of presentation contexts accepted.

If Query/Retrieve Server AE runs out of resources when trying to accept multiple presentation contexts, Query/Retrieve Server AE will reject the association request. Query/Retrieve Server AE does not check for duplicate presentation contexts and will accept duplicate presentation contexts.

#### 5.2.4.2.1.3 *Transfer Syntax Selection Policies*

Query/Retrieve Server AE prefers Explicit Little Endian Transfer Syntax with compressed pixel data.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priorities to the choice of Transfer Syntax:

1. JPEG Lossless, Hierarchical, First-Order Prediction Transfer Syntax
2. Explicit Little Endian Transfer Syntax
3. Implicit Little Endian Transfer Syntax
4. Explicit Big Endian Transfer Syntax

### 5.2.4.3 Real World Activity – Finding instances

#### Associated Real World Activity

The Associated Real-World Activity associated with the C-FIND operation is the finding of the instance in the Change Healthcare Cardiology system.

Query/Retrieve Server AE will issue a failure status response if it is unable to find

the instance. The search is performed by comparing the keys specified in request with corresponding keys of instances in system.

#### Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 16 are acceptable to Query/Retrieve Server AE for finding instances.

**Table 16- Acceptable Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### SOP Specific Conformance for FIND SOP Classes

Query/Retrieve Server AE conforms to the SOPs of the Find Service Class at Level 2 (Full).

**Table 17-Patient C-FIND Supported Elements**

Attribute Name	Tag	VR	Type	Matching
<b>Patient Level</b>				
Patient's Name	(0010,0010)	PN	R	*,U
Patient ID	(0010,0020)	LO	U	*,U
Issuer of Patient ID	(0010,0021)	LO	O	*,U
Patient's Birth Date	(0010,0030)	DA	O	R,U

Attribute Name	Tag	VR	Type	Matching
Patient's Sex	(0010,0040)	CS	O	S,U
<b>Study Level</b>				
Study Date	(0008,0020)	DA	R	R,U
Study Time	(0008,0030)	TM	R	R,U
Accession Number	(0008,0050)	SH	R	*,U
Study Instance UID	(0020,000D)	UI	U	S,U
Study ID	(0020,0010)	SH	O	*,U
Modalities in Study (NOTE1)	(0008,0061)	CS	O	S,U
Referring Physician's Name	(0008,0090)	LO	O	*,U
Study Description	(0008,1030)	LO	O	*,U
Number of Study Related Series	(0020,1206)	IS	O	NONE
Number of Study Related Instances	(0020,1208)	IS	O	NONE
<b>Series Level</b>				
Modality	(0008,0060)	CS	R	S,U
Series Instance UID	(0020,000E)	UI	U	S,U
Series Number	(0020,0011)	IS	R	*,U
Series Description	(0008,103E)	LO	O	*,U
Performing Physician's Name	(0008,1050)	PN	O	*,U
<b>Instance Level</b>				
Instance Number	(0020,0013)	IS	R	*,U
SOP Instance UID	(0008,0018)	UI	U	S,U
SOP Class UID	(0008,0016)	UI	O	NONE

**Table 18 - Study Root C-FIND Supported Elements**

Attribute Name	Tag	VR	Type	Matching
<b>Study Level</b>				
Study Date	(0008,0020)	DA	R	R,U
Study Time	(0008,0030)	TM	R	R,U
Accession Number	(0008,0050)	SH	R	*,U
Patient's Name	(0010,0010)	PN	R	*,U

Attribute Name	Tag	VR	Type	Matching
Patient ID	(0010,0020)	LO	R	*,U
Study ID	(0020,0010)	SH	R	*,U
Study Instance UID	(0020,000D)	UI	U	S,U
Issuer of Patient ID	(0010,0021)	LO	O	*,U
Patient's Birth Date	(0010,0030)	DA	O	R,U
Patient's Sex	(0010,0040)	CS	O	S,U
Modalities in Study (NOTE1)	(0008,0061)	CS	O	S,U
Referring Physician's Name	(0008,0090)	LO	O	*,U
Study Description	(0008,1030)	LO	O	*,U
Number of Study Related Series	(0020,1206)	IS	O	NONE
Number of Study Related Instances	(0020,1208)	IS	O	NONE
<b>Series Level</b>				
Modality	(0008,0060)	CS	R	S,U
Series Number	(0020,0011)	IS	R	*,U
Series Instance UID	(0020,000E)	UI	U	S,U
Series Description	(0008,103E)	LO	O	*,U
Performing Physician's Name	(0008,1050)	PN	O	*,U
Number of Series Related Instances	(0020,1209)	IS	O	NONE
<b>Instance Level</b>				
Instance Number	(0020,0013)	IS	R	*,U
SOP Instance UID	(0008,0018)	UI	U	S,U
SOP Class UID	(0008,0016)	UI	O	NONE

The Key Types Symbols for the Query/Retrieve Information Models:

U – Unique Key Attribute

R – Required Key Attribute

O – Optional Key Attribute

The types of Matching supported by the Query/Retrieve Server AE:

S - indicates Single Value Matching is supported.

R - indicates Range Matching is supported.

\* - indicates Wildcard Matching is supported.

U - indicates Universal Matching is supported.

NOTE1 – “Modalities in Study” attribute also supports matching a list of single values, delimited by backslash (“\”). Each value in the list of the request may generate a match.

The Query/Retrieve Server AE searches the Change Healthcare Cardiology Database for the requested Information Objects described in the C-FIND identifier and returns a response for each match. Possible response status values are listed in the following table:

Status	Action	Status	Description
A700	Refused	Out of resources	Indicates that there is not enough space to store the instance.
A900	Failed	Data Set does not match SOP Class	Indicates that the Data Set does not encode an instance of the SOP Class specified. This indicates a problem with SCU of the Service Class
C000	Unable to Process	Unable to understand	Indicates that Query/Retrieve Server AE cannot parse the Data Set into elements. This indicates a problem with the SCU
FE00	Cancel		Terminated due to Cancel Request
0000	Success		Matching completed
FF00	Pending		Matches are continuing

The attribute (0000,0902) contains a descriptive message to explain error returns.

#### Presentation Context Acceptance Criterion

Query/Retrieve Server AE defines no limit on the number of presentation contexts accepted.

If Query/Retrieve Server AE runs out of resources when trying to accept multiple presentation contexts, Query/Retrieve Server AE will reject the association

request. Query/Retrieve Server AE does not check for duplicate presentation contexts and will accept duplicate presentation contexts.

#### Transfer Syntax Selection Policy

The Query/Retrieve Server AE Application Entity conforms to the DICOM Patient Root Query/Retrieve and DICOM Study Root Query/Retrieve Service Class as an SCP for the Abstract Syntaxes listed in [Table 16](#).

Query/Retrieve Server AE prefers Explicit Little Endian Transfer Syntax.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priority to the choice of Transfer Syntax:

1. Explicit Little Endian Transfer Syntax
2. Implicit Little Endian Transfer Syntax
3. Explicit Big Endian Transfer Syntax

#### 5.2.4.4 Real World Activity – Retrieving

##### Associated Real World Activity

The Real-World Activity associated with the C-MOVE operation is retrieving of the instance from the Change Healthcare Cardiology system by a remote system. Query/Retrieve Server AE will issue a failure status response if it is unable to retrieve the instance.

##### Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 19 are acceptable to Query/Retrieve Server AE for retrieving instances.

**Table 19 - Acceptable Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

A response is returned for each match found in the Change Healthcare Cardiology database.

#### SOP Specific Conformance for MOVE SOP Classes

Query/Retrieve Server AE conforms to the SOPs of the Move Service Class at Level 2 (Full). Possible response status values are listed in the following table.

Status Code	Action	Status
A700	Refused	Out of resources
A702		Unable to perform sub-operation
A801		Move destination unknown
A900	Failed	Data Set does not match SOP Class
C000		Unable to Process
FE00	Cancel	Terminated due to Cancel Request
0000	Success	Sub-operations completed
B000	Warning	Sub-operations completed – 1 or more failures
FF00	Pending	Matches are continuing

The attribute (0000,0902) contains a descriptive message to explain error returns.

#### Presentation Context Acceptance Criterion

Query/Retrieve Server AE defines no limit on the number of presentation contexts accepted.

If Query/Retrieve Server AE runs out of resources when trying to accept multiple presentation contexts, Query/Retrieve Server AE will reject the association request. Query/Retrieve Server AE does not check for duplicate presentation contexts and will accept duplicate presentation contexts.

### Transfer Syntax Selection Policy

Query/Retrieve Server AE prefers Explicit Little Endian Transfer Syntax.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priority to the choice of Transfer Syntax:

1. Explicit Little Endian Transfer Syntax
2. Implicit Little Endian Transfer Syntax
3. Explicit Big Endian Transfer Syntax

#### 5.2.4.5 Real-World Activity – Storage Commitment

##### Associated Real-World Activity

The associated Real-World Activity is an attempt to make the commitment for the safekeeping of the SOP instances. Query/Retrieve Server AE uses Storage Commitment SOP Class Push Model implementation in order to guarantee the safe storage of SOP instances.

Query/Retrieve Server AE always returns the N-EVENT-REPORT on a separate association. This association is opened with reverse role negotiation, that is, the Calling AE is the SCP and the Called AE is the SCU.

After an N-ACTION request containing the Study Component Sequence has been received, the Storage Commitment N-EVENT-REPORT is built and returned.

##### Proposed Presentation Contexts

For this Real-World Activity, Query/Retrieve Server AE will propose the Presentation Contexts listed in Table 20.

**Table 20- Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.2	SCU	None



## 5.3 Gateway AE Specification

### 5.3.1 SOP Classes

Gateway AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	No	Yes
<b>Transfer</b>			
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	No	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	No	Yes
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	No	Yes
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	No	Yes
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	No	Yes
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	No	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	No	Yes
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	No	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	No	Yes
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	No	Yes
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	No	Yes
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	No	Yes
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	No	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	No	Yes
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	No	Yes

SOP Class Name	SOP Class UID	SCU	SCP
Storage			
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3	No	Yes
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	No	Yes
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5	No	Yes
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	No	Yes
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	No	Yes
RT Image	1.2.840.10008.5.1.4.1.1.481.1	No	Yes
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	No	Yes
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	No	Yes
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	No	Yes
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	No	Yes
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	No	Yes
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	No	Yes
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	No	Yes
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	No	Yes
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	No	Yes
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	No	Yes
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	No	Yes
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	No	Yes
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	No	Yes
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	No	Yes
Cardiac Electrophysiology	1.2.840.10008.5.1.4.1.1.9.3.1	No	Yes

SOP Class Name	SOP Class UID	SCU	SCP
Waveform Storage			
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	No	Yes
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1	No	Yes
Intravascular Optical Coherence Tomography Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.14.1	No	Yes
Intravascular Optical Coherence Tomography Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.14.2	No	Yes
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59	No	Yes
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	No	Yes
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	No	Yes
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	No	Yes
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	No	Yes
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	No	Yes
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	No	Yes*
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	No	Yes

\*The Gateway AE is able to receive Raw Data Storage instances, however, the Gateway AE cannot serve as an archive for Raw Data Storage instances as they are not stored in the Change Healthcare Cardiology image cache (online depository) but on a temporary storage location managed by the customer. The Gateway AE is not able to provide a storage commitment for Raw Data Storage instances. Additional limitations apply. For more information please contact your support representative.

### 5.3.2 Association Policies

#### 5.3.2.1 General

DICOM application context for Gateway AE :

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes).

**5.3.2.2 Number of Associations**

Number of Associations as an Association Acceptor:

Maximum number of simultaneous associations	1 by default (configurable)
---	-----------------------------

**5.3.2.3 Asynchronous Nature**

Asynchronous mode (multiple concurrent operations on one association) is not supported.

**5.3.2.4 Implementation Identifying Information****DICOM Implementation Class and Version for Gateway AE**

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

**5.3.3 Association Initiation Policy****5.3.3.1 Real-World Activity – Verification****Associated Real-World Activity**

The associated Real-World Activity is an attempt to check whether remote AE is ready for DICOM dialog.

**Proposed Presentation Contexts**

For this Real-World Activity, the client AE will propose one of the Presentation Contexts listed in Table 21.

**Table 21 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

**5.3.3.2 Real-World Activity – Send Storage Commitment Response****Associated Real-World Activity**

The associated Real-World Activity is an attempt to make the commitment for the safekeeping of the SOP instances. Gateway AE uses Storage Commitment SOP Class Push Model implementation in order to guarantee the safe storage of SOP instances.

After an N-ACTION request containing the Study Component Sequence has been received, the Storage Commitment N-EVENT-REPORT is built and returned.

Depending on configuration, Gateway AE may return the N-EVENT-REPORT on a separate association. This association is opened with reverse role negotiation, that is, the Calling AE is the SCP and the Called AE is the SCU.

### Proposed Presentation Contexts

For this Real-World Activity, Query/Retrieve Server AE will propose the Presentation Contexts listed in Table 22.

**Table 22- Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Storage Commitment Push Model	1.2.840.10008.1.20.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

### 5.3.4 Association Acceptance Policy

Gateway AE accepts an association for storing instances and for storage commitment requests.

#### 5.3.4.1 Real World Activity – Verification

Gateway AE accepts associations from nodes that wish to perform a verification operation.

#### Associated Real World Activity – Verification

The Real World Activity associated with the C-ECHO request is that an external node wishes to verify network or server operation without initiating any actual work.

### Accepted Presentation Contexts

[Table 23](#) shows the Presentation Contexts that may be accepted by Gateway AE for verification operations.

**Table 23 - Acceptable Presentation Contexts for Gateway AE for Verification**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

**SOP Specific Conformance for SOP Class Verification**

Not Applicable.

**Presentation Context Acceptance Criterion**

Gateway AE will accept the verification SOP classes listed in Table 23 above.

Gateway AE defines no limit on the number of presentation contexts accepted.

If Gateway AE runs out of resources when trying to accept multiple presentation contexts, it will reject the association request.

**Transfer Syntax Selection Policies**

Gateway AE prefers Explicit Little Endian Transfer Syntax.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priority to the choice of Transfer Syntax:

1. Explicit Little Endian Transfer Syntax
2. Implicit Little Endian Transfer Syntax
3. Explicit Big Endian Transfer Syntax

**5.3.4.2 Real-World Activity – Storing Instances**

The Real-World Activity associated with the C-STORE operation is the storage of the instance in the Change Healthcare Cardiology system. Gateway AE will issue a failure status response if it is unable to store the instance.

When Gateway AE receives the association request, it will allow the following activities to be performed during that association:

- Verification - Allow a remote DICOM device to verify that Gateway AE is active on the DICOM network
- Storage Commitment - Receive the request for storage commitment.

**Associated Real-World Activity**

The Real-World activity associated with the C-STORE operation is the storage of the instance on the disk of the system upon which Gateway AE is running. Instances are stored by writing the data set of the C-STORE command to disk and adding the PS 3.10 header.

Gateway AE will issue a failure status response if it is unable to store the instance on disk or if the instance does not conform to the IOD of the SOP class under which it was transmitted.

**Accepted Presentation Contexts**

Any of the Presentation Contexts shown in Table 24 are acceptable to Gateway AE for receiving instances.

**Table 24 - Acceptable Presentation Contexts for Gateway AE**

<b>Presentation Context Table</b>					
<b>Abstract Syntax</b>		<b>Transfer Syntax</b>		<b>Role</b>	<b>Extended Negotiation</b>
<b>Name</b>	<b>UID</b>	<b>Name</b>	<b>UID</b>		
See Note	See Note	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
See Note	See Note	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
See Note	See Note	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
See Note	See Note	JPEG Lossless Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCP	None
See Note	See Note	JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCP	None
See Note	See Note	RLE Lossless	1.2.840.10008.1.2.4.5	SCP	None

**Note:** The Abstract Syntax corresponds to the SOP Class UID for Series modality and can be one of the syntaxes listed on Table 25.

**Table 25- Abstract Syntaxes**

<b>Abstract Syntax</b>	
<b>Name</b>	<b>UID</b>
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1

<b>Abstract Syntax</b>	
<b>Name</b>	<b>UID</b>
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Radiotherapy Image	1.2.840.10008.5.1.4.1.1.481.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage –	1.2.840.10008.5.1.4.1.1.1.3



Abstract Syntax	
Name	UID
For Presentation	
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Visible Light Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1
Visible Light Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2
Visible Light Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3
Visible Light Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59
Basic Text Structure Report	1.2.840.10008.5.1.4.1.1.88.11
Enhanced Structure Report	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive Structure Report	1.2.840.10008.5.1.4.1.1.88.33
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66

The Gateway AE is able to receive Raw Data Storage instances, however, the Gateway AE cannot serve as archive for them as they are not stored in the Change Healthcare Cardiology image cache (online depository) but on a storage location managed by the customer. The Gateway AE is not able to provide a storage commitment for Raw Data Storage instances. Additional limitations apply. For more information please contact your support representative.

## SOP Specific Conformance

### 5.3.4.2.1.1 *SOP Specific Conformance to Storage SOP Classes*

Gateway AE conforms to the SOPs of the Storage Service Class at Level 2 (Full). No elements are discarded or coerced by Gateway AE. In the event of a successful C-STORE operation, the instances have successfully been written to Change Healthcare Cardiology system. They may be accessed by Change

Healthcare applications or through DICOM Query/Retrieve Model (except for Raw Data Storage).

If Gateway AE returns one of the following status codes, then the C-STORE was unsuccessful.

Status	Action	Status	Description
A700	Refused	Out of resources	Indicates that there is not enough space to store the instance.
A800		SOP Class not supported	Indicates that the SOP Class of the instance in the C-Store operation did not match the Abstract Syntax negotiated for the Presentation Context. This indicates a problem with the SCU of the Service Class.
A900	Failed	Data Set does not match SOP Class	Indicates that the Data Set does not encode an instance of the SOP Class specified. This indicates a problem with SCU of the Service Class.
C000	Unable to Process	Unable to understand	Indicates that Change Healthcare Cardiology cannot parse the Data Set into elements. This indicates a problem with the SCU.

#### 5.3.4.2.1.2 *Presentation Context Acceptance Criterion*

Gateway AE defines no limit on the number of presentation contexts accepted.

If Gateway AE runs out of resources when trying to accept multiple presentation contexts, Gateway AE will reject the association request. Gateway AE does not check for duplicate presentation contexts and will accept duplicate presentation contexts.

#### 5.3.4.2.1.3 *Transfer Syntax Selection Policies*

If offered a choice of Transfer Syntaxes in a Presentation Context, Gateway AE will apply the following priorities to the choice of Transfer Syntax:

1. JPEG Lossless, Hierarchical, First-Order Prediction Transfer Syntax
2. Explicit Little Endian Transfer Syntax
3. Implicit Little Endian Transfer Syntax
4. Explicit Big Endian Transfer Syntax

The associated Real-World Activity is an attempt to make the commitment for the safekeeping of the SOP instances. Gateway AE uses Storage Commitment SOP Class Push Model implementation in order to guarantee the safe storage of SOP instances.

Depeding on configuration, Gateway AE may return the N-EVENT-REPORT on a separate association or the same association. This association is opened with reverse role negotiation, that is, the Calling AE is the SCP and the Called AE is the SCU.

After an N-ACTION request containing the Study Component Sequence has been received, the Storage Commitment N-EVENT-REPORT is built and returned to requester.

## 5.4 Storage Manager Committer AE Specification

### 5.4.1 SOP Classes

Storage Manager Committer AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	No
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No

### 5.4.2 Association Policies

#### 5.4.2.1 General

DICOM application context for Storage Manager Committer AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes).

#### 5.4.2.2 Number of Associations

Number of Association as Association Initiator:

Maximum number of simultaneous associations	1
---	---

Number of Associations as an Association Acceptor:

Maximum number of simultaneous associations	1
---	---

#### 5.4.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

#### 5.4.2.4 Implementation Identifying Information

DICOM Implementation Class and Version for Storage Manager Committer AE:

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

### 5.4.3 Association Initiation Policy

#### 5.4.3.1 Real-World Activity – Verification

##### Associated Real-World Activity

The associated Real-World Activity is an attempt to check whether remote AE is ready for DICOM dialog.

##### Proposed Presentation Contexts

For this Real-World Activity, the Storage Manager Committer AE will propose one of the Presentation Contexts listed in Table 26.

**Table 26 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

### 5.4.3.2 Real-World Activity – Getting Storage Commitment from a Remote System

#### Associated Real-World Activity

Storage Manager Committer AE requests Storage Commitment from the remote DICOM Archive solution after sending instances to the remote DICOM Archive and receiving a response confirming the instances were archived.

#### Proposed Presentation Contexts

For this Real-World Activity, the Storage Manager Committer AE will propose one of the Presentation Contexts listed in [Table 26](#).

**Table 27 -Proposed Presentation Contexts**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

### 5.4.4 Association Acceptance Policy

#### 5.4.4.1 Real-World Activity – Receive Storage Commitment Response

#### Associated Real-World Activity

The associated Real-World Activity is receiving a storage commitment response on a separate association than the storage commitment request.

#### Accepted Presentation Contexts

Table 28 shows the Presentation Contexts that may be accepted by Storage Manager Committer AE for receiving Storage Commitment Response.

**Table 28 - Acceptable Presentation Contexts by Storage Manager Committer AE for receiving Storage Commitment Response**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

## 5.5 Modality Worklist Server AE Specification

### 5.5.1 SOP Classes

Modality Worklist Server AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	No	Yes
<b>Workflow Management</b>			
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	No	Yes

### 5.5.2 Association Policies

#### 5.5.2.1 General

DICOM application context for Modality Worklist Server AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes).

#### 5.5.2.2 Number of Associations

Number of Associations as an Association Acceptor:

Maximum number of simultaneous associations	3 by default (configurable)
---	-----------------------------

#### 5.5.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

**5.5.2.4 Implementation Identifying Information**

DICOM Implementation Class and Version for Modality Worklist Server AE:

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

**5.5.3 Association Initiation Policy**

The Modality Worklist Server AE does not initiate associations.

**5.5.4 Association Acceptance Policy**

Modality Worklist Server AE accepts an association for verification and providing modality worklist.

**5.5.4.1 Real World Activity – Verification**

Modality Worklist Server AE accepts associations from nodes that wish to perform a verification operation on Change Healthcare Cardiology.

**Associated Real World Activity – Verification**

The Real World Activity associated with the C-ECHO request is that an external node wishes to verify network or server operation without initiating any actual work.

**Accepted Presentation Contexts**

Table 29 shows the Presentation Contexts that may be accepted by Modality Worklist Server AE for verification operations.

**Table 29 - Acceptable Presentation Contexts by Modality Worklist Server AE for Verification**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

**SOP Specific Conformance for SOP Class Verification**

Not Applicable.

**Presentation Context Acceptance Criterion**

Modality Worklist Server AE will accept the verification SOP classes listed in Table 29 above. Modality Worklist Server AE defines no limit on the number of presentation contexts accepted. If Modality Worklist Server AE runs out of

resources when trying to accept multiple presentation contexts, Modality Worklist Server AE will reject the association request.

#### Transfer Syntax Selection Policies

Modality Worklist Server AE prefers Explicit Little Endian Transfer Syntax.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priority to the choice of Transfer Syntax:

1. Explicit Little Endian Transfer Syntax
2. Implicit Little Endian Transfer Syntax
3. Explicit Big Endian Transfer Syntax

#### 5.5.4.2 Real-World Activity – Providing Modality Worklist

##### Associated Real World Activity – Providing Modality worklist

The Real World Activity associated is that an external system wishes to query for modality worklist.

Modality Worklist Server AE will wait for an association as an SCP for the Modality Worklist Service Class. When a C-FIND request is received, a search is done in Change Healthcare Cardiology database for the data with the requested attributes, and a list of found attributes is returned to the remote requester. The Modality Worklist Server AE accepts a number of associations, which is configured at the time of system initialization.

#### Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 30 are acceptable by Modality Worklist Server AE for providing modality worklist.

**Table 30- Accepted Presentation Contexts**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCP
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP



**SOP Specific Conformance for Modality Worklist SOP Class**

Modality Worklist Server AE supports attribute matching as defined by the Modality Worklist Information Model.

If the requesting station is associated (by AE title) to a certain facility in the Change Healthcare Cardiology system, the results sent back to the station will be filtered by its associated facility.

The supported Return Key Attributes are listed in the following table. The actual return key attributes will depend on the customer's configuration.

Description	Tag	Matching Key Type	Return Key Type
<b>Scheduled Procedure Step</b>			
Scheduled Procedure Step Sequence	(0040,0100)	R	1
>Scheduled Station AE Title	(0040,0001)	R	1
>Scheduled Procedure Step Start Date	(0040,0002)	R	1
>Scheduled Procedure Step Start Time	(0040,0003)	R	1
>Modality	(0008,0060)	R	1
>Scheduled Performing Physician's Name	(0040,0006)	R	2
>Scheduled Procedure Step Description	(0040,0007)	O	1C
>Scheduled Station Name	(0040,0010)	O	2
>Scheduled Procedure Step ID	(0040,0009)	O	1
>Scheduled Procedure Step Location	(0040,0011)	O	2
>Scheduled Action Item Code Sequence	(0040,0008)	O	1C
>>Code Value	(0008,0100)	O	1C
>>Coding Scheme Designator	(0040,0102)	O	1C
>>Pre-Medication	(0040,0012)	O	2C
>Scheduled Procedure Step Status	(0040,0020)	O	3

Description	Tag	Matching Key Type	Return Key Type
<b>Requested Procedure</b>			
Requested Procedure ID	(0040,1001)	O	1
Requested Procedure Description	(0032,1060)	O	1C
Requested Procedure Code Sequence	(0032,1064)	O	1C
>Code Value	(0008,0100)	O	1C
>Coding Scheme Designator	(0008,0102)	O	1C
Study Instance UID	(0020,000D)	O	1
Referenced Study Sequence	(0008,1110)	O	2
>Referenced SOP Class UID	(0008,1150)	O	1C
>Referenced SOP Instance UID	(0008,1155)	O	1C
Requested Procedure Priority	(0040,1003)	O	2
<b>Imaging Service Request</b>			
Accession Number	(0008,0050)	O	2
<b>Scheduled Procedure Step</b>			
Requesting Physician	(0032,1032)	O	2
Referring Physician's Name	(0008,0090)	O	2
<b>Visit Identification</b>			
Admission ID	(0038,0010)	O	2
Current Patient Location	(0038,0300)	O	2
<b>Patient Identification</b>			
Patient's Name	(0010,0010)	R	1
Patient ID	(0010,0020)	R	1
<b>Patient Demographics</b>			
Patients Birth Date	(0010,0030)	O	2
Patient's Sex	(0010,0040)	O	2

Description	Tag	Matching Key Type	Return Key Type
Patient's Weight	(0010,1030)	O	2
Confidentiality constraint on patient data	(0040,3001)	O	2
<b>Patient Medical</b>			
Patient State	(0038,0500)	O	2
Pregnancy Status	(0010,21C0)	O	2
Medical Alerts	(0010,2000)	O	2
Contrast Allergies	(0010,2110)	O	2
Special Needs	(0038,0050)	O	2
All other Attributes from the Patient Medical Module		O	3

## 5.6 MPPS Server AE Specification

### 5.6.1 SOP Classes

MPPS Server AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	No	Yes
<b>Workflow Management</b>			
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	No	Yes

### 5.6.2 Association Policies

#### 5.6.2.1 General

DICOM application context for MPPS Server AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes).

#### 5.6.2.2 Number of Associations

Number of Associations as an Association Initiator:

Maximum number of simultaneous associations	1
---	---

Number of Associations as an Association Acceptor:

Maximum number of simultaneous associations	1
---	---

### 5.6.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

### 5.6.2.4 Implementation Identifying Information

DICOM Implementation Class and Version for MPPS Server AE:

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

## 5.6.3 Association Initiation Policy

### 5.6.3.1 Real-World Activity – Forwarding Modality Performed Procedure Step (MPPS)

#### Associated Real World Activity – Forwarding MPPS request

The associated real world activity is that a remote system is sending an MPPS request to the MPPS server AE, and that the MPPS service is configured to forward MPPS messages to another MPPS SCP.

#### Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 31 are acceptable by MPPS server AE for receiving MPPS.

**Table 31- Accepted Presentation Contexts**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

#### 5.6.4 Association Acceptance Policy

MPPS Server AE accepts an association for verification and receiving modality performed procedure step.

##### 5.6.4.1 Real World Activity – Verification

MPPS Server AE accepts associations from nodes that wish to perform a verification operation on MPPS Server AE.

#### Associated Real World Activity – Verification

The Real World Activity associated with the C-ECHO request is that an external node wishes to verify network or server operation without initiating any actual work.

#### Presentation Context Table

Table 32 shows the Presentation Contexts that may be accepted by MPPS Server AE for verification operations.

**Table 32 - Acceptable Presentation Contexts by MPPS Server AE for Verification**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

#### SOP Specific Conformance for SOP Class Verification

Not Applicable.

#### Presentation Context Acceptance Criterion

MPPS Server AE will accept the verification SOP classes listed in Table 32 above. Modality Worklist Server AE defines no limit on the number of presentation contexts accepted. If MPPS Server AE runs out of resources in the process of trying to accept multiple presentation contexts, Modality Worklist Server AE will reject the association request.

#### Transfer Syntax Selection Policies

MPPS Server AE prefers Explicit Little Endian Transfer Syntax.

If offered a choice of Transfer Syntaxes in a Presentation Context, it will apply the following priority to the choice of Transfer Syntax:

1. Explicit Little Endian Transfer Syntax

2. Implicit Little Endian Transfer Syntax
3. Explicit Big Endian Transfer Syntax

#### 5.6.4.2 Real-World Activity – Receiving Modality Performed Procedure Step (MPPS)

##### Associated Real World Activity – Receiving MPPS request

The associated real world activity is that a remote system is sending an MPPS request to the MPPS server AE.

MPPS server AE application will wait for an association as an SCP for the MPPS Service Class. When N-CREATE/N-SET events are received, a search for the data with the received attributes is performed on the Change Healthcare Cardiology database and the required data are stored on the Change Healthcare Cardiology database.

The Change Healthcare Cardiology MPPS SCP can also serve as MPPS SCU in order to transfer an entire data set, as is, to another MPPS SCP, if configured to do so.

##### Accepted Presentation Contexts

Any of the Presentation Contexts shown in Table 33 are acceptable by MPPS server AE for receiving an MPPS request.

**Table 33- Accepted Presentation Contexts**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP

**5.6.4.3 SOP Specific Conformance for MPPS SOP Class**

The supported Return Key Attributes are as follows:

Description	Tag	Return Key Type N-CREATE	Return Key Type N-Set	Requirement Type Final State
<b>SOP Common</b>				
Specific Character Set	(0008,0005)	1C (Required if an extended or replacement character set is used)	Not allowed	
<b>Performed Procedure Step Information</b>				
Performed Station AE Title	(0040,0241)	1	Not allowed	
Performed Station Name	(0040,0242)	2	Not allowed	
Performed Location	(0040,0243)	2	Not allowed	
Performed Procedure Step ID	(0040,0253)	1	Not allowed	
Performed Procedure Step Start Date	(0040,0244)	1	Not allowed	
Performed Procedure Step Start Time	(0040,0245)	1	Not allowed	
Performed Procedure Step Status	(0040,0252)	1	1	
Performed Procedure Step End Date	(0040,0250)	1	1	1
Performed Procedure Step End Time	(0040,0251)	1	1	1
Performed Procedure Step Description	(0040,0254)	2	2	
Performed Procedure Type Description	(0040,0255)	2	2	
Procedure Code	(0008,1032)	2	2	

Description	Tag	Return Key Type N-CREATE	Return Key Type N-Set	Requirement Type Final State
Sequence				
>Code Value	(0008,0100)	1C (Required if Sequence Item is present)	1C (Required if Sequence Item is present)	
>Coding Scheme Designator	(0008,0102)	1C (Required if Sequence Item is present)	1C (Required if Sequence Item is present)	
>Coding Scheme Version	(0008,0103)	3	3	
>Code Meaning	(0008,0104)	3	3	
Comments on the Performed Procedure Step	(0040,0280)	1	3	
<b>Performed Procedure Step Relationship</b>				
Scheduled Step Attribute Sequence	(0040,0270)	1	Not allowed	
>Study Instance UID	(0020,000D)	1	Not allowed	
>Referenced Study Sequence	(0008,1110)	2	Not allowed	
>>Referenced SOP Class UID	(0008,1150)	1C (Required if Sequence Item is present)	Not allowed	
>>Referenced SOP Instance UID	(0008,1155)	1C (Required if Sequence Item is present)	Not allowed	
>Accession Number	(0008,0050)	2	Not allowed	
>Place Order Number/Imaging Service Request	(0040,2016)	3	Not allowed	
>Filler Order Number/Imaging Service Request	(0040,2017)	3	Not allowed	
>Requested Procedure ID	(0040,1001)	2	Not allowed	
>Requested Procedure Step	(0032,1060)	2	Not allowed	



<b>Description</b>	<b>Tag</b>	<b>Return Key Type N-CREATE</b>	<b>Return Key Type N-Set</b>	<b>Requirement Type Final State</b>
Description				
>Scheduled Procedure Step ID	(0040,0009)	2	Not allowed	
>Scheduled Procedure Step Description	(0040,0007)	2	Not allowed	
>Scheduled Protocol Code Sequence	(0040,0008)	2	Not allowed	
>>Code Value	(0008,0100)	1C (Required if Sequence Item is present)	Not allowed	
>>Coding Scheme designator	(0008,0102)	1C (Required if Sequence Item is present)	Not allowed	
>>Coding Scheme Version	(0008,0103)	3	Not allowed	
>>Code Meaning	(0008,0104)	3	Not allowed	
Patient's Name	(0010,0010)	2	Not allowed	
Patient's ID	(0010,0020)	2	Not allowed	
Patient's Birth Date	(0010,0030)	2	Not allowed	
Patient's Sex	(0010,0040)	2	Not allowed	
Referenced Patient Sequence	(0008,1120)	2	Not allowed	
>Referenced SOP Class UID	(0008,1150)	1C (Required if Sequence Item is present)	Not allowed	
>Referenced SOP Instance UID	(0008,1155)	1C (Required if Sequence Item is present)	Not allowed	
Performed Procedure Discontinuation Reason Code Sequence	(0040,0281)	3	3	
>Code Value	(0008,0100)	1	1	
>Coding	(0008,0102)	1	1	

Description	Tag	Return Key Type N-CREATE	Return Key Type N-Set	Requirement Type Final State
SchemeDesignator				
>Coding SchemeVersion	(0008,0103)	3	3	
>Code Meaning	(0008,0104)	3	3	
<b>Image Acquisition Results</b>				
Modality	(0008,0060)	1	Not allowed	
Study ID	(0020,0010)	2	Not allowed	
Performed Protocol Code Sequence	(0040,0260)	2	2	
>Code Value	(0008,0100)	1	1	
>Coding Scheme Designator	(0008,0102)	1	1	
>Coding Scheme Version	(0008,0103)	3	3	
>Code Meaning	(0008,0104)	3	3	
Performed Series Sequence	(0040,0340)	2	1	1
>Performed Physician's Name	(0008,1050)	2	2	2
>Protocol Name	(0018,1030)	1	1	1
>Operator's Name	(0008,1070)	2	2	2
>Series Instance UID	(0020,000E)	1	1	1
>Series Description	(0008,103E)	2	2	2
>Retrieve AE Title	(0008,0054)	2	2	2
>Referenced Image Sequence	(0008,1140)	2	2	
>>Referenced SOP Class UID	(0008,1150)	1	1	
>>Referenced SOP InstanceUID	(0008,1155)	1	1	
>Referenced Non-Image Composite SOP Image Sequence	(0040,0220)	2	2	

Description	Tag	Return Key Type N-CREATE	Return Key Type N-Set	Requirement Type Final State
>>Referenced SOP Class UID	(0008,1150)	1	1	
>>Referenced SOP InstanceUID	(0008,1155)	1	1	
>All other attributes from wPerformed Series Sequence		3	3	
All other attributes from Radiation Dose Module and Billing and Material Code Module		3	3	

Possible response status values are:

Status Code	Action	Status
A7xx	Refused	Out of resources
A9xx	Failed	Identifier does not match SOP Class
Cxxx		Unable to Process
0110		Unable to generate data
0000	Success	Sub-operations completed

## 5.7 Sync Storer AE Specification

### 5.7.1 SOP Classes

Sync Storer AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	No
<b>Transfer</b>			
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	No
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	No

SOP Class Name	SOP Class UID	SCU	SCP
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	No
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	No
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	No
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	No
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	No
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Yes	No
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	No
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Yes	No
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	No
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Yes	No
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	No
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	No
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	No
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3	Yes	No
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	No
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5	Yes	No
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Yes	No
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	No
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Yes	No

SOP Class Name	SOP Class UID	SCU	SCP
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	No
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	No
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	No
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	No
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	No
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	No
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	No
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	No
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	No
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	No
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	No
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	No
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	No
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	No
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	No
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	No
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1	Yes	No
Intravascular Optical Coherence Tomography Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.14.1	Yes	No
Intravascular Optical Coherence Tomography Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.14.2	Yes	No
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59	Yes	No

SOP Class Name	SOP Class UID	SCU	SCP
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Yes	No
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Yes	No
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Yes	No
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	No

## 5.7.2 Association Policies

### 5.7.2.1 General

DICOM application context for Sync Storer AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes)

### 5.7.2.2 Number of Associations

Number of Association as Association Initiator:

Maximum number of simultaneous associations	10 by default. Configurable from 1 to 10.
---	---

### 5.7.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

### 5.7.2.4 Implementation Identifying Information

#### DICOM Implementation Class and Version for Sync Storer AE

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

## 5.7.3 Association Initiation Policy

Sync Storer AE attempts to initiate a new association in the following cases:

- To check the connection to the remote system
- To synchronize DICOM archive upon instance deletion and provide corrected instances as part of the IOCM profile.

### 5.7.3.1 Real-World Activity – Verification

#### Associated Real-World Activity

The associated Real-World Activity is an attempt to check whether remote AE is ready for DICOM dialog.

### Proposed Presentation Contexts

For this Real-World Activity, the client AE will propose one of the Presentation Contexts listed in Table 34.

**Table 34 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

### 5.7.3.2 Real-World Activity – Synchronize DICOM Archive (IOCM activity)

#### Description and Sequencing of Activities

Sync Storer AE can export DICOM Key Object Selection (KOS) objects as a rejection note to a DICOM Archive as a result of an internal “Delete Image” event.

- **Delete Images:**  
Deleting images (or instances) triggers the creation of an outbound delete Instances KOS.
- **Merge or Move Study:**  
When moving or merging a study, Change Healthcare Cardiology will send a DICOM KOS to notify the DICOM archive on instance deletion from the source study and will send the relevant corrected instances associated to the destination study.

### Proposed Presentation Contexts

Each time an association is initiated, the Sync Storer AE proposes one or more Presentation Contexts to be used on that association, as shown in Table 35.

**Table 35 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Note		Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
See Note		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
See Note		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
See Note		JPEG Lossless, Hierarchical, First-Order Prediction	1.2.840.10008.1.2.4.70	SCU	None

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
See Note		JPEG Lossy Process 1	1.2.840.10008.1.2.4.50	SCU	None
See Note		RLE Lossless	1.2.840.10008.1.2.5	SCU	None

---

**Note:** The Abstract Syntax corresponds to the SOP Class UID for Series modality. The selection of these syntaxes can be found in [Table 36](#)

---



**Table 36 - Abstract Syntaxes**

<b>Abstract Syntax</b>	
<b>Name</b>	<b>UID</b>
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Single bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
X-Ray Bi-Plane Angiographic Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.12.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
Nuclear Medicine Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.5
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Radiotherapy Image	1.2.840.10008.5.1.4.1.1.481.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital Mammography Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2

Abstract Syntax	
Name	UID
Digital Mammography Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Visible Light Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1
Visible Light Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2
Visible Light Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3
Visible Light Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Waveform Storage – Trial (Retired)	1.2.840.10008.5.1.4.1.1.9.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59
Basic Text Structure Report	1.2.840.10008.5.1.4.1.1.88.11
Enhanced Structure Report	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive Structure Report	1.2.840.10008.5.1.4.1.1.88.33
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

#### SOP Specific Conformance – Storage SOP Classes

See more information about rejection note contents in [9.1.1 - Rejection Note Key Object Selection \(KOS\) Object Contents](#).

#### 5.7.4 Association Acceptance Policy

Sync Storer AE does not accept associations.

## 5.8 Sync Committer AE Specification

### 5.8.1 SOP Classes

Sync Committer AE provides Standard Conformance to the following DICOM 3.0 SOP Classes:

SOP Class Name	SOP Class UID	SCU	SCP
<b>Verification</b>			
Verification	1.2.840.10008.1.1	Yes	No
<b>Workflow Management</b>			
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No

### 5.8.2 Association Policies

#### 5.8.2.1 General

DICOM application context for Sync Committer AE:

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

Maximum PDU size is configurable (default is 16,384 bytes).

#### 5.8.2.2 Number of Associations

Number of Association as Association Initiator:

Maximum number of simultaneous associations	1
---	---

Number of Associations as an Association Acceptor:

Maximum number of simultaneous associations	Unlimited
---	-----------

#### 5.8.2.3 Asynchronous Nature

Asynchronous mode (multiple concurrent operations on one association) is not supported.

#### 5.8.2.4 Implementation Identifying Information

DICOM Implementation Class and Version for Sync Committer AE:

Implementation Class UID	2.16.376.1.1.511752891.1
Implementation Version Name	MEDCON01MAR2012

### 5.8.3 Association Initiation Policy

#### 5.8.3.1 Real-World Activity – Verification

##### Associated Real-World Activity

The associated Real-World Activity is an attempt to check whether remote AE is ready for DICOM dialog.

##### Proposed Presentation Contexts

For this Real-World Activity, the Sync Committer AE will propose one of the Presentation Contexts listed in Table 37.

**Table 37 - Proposed Presentation Contexts**

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	DICOM Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
Verification	1.2.840.10008.1.1	DICOM Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

### 5.8.3.2 Real-World Activity – Getting Storage Commitment from a Remote System

#### Associated Real-World Activity

Sync Committer AE requests Storage Commitment from the remote DICOM Archive solution after sending instances or DICOM KOS object to the remote DICOM Archive and receiving a response confirming the instances were archived.

The storage commitment response may be received on the same association or on a separate association.

#### Proposed Presentation Contexts

For this Real-World Activity, the Sync Committer AE will propose one of the Presentation Contexts listed in Table 38.

**Table 38 -Proposed Presentation Contexts**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

## 5.8.4 Association Acceptance Policy

### 5.8.4.1 Real-World Activity – Receive Storage Commitment Response

#### Associated Real-World Activity

The associated Real-World Activity is receiving a storage commitment response on a separate association than the storage commitment request.

#### Accepted Presentation Contexts

Table 39 shows the Presentation Contexts that may be accepted by Sync Committer AE for receiving Storage Commitment Response.

**Table 39 - Acceptable Presentation Contexts by Storage Manager Committer AE for receiving Storage Commitment Response**

Presentation Context Table				
Abstract Syntax		Transfer Syntax		Role
Name	UID	Name	UID	
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU
Storage Commitment Push Model	1.2.840.10008.1.20.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU

## **6. Communication Profiles**

### **6.1 TCP/IP Stack**

Change Healthcare Cardiology provides DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

#### **6.1.1 TCP/IP API**

Change Healthcare Cardiology AEs inherits their TCP/IP stack from the computer system upon which it executes.

## 7. Extensions/Specializations/Privatization

Change Healthcare Cardiology supports all the private tags on Level 2. Change Healthcare Cardiology private tags are listed in Table 40.

**Table 40- Change Healthcare Private Attributes**

<b>Data Element Tag</b>	<b>Name</b>	<b>Value Representation</b>	<b>Remark</b>
(000D,0010)	Private Attributes Identification Code	LO	MEDCON
(000D,1000)	Patient TCS Location ID	SH	
(000D,1001)	Study TCS Location ID	SH	
(000D,1002)	Instance TCS Location ID	SH	
(000D,1003)	Instance TCS ID	SH	
(000D,1004)	Instance TCS Location ID	SH	
(000D,1005)	Patient TCS ID	SH	
(000D,1006)	Related File	LO	
(000D,1007)	Additional Patient ID	LO	
(000D,1021)	Patient Creation Date	DA	
(000D,1022)	Patient Creation Time	TM	
(000D,1038)	Instance Description	LO	
(000D,1062)	TCS Document File	LO	
(000D,1063)	Annotation Note	SH	When exists in Changing Information Sequence (000D,1302) item, contains date and time of update
(000D,1076)	Annotation Creation Date	DA	
(000D,1077)	Annotation Creation Time	TM	
(000D,1082)	Instance Creation Date	DA	
(000D,1083)	Instance Creation Time	TM	
(000D,1090)	TCS Document Type	US	Internal enumerator for document type



(000D,1095)	Referenced Instance Sequence	SQ	1 item
(000D,1096)	Procedure Type Code	LO	
(000D,1097)	Patient Optional ID	LO	
(000D,1098)	Patient NHS number	LO	
(000D,1099)	Patient NHS status	LO	
(000D,0011)	Private Attributes Identification Code	LO	MEDCON
(000D,1101)	Patient Name	OW	
(000D,1102)	Patient ID	OW	
(000D,1103)	Patient Additional ID	OW	
(000D,1104)	Patient Optional ID	OW	
(000D,1105)	Series Description	OW	
(000D,1106)	Series Optional ID	OW	
(000D,1107)	Referring Physicians Name	OW	
(000D,1108)	Performing Physicians Name	OW	Names are Delimited by “\”
(000D,1109)	Instance Name	OW	
(000D,1110)	Instance Description	LO	
(000D,0012)	Private Attributes Identification Code	LO	MEDCON WRAPPED REPORT or MEDCON WRAPPED ANNOTATION
(000D,1202)	MMI Type	SH	Encapsulated document extension
(000D,1203)	Encapsulated Document Sequence	SQ	1 or more items
(000D,1204)	Encapsulated Document	OB	
(000D, 1205)	Encapsulated Document Length	UL	
(000D,0013)	Private Attributes Identification Code	LO	MEDCON

(000D,1301)	Hostname	LO	Internal use in Modality Worklist
(000D,1302)	Changing Information Sequence	SQ	1 or more items containing elements before update
(000D,1303)	Calling AE Title	LO	Internal use in Modality Worklist

Elements from (000D,1101) – (000D,1110) are used for recording the UNICODE version of the relevant standard and private elements (if required).

Elements from (000D,1202) – (000D, 1205) are used to encapsulate non-DICOM files.

Element (000D, 1302) is used to save sequences of elements that were changed when a DICOM file is updated. All elements represent internal information used for media exchanges between Change Healthcare Cardiology Systems.

## 8. Configuration

Change Healthcare Cardiology maintains configuration data in registry and configuration files as well as in the database. All parameters of DICOM services (including AE Title and TCP Listen Port) are configurable. Configuration may be performed by the Change Healthcare Cardiology Administration utility or manually.

The Change Healthcare Cardiology AEs uses registry and configuration files that contain information used to validate association attempts from Local and Remote Application entities. The Change Healthcare Cardiology AEs then listens for association requests on the configured port.

An association request for Storage Services from a Remote Application Entity causes the Change Healthcare Cardiology Gateway AE to validate the request according to the configuration parameters set at execution time. The Remote Application Entity then sends the Information Object Instance.

If the data is not currently stored, the Change Healthcare Cardiology Gateway AE saves the received Information Object Instance on its database and in a predefined backup directory on the hard disk. The data remains in that directory until it is removed by the Change Healthcare Cardiology Quota Manager service based on the quota configuration.

The Change Healthcare Cardiology Query/Retrieve Server AE searches the local database for the instance(s) specified. If the request was C-FIND, then a response is returned for each match. If the request was C-MOVE, then a sub association is created for the C-STORE operation with the destination Application Entity specified in the C-MOVE message.

## 9. Annexes

### 9.1 IOD Contents

#### 9.1.1 Rejection Note Key Object Selection (KOS) Object Contents

When the DICOM storage Synchronization Service is set as active, instance deletion involves a creation of a rejection note KOS object according to the IOCM profile.

Table 41 below contains a list of DICOM elements of KOS file intended for flagging one or more images, waveforms, or other composite SOP Instances that were deleted by applications. The reason for deleting Merge and Delete operations performed by a client is defined as “Incorrect Modality Worklist Entry”.

*The following abbreviations are used in table 39:*

AUTO – Value is generated automatically

USER – Value is sourced from user input

EMPTY – Attribute is sent without a value

VNAP – Value not always present

**Table 41 – Rejection note elements**

(Group, Element)	VR	Meaning	Value	Comments
(0008,0012)	DA	Instance Creation Date	AUTO	
(0008,0013)	TM	Instance Creation Time	AUTO	
(0008,0016)	UI	SOP Class UID	1.2.840.10008.5.1.4.1.1.88.59	Key Object Selection Document
(0008,0018)	UI	SOP Instance UID	AUTO	
(0008,0021)	DA	Series Date	AUTO	
(0008,0023)	DA	Content Date	AUTO	
(0008,0031)	TM	Series Time	AUTO	
(0008,0033)	TM	Content Time	AUTO	
(0008,0050)	SH	Accession Number	USER; VNAP	
(0008,0060)	CS	Modality	KO	

(Group, Element)	VR	Meaning	Value	Comments
(0008,0070)	LO	Manufacturer	EMPTY	
(0010,0010)	PN	Patient's Name	USER	
(0010,0020)	LO	Patient ID	USER	
(0010,0021)	LO	Issuer of Patient ID	USER	
(0010,0030)	DA	Patient's Birth Date	USER	
(0010,0040)	CS	Patient's Sex	enumeration: M,F,O; USER	
(0020,000D)	UI	Study Instance UID	USER	
(0020,000E)	UI	Series Instance UID	USER	
(0020,0011)	IS	Series Number	1	
(0020,0013)	IS	Instance Number	1	
(0040,A040)	CS	Value Type	CONTAINER	
(0040,A043)	SQ	Concept Name Code Sequence		Sequence with 1 item
>(0008,0100)	SH	Code Value	113038	
>(0008,0102)	SH	Coding Scheme Designator	DCM	
>(0008,0104)	LO	Code Meaning	Incorrect Modality Worklist Entry	
(0040,A050)	CS	Continuity Of Content	SEPARATE	
(0040,A375)	SQ	Current Requested Procedure Evidence Sequence		
>(0008,1115)	SQ	Referenced Series Sequence	USER	Sequence with 1 or more items
>>(0008,1199)	SQ	Referenced SOP Sequence	USER	Sequence with 1 or more items
>>>(0008,1150)	UI	Referenced SOP Class UID	USER	
>>>(0008,1155)	UI	Referenced SOP Instance UID	USER	

(Group, Element)	VR	Meaning	Value	Comments
>>(0020,000E)	UI	Series Instance UID	USER	
>(0020,000D)	UI	Study Instance UID	USER	
(0040,A504)	SQ	Content Template Sequence	USER	Sequence with 1 item
>(0008,0105)	CS	Mapping Resource	DCMR	
>(0040,DB00)	CS	Template Identifier	2010	
(0040,A730)	SQ	Content Sequence	USER	Sequence with 1 item
>(0008,1199)	SQ	Referenced SOP Sequence	USER	Sequence with 1 or more items
>>(0008,1150)	UI	Referenced SOP Class UID	USER	
>>(0008,1155)	UI	Referenced SOP Instance UID	USER	
>(0040,A010)	CS	Relationship Type	CONTAINS	
>(0040,A040)	CS	Value Type	enumeration: IMAGE, WAVEFORM, COMPOSITE;	COMPOSITE type used for Structure Report, Encapsulated Document (PDF), Encapsulated non-DICOM documents , any other supported documents differ from IMAGE and WAVEFORM.

## **10. Contact and Support Information**

### **10.1 Support information**

For technical support or any service related to your product, call the toll-free number for your region listed at <https://iwcrm.changehealthcare.com>. Standard coverage may include software support, hardware support, and software updates as covered in the support maintenance agreement.